

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011722\
 Data File : VW024375.D
 Acq On : 17 Jan 2022 14:10
 Operator : SY/MD
 Sample : N1168-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLX7

Quant Time: Jan 17 14:54:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 13 02:28:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	303864	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	280790	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	138219	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	99919	45.690	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.380%
7) Chloroethane-d5	1.568	69	75642	45.533	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.060%
11) 1,1-Dichloroethene-d2	2.108	63	143388	35.082	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.160%
21) 2-Butanone-d5	3.879	46	117336	96.303	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.300%
24) Chloroform-d	4.342	84	196164	49.080	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.160%
26) 1,2-Dichloroethane-d4	5.024	65	125536	46.912	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.820%
32) Benzene-d6	5.043	84	390108	53.240	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.480%
36) 1,2-Dichloropropane-d6	6.063	67	116070	56.522	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	113.040%
41) Toluene-d8	7.310	98	367879	51.854	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.700%
43) trans-1,3-Dichloroprop...	7.616	79	58362	49.355	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.720%
47) 2-Hexanone-d5	8.085	63	82698	92.692	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.690%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	141909	48.356	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.720%
66) 1,2-Dichlorobenzene-d4	11.622	152	150606	54.665	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.340%
Target Compounds						
					Qvalue	
13) Acetone	2.178	43	8375	6.962	ug/L	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011722\
Data File : VV024375.D
Acq On : 17 Jan 2022 14:10
Operator : SY/MD
Sample : N1168-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLX7

Quant Time: Jan 17 14:54:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 13 02:28:22 2022
Response via : Initial Calibration

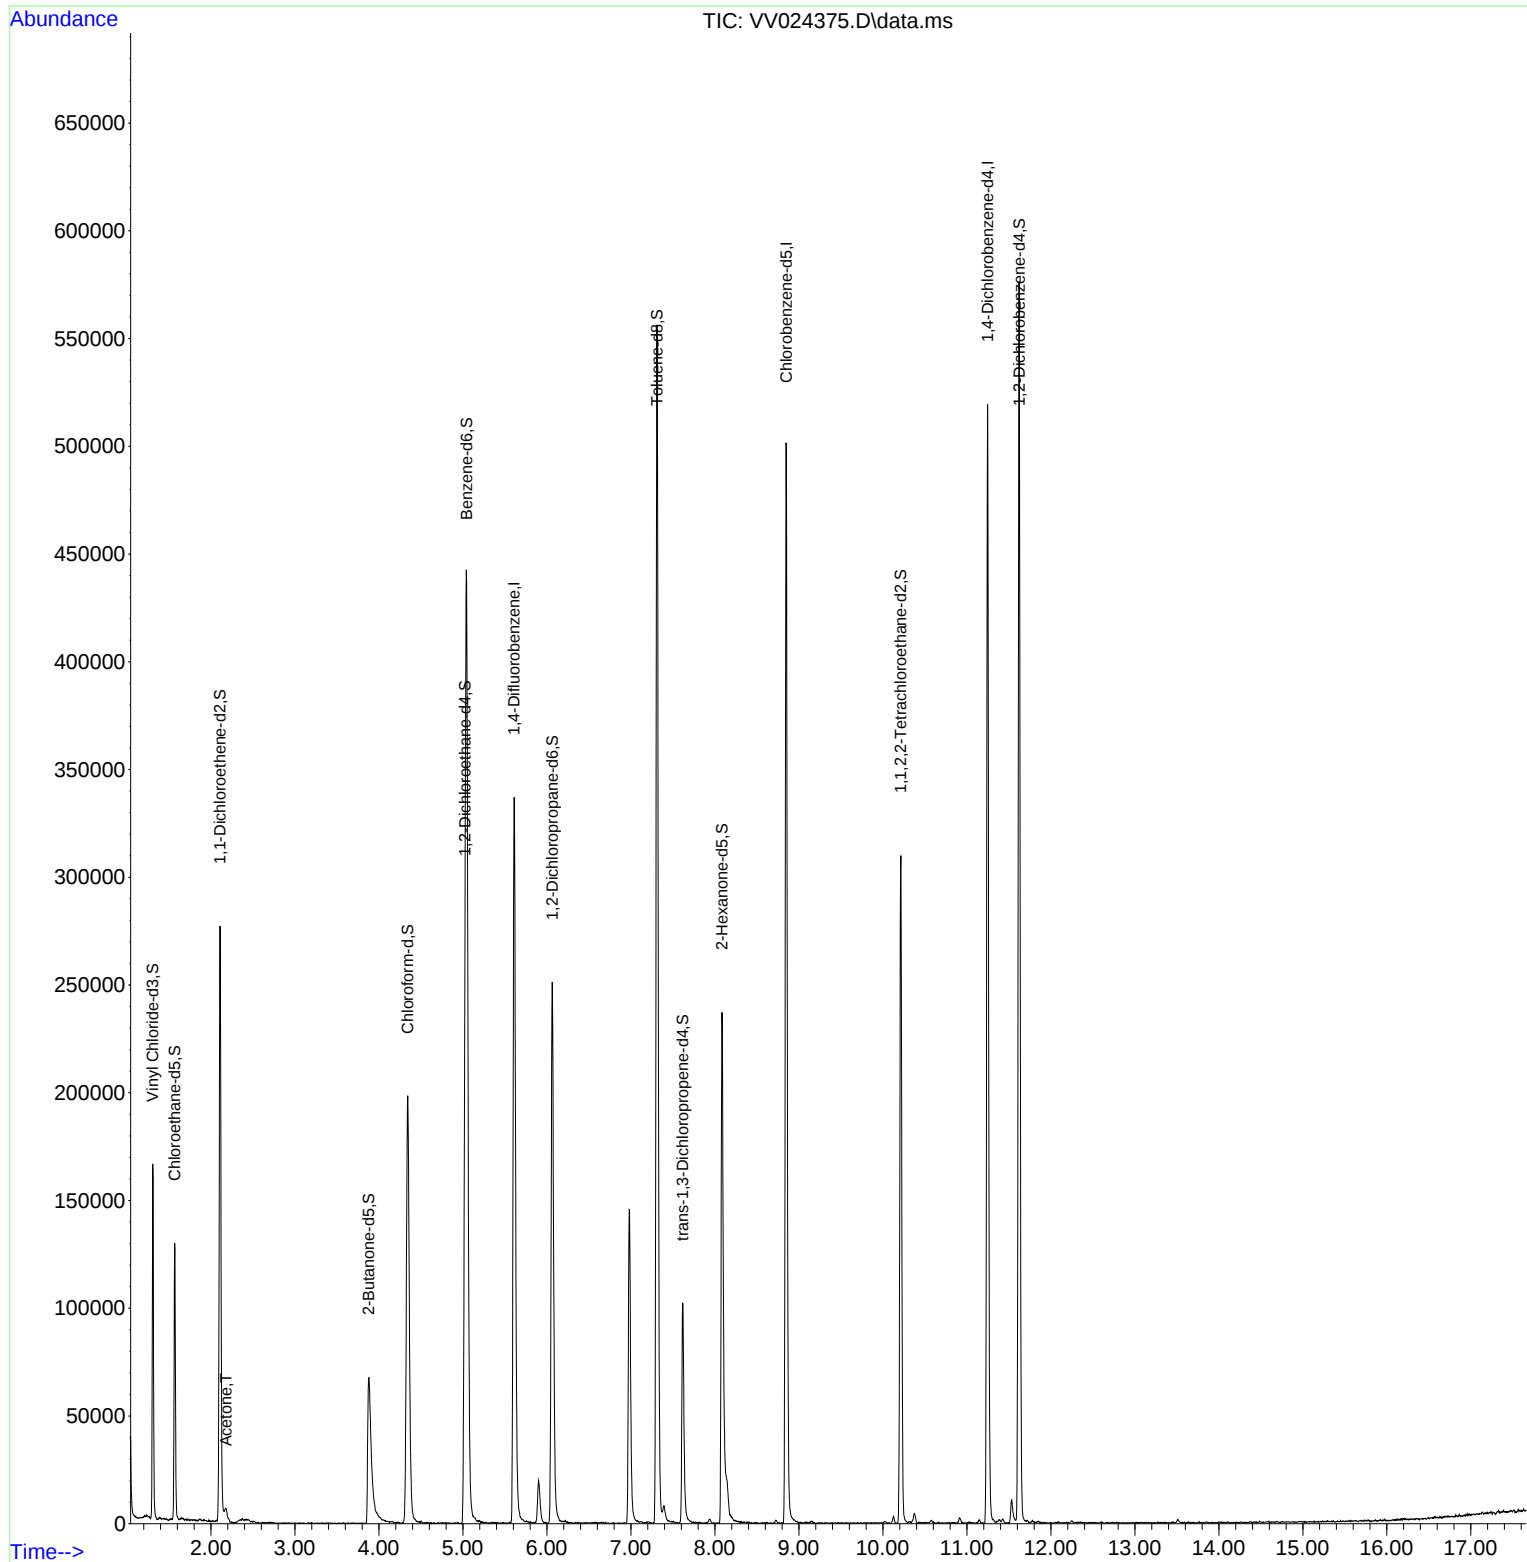

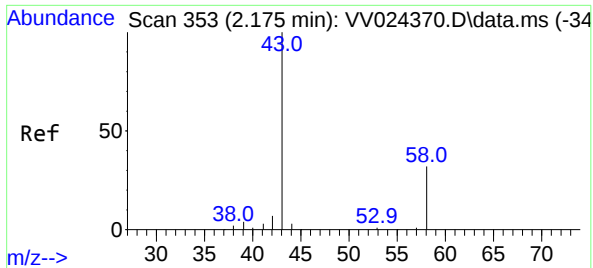

#13
 Acetone
 Concen: 6.962 ug/L
 RT: 2.178 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VV024375.D
 Acq: 17 Jan 2022 14:10

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLX7

Tgt Ion: 43 Resp: 8375
 Ion Ratio Lower Upper
 43 100
 58 12.9 0.0 63.0

