

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011722\
 Data File : VW024379.D
 Acq On : 17 Jan 2022 16:44
 Operator : SY/MD
 Sample : N1115-11ME
 Misc : 7.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLS1ME

Quant Time: Jan 18 05:57:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 13 02:28:22 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	401445	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	379118	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	205936	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	149330	51.686	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	103.380%	
7) Chloroethane-d5	1.568	69	110128	50.178	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	100.360%	
11) 1,1-Dichloroethene-d2	2.095	63	225774	41.812	ug/L	-0.02
Spiked Amount	50.000	Range 60 - 125	Recovery	=	83.620%	
21) 2-Butanone-d5	3.886	46	206487	128.279	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	128.280%	
24) Chloroform-d	4.339	84	336881	63.799	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	127.600%#	
26) 1,2-Dichloroethane-d4	5.024	65	227050	64.223	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	128.440%#	
32) Benzene-d6	5.040	84	676753	68.405	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	136.820%#	
36) 1,2-Dichloropropane-d6	6.063	67	203814	73.509	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	147.020%#	
41) Toluene-d8	7.310	98	666901	69.622	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	139.240%#	
43) trans-1,3-Dichloroprop...	7.616	79	111335	69.734	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	139.460%#	
47) 2-Hexanone-d5	8.114	63	166684	138.372	ug/L	0.03
Spiked Amount	100.000	Range 45 - 130	Recovery	=	138.370%#	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	266563	67.274	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	134.540%#	
66) 1,2-Dichlorobenzene-d4	11.625	152	287669	70.081	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	140.160%#	
Target Compounds						
13) Acetone	2.185	43	3897	2.452	ug/L	81
46) Tetrachloroethene	7.972	164	20213	8.354	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011722\
 Data File : VV024379.D
 Acq On : 17 Jan 2022 16:44
 Operator : SY/MD
 Sample : N1115-11ME
 Misc : 7.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLS1ME

Quant Time: Jan 18 05:57:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 13 02:28:22 2022
 Response via : Initial Calibration




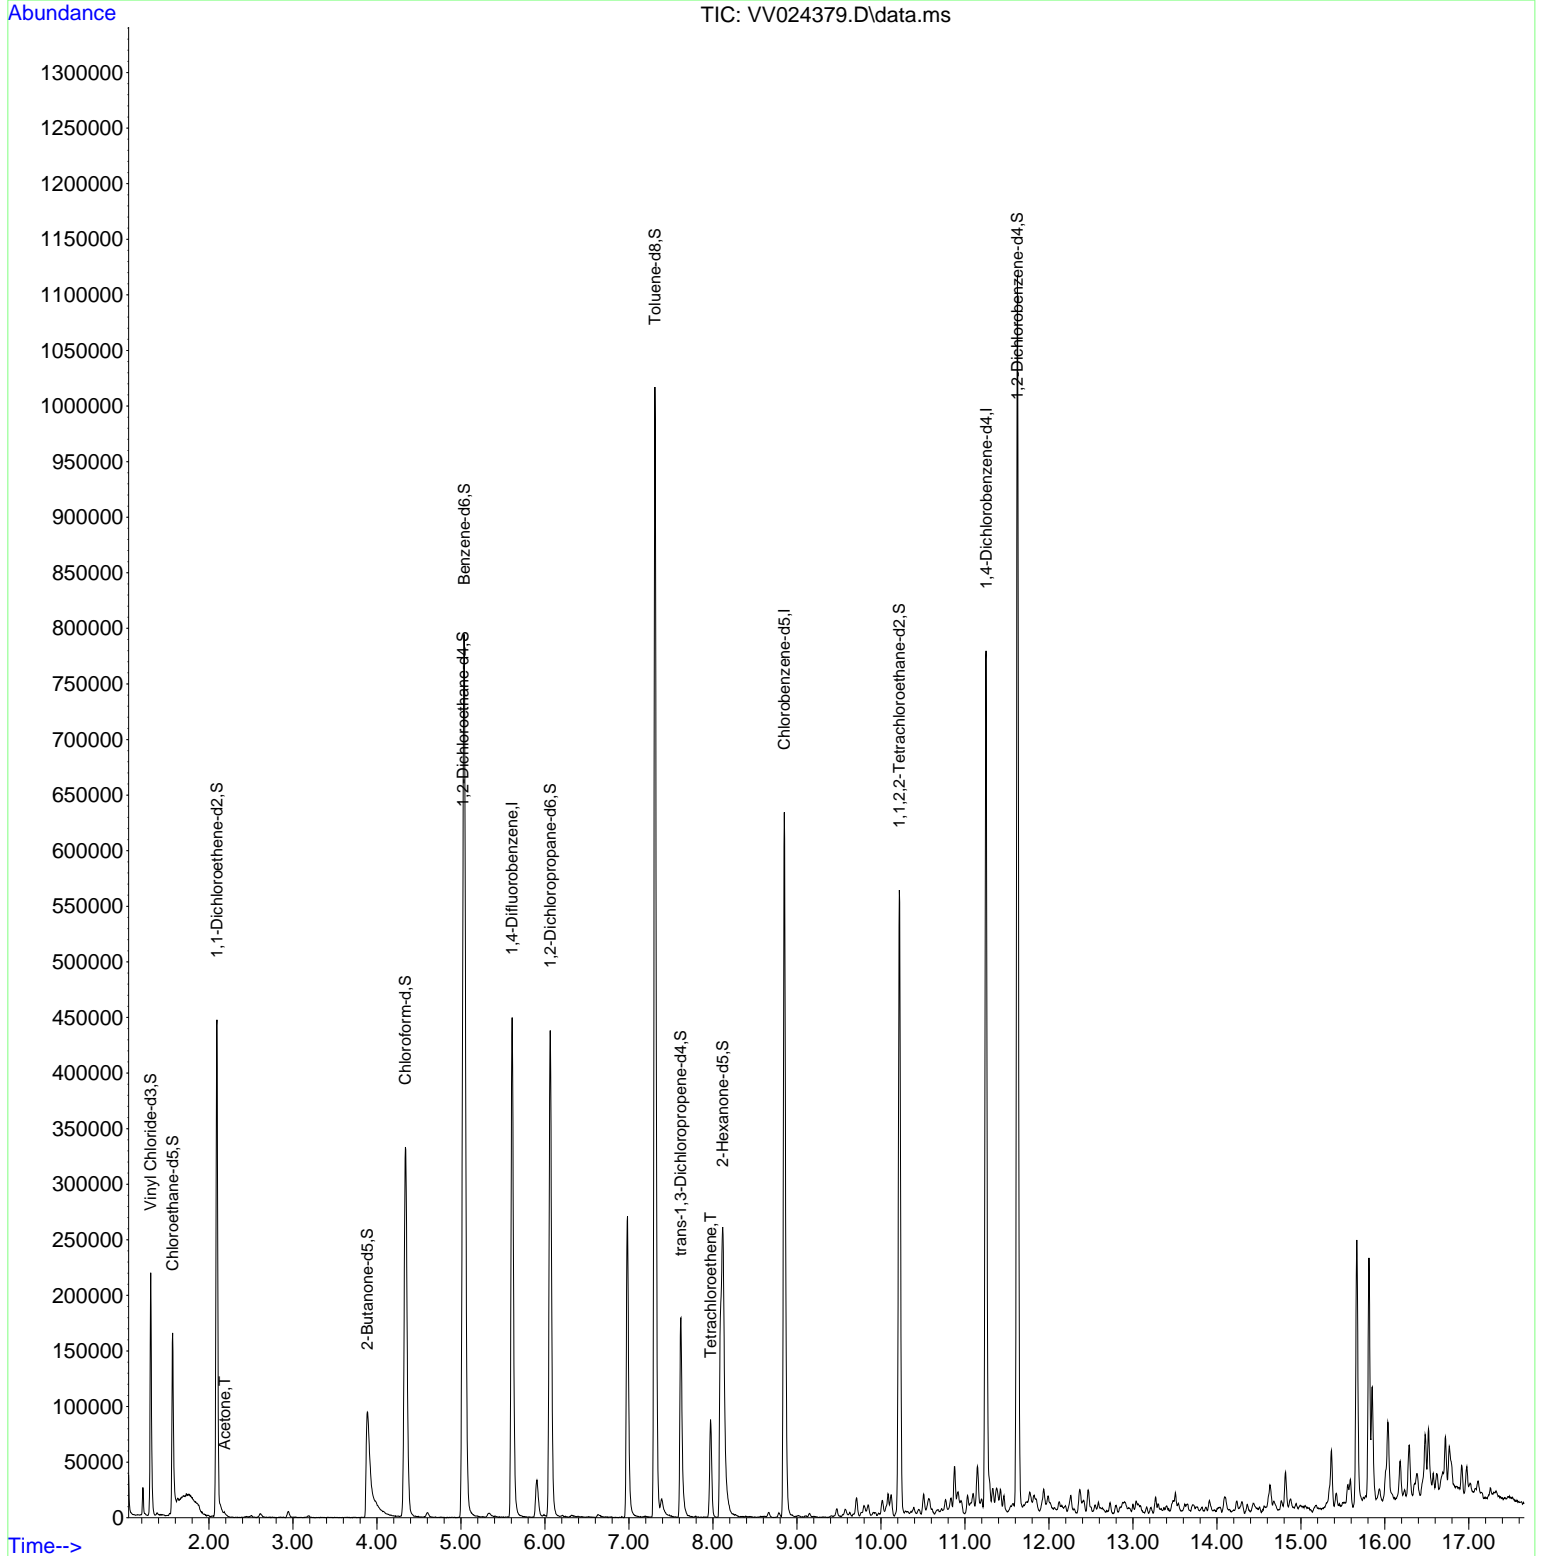


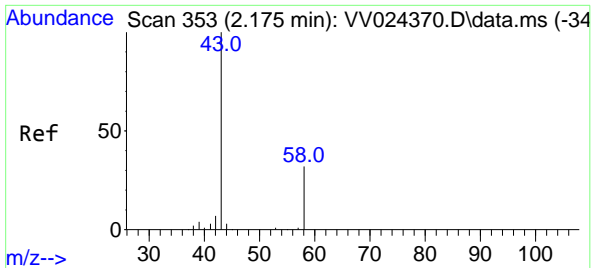

#13
 Acetone
 Concen: 2.452 ug/L
 RT: 2.185 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV024379.D
 Acq: 17 Jan 2022 16:44

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLS1ME

Tgt Ion: 43 Resp: 3897
 Ion Ratio Lower Upper
 43 100
 58 20.8 0.0 63.0

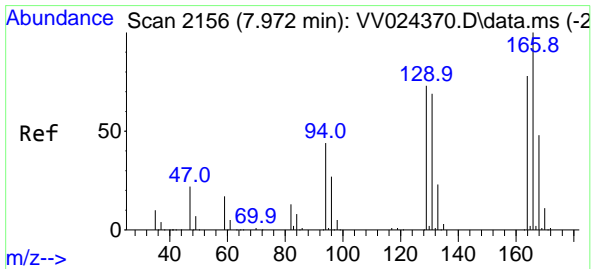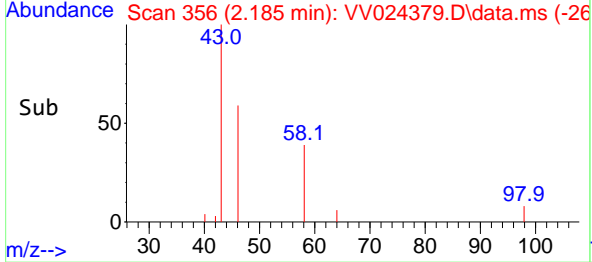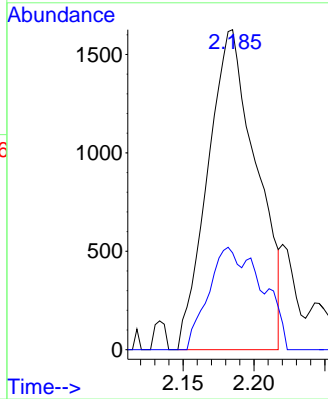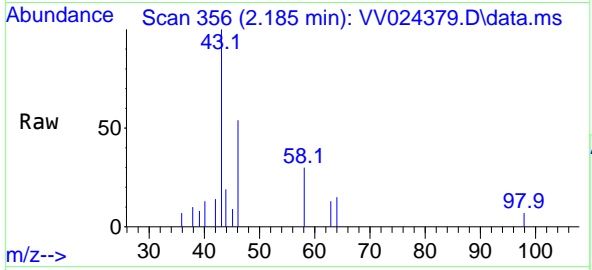

#46
 Tetrachloroethene
 Concen: 8.354 ug/L
 RT: 7.972 min Scan# 2156
 Delta R.T. -0.000 min
 Lab File: VV024379.D
 Acq: 17 Jan 2022 16:44

Tgt Ion:164 Resp: 20213
 Ion Ratio Lower Upper
 164 100
 129 86.5 61.5 114.1
 131 90.4 62.2 115.4
 166 129.0 89.9 166.9

