

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011722\
 Data File : VV024374.D
 Acq On : 17 Jan 2022 13:11
 Operator : SY/MD
 Sample : N1168-12RE
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLX7RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

Signal : TIC: VV024373.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	102	rVB	151333	151417	14.30%	1.715%
2	1.568	157	164	178	rBV	116668	128456	12.13%	1.455%
3	2.108	321	332	347	rBV	257215	374695	35.39%	4.244%
4	2.252	374	377	378	rBV	234	113	0.01%	0.001%
5	2.625	490	493	497	rBV3	457	379	0.04%	0.004%
6	2.686	510	512	514	rBV2	450	208	0.02%	0.002%
7	2.748	527	531	536	rVB3	537	499	0.05%	0.006%
8	2.770	536	538	539	rBV3	123	34	0.00%	0.000%
9	2.831	552	557	559	rBV2	179	189	0.02%	0.002%
10	2.950	591	594	597	rBV2	237	181	0.02%	0.002%
11	3.043	620	623	629	rVB2	218	235	0.02%	0.003%
12	3.108	640	643	645	rVB	205	110	0.01%	0.001%
13	3.130	645	650	651	rBV	165	127	0.01%	0.001%
14	3.146	653	655	658	rBV2	294	238	0.02%	0.003%
15	3.194	666	670	674	rBV2	178	188	0.02%	0.002%
16	3.211	674	675	677	rBV2	224	90	0.01%	0.001%
17	3.236	680	683	686	rVB	185	109	0.01%	0.001%
18	3.249	686	687	690	rBV	135	80	0.01%	0.001%
19	3.294	698	701	704	rVB	308	171	0.02%	0.002%
20	3.330	709	712	718	rVB2	234	158	0.01%	0.002%
21	3.391	726	731	735	rBB2	216	224	0.02%	0.003%
22	3.416	735	739	741	rBV	211	165	0.02%	0.002%
23	3.481	756	759	762	rBV	208	207	0.02%	0.002%
24	3.494	762	763	765	rBV	238	118	0.01%	0.001%
25	3.561	781	784	786	rBV2	210	140	0.01%	0.002%
26	3.619	799	802	803	rBV2	187	100	0.01%	0.001%
27	3.680	820	821	824	rVB2	123	47	0.00%	0.001%
28	3.709	827	830	832	rBV	167	112	0.01%	0.001%
29	3.751	841	843	845	rBV	249	82	0.01%	0.001%
30	3.773	848	850	856	rBV2	299	207	0.02%	0.002%
31	3.818	863	864	867	rBV2	205	74	0.01%	0.001%
32	3.879	873	883	928	rBV	61773	189632	17.91%	2.148%
33	4.198	979	982	985	rVB3	576	364	0.03%	0.004%
34	4.342	1010	1027	1054	rBV	171815	435591	41.14%	4.933%
35	4.680	1131	1132	1136	rBV2	238	182	0.02%	0.002%
36	4.696	1136	1137	1140	rVB	215	77	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011722\
 Data File : VW024374.D
 Acq On : 17 Jan 2022 13:11
 Operator : SY/MD
 Sample : N1168-12RE
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLX7RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

37	4.792	1165	1167	1168	rBV	533	278	0.03%	0.003%
38	5.040	1227	1244	1278	rBV2	398894	1047158	98.89%	11.860%
39	5.346	1337	1339	1340	rBV	353	166	0.02%	0.002%
40	5.519	1391	1393	1395	rBV	416	234	0.02%	0.003%
41	5.612	1410	1422	1451	rBV	439381	888742	83.93%	10.066%
42	5.902	1502	1512	1537	rVB2	17607	39006	3.68%	0.442%
43	5.992	1537	1540	1541	rBV	384	197	0.02%	0.002%
44	6.066	1549	1563	1593	rBV	225601	465722	43.98%	5.275%
45	6.310	1636	1639	1641	rBV	272	150	0.01%	0.002%
46	6.468	1685	1688	1689	rBV	151	85	0.01%	0.001%
47	6.500	1696	1698	1700	rBV	146	73	0.01%	0.001%
48	6.519	1702	1704	1708	rBV2	342	336	0.03%	0.004%
49	6.554	1712	1715	1718	rVV2	297	224	0.02%	0.003%
50	6.641	1740	1742	1743	rBV2	258	84	0.01%	0.001%
51	6.747	1772	1775	1777	rBV	298	174	0.02%	0.002%
52	6.854	1805	1808	1809	rBV	162	92	0.01%	0.001%
53	6.982	1837	1848	1867	rBV	136878	240545	22.72%	2.724%
54	7.185	1909	1911	1914	rBV2	367	298	0.03%	0.003%
55	7.243	1926	1929	1932	rBV2	351	222	0.02%	0.003%
56	7.262	1933	1935	1938	rBV	350	201	0.02%	0.002%
57	7.310	1939	1950	1970	rBV	507828	872093	82.36%	9.877%
58	7.619	2036	2046	2066	rBV	91834	159921	15.10%	1.811%
59	7.934	2137	2144	2154	rBV3	2424	3951	0.37%	0.045%
60	8.046	2176	2179	2181	rBV	330	180	0.02%	0.002%
61	8.085	2181	2191	2232	rVV	211010	422855	39.93%	4.789%
62	8.497	2316	2319	2324	rBV2	281	269	0.03%	0.003%
63	8.529	2326	2329	2330	rBV2	487	200	0.02%	0.002%
64	8.570	2339	2342	2346	rBV2	231	243	0.02%	0.003%
65	8.641	2362	2364	2365	rBV	227	117	0.01%	0.001%
66	8.667	2370	2372	2374	rBV	266	151	0.01%	0.002%
67	8.802	2412	2414	2416	rBV2	352	211	0.02%	0.002%
68	8.847	2416	2428	2452	rBV	653139	1058906	100.00%	11.993%
69	9.146	2517	2521	2531	rVB3	896	1264	0.12%	0.014%
70	9.217	2541	2543	2547	rBV2	281	205	0.02%	0.002%
71	9.368	2588	2590	2592	rBV	295	196	0.02%	0.002%
72	9.423	2603	2607	2610	rVB2	269	227	0.02%	0.003%
73	9.471	2617	2622	2626	rBV2	345	322	0.03%	0.004%
74	9.542	2642	2644	2646	rBV	235	92	0.01%	0.001%
75	9.635	2669	2673	2674	rBV	283	150	0.01%	0.002%
76	9.667	2680	2683	2685	rBV2	295	154	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011722\
 Data File : VV024374.D
 Acq On : 17 Jan 2022 13:11
 Operator : SY/MD
 Sample : N1168-12RE
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLX7RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

77	9.734	2701	2704	2705	rBV	238	104	0.01%	0.001%
78	9.805	2724	2726	2728	rBV	268	152	0.01%	0.002%
79	9.857	2740	2742	2744	rBV	216	93	0.01%	0.001%
80	10.095	2815	2816	2817	rBV	172	43	0.00%	0.000%
81	10.123	2817	2825	2834	rVV3	2433	4029	0.38%	0.046%
82	10.214	2841	2853	2872	rBV	286778	444725	42.00%	5.037%
83	10.445	2922	2925	2926	rBV	440	230	0.02%	0.003%
84	10.673	2994	2996	2999	rBV	247	137	0.01%	0.002%
85	10.831	3042	3045	3047	rBV2	513	319	0.03%	0.004%
86	11.146	3136	3143	3150	rBV7	1470	2197	0.21%	0.025%
87	11.246	3163	3174	3202	rBV	682561	1046524	98.83%	11.853%
88	11.529	3254	3262	3280	rBV3	9432	19778	1.87%	0.224%
89	11.622	3280	3291	3314	rVB	525129	818454	77.29%	9.270%
90	11.840	3354	3359	3360	rBV2	508	462	0.04%	0.005%
91	11.979	3399	3402	3405	rBV2	473	314	0.03%	0.004%
92	12.059	3425	3427	3429	rVB	302	119	0.01%	0.001%
93	12.738	3636	3638	3639	rBV	335	107	0.01%	0.001%
94	12.982	3713	3714	3718	rVB	398	140	0.01%	0.002%
95	13.172	3769	3773	3775	rBV2	462	361	0.03%	0.004%
96	13.811	3969	3972	3977	rBV3	543	421	0.04%	0.005%




Sum of corrected areas: 8829402

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011722\
Data File : VV024374.D
Acq On : 17 Jan 2022 13:11
Operator : SY/MD
Sample : N1168-12RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLX7RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

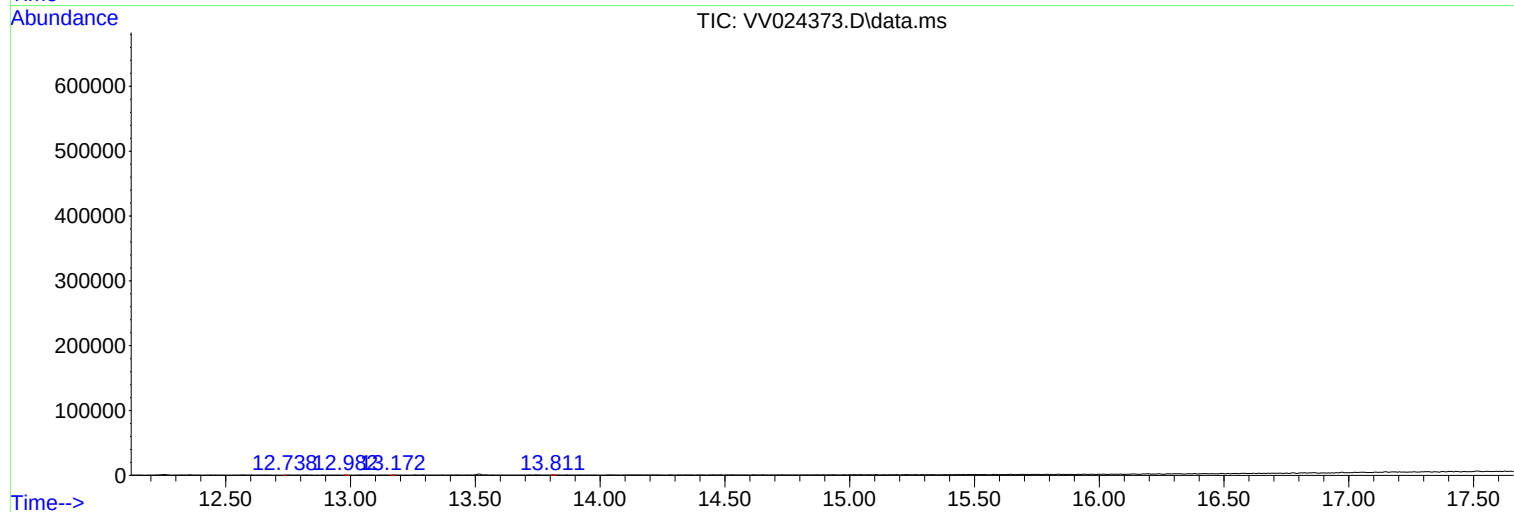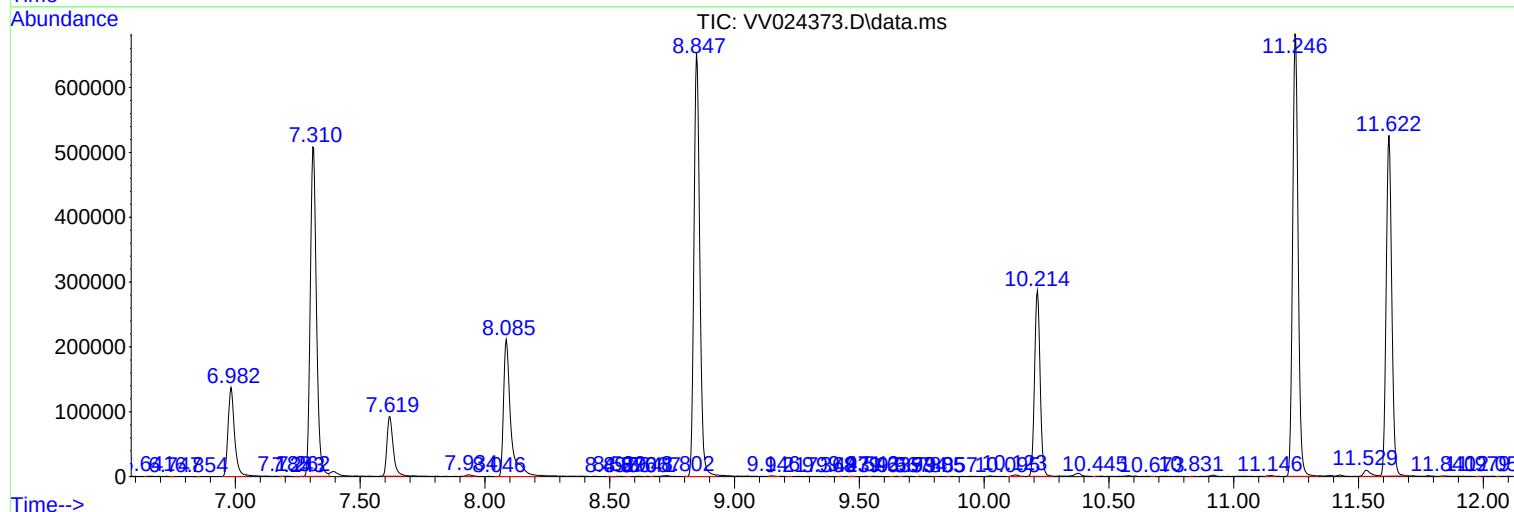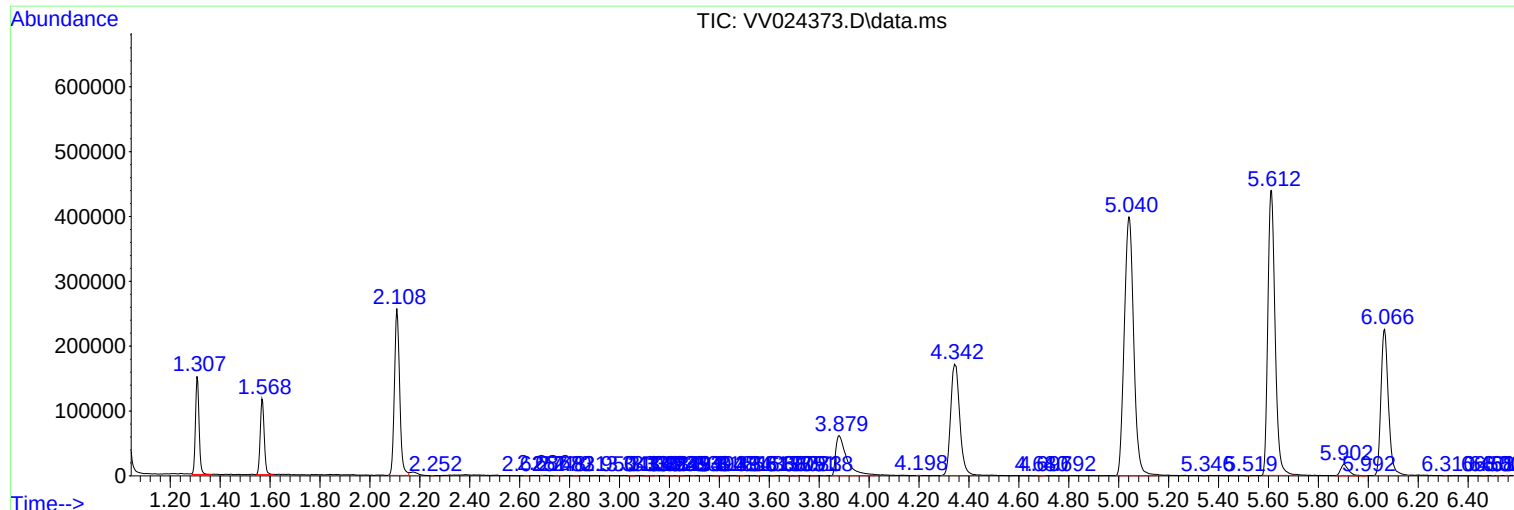

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011722\
Data File : VV024374.D
Acq On : 17 Jan 2022 13:11
Operator : SY/MD
Sample : N1168-12RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLX7RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011722\
Data File : VV024374.D
Acq On : 17 Jan 2022 13:11
Operator : SY/MD
Sample : N1168-12RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLX7RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc