
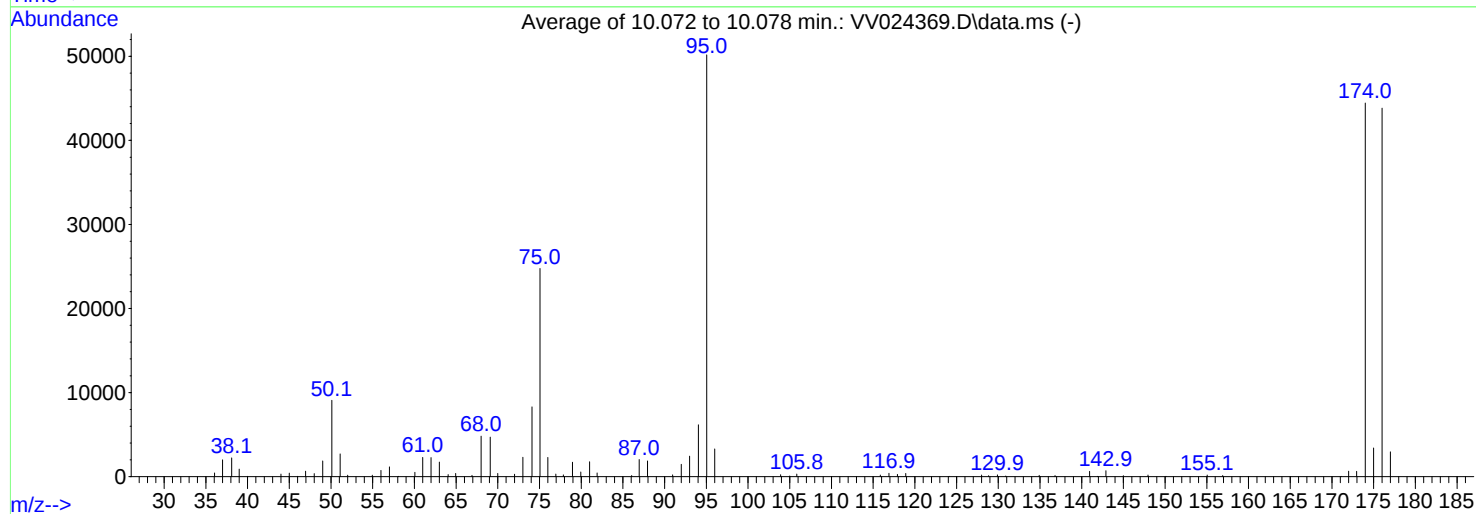


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011722\
 Data File : VV024369.D
 Acq On : 17 Jan 2022 09:02
 Operator : SY/MD
 Sample : BFB256
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB256

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis
 Last Update : Fri Jan 21 00:04:44 2022

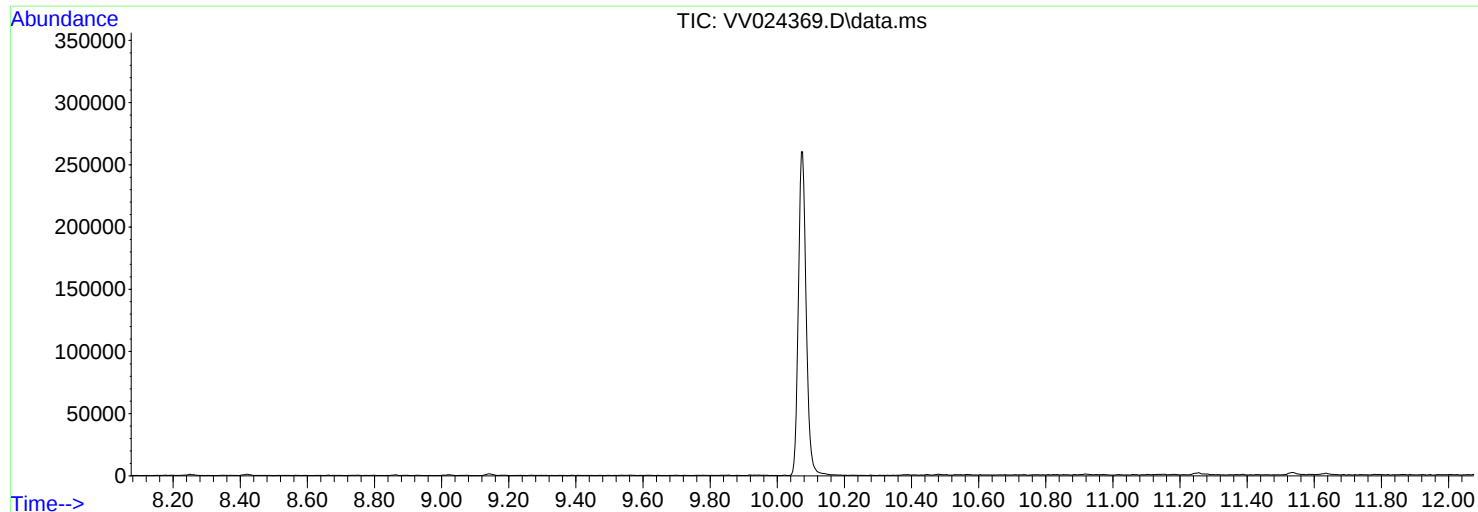

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	9070	PASS
75	95	30	80	49.4	24763	PASS
95	95	100	100	100.0	50176	PASS
96	95	5	9	6.6	3290	PASS
173	174	0.00	2	1.4	634	PASS
174	95	50	120	88.6	44443	PASS
175	174	5	9	7.7	3413	PASS
176	174	95	105	98.6	43840	PASS
177	176	5	10	6.7	2949	PASS

m/z	Abundance
39.90	189.0
44.10	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
36.00	531.0
37.00	2079.0
38.10	2275.0
39.00	939.0
39.80	162.0
44.00	436.0
45.00	455.0
46.00	140.0
46.90	636.0
48.00	353.0
49.00	1957.0
50.10	9801.0
51.10	2904.0
52.00	191.0
54.90	189.0
56.00	744.0
57.00	1257.0
60.00	470.0
61.00	2249.0
62.00	2461.0
63.00	1792.0
64.10	281.0
64.90	354.0
66.90	159.0
68.00	5022.0
69.10	5055.0
70.00	384.0
72.00	322.0
73.00	2340.0
74.10	8561.0
75.00	25864.0
76.00	2467.0
77.00	323.0
77.80	214.0
78.90	1791.0
80.00	556.0
81.00	1863.0
81.90	407.0
86.00	117.0
86.90	2121.0
88.00	1937.0
90.90	212.0
92.00	1534.0
93.00	2357.0
94.10	6458.0
95.10	51496.0
96.00	3426.0
103.90	246.0
105.00	121.0
105.80	335.0
115.80	178.0
116.90	417.0
117.90	288.0
118.90	408.0
128.00	200.0
128.90	114.0
129.90	230.0
130.90	125.0
134.90	150.0
136.80	120.0
140.90	633.0
142.90	691.0
145.00	194.0
147.90	156.0
155.10	178.0
156.90	135.0
171.10	127.0
172.00	718.0
173.00	680.0
174.00	45760.0
175.00	3526.0
176.00	44072.0
177.00	3092.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
36.10	431.0
37.00	2071.0
38.10	2317.0
39.00	901.0
44.00	430.0
45.00	433.0
47.00	681.0
48.00	382.0
49.00	1940.0
50.10	9369.0
51.10	2821.0
52.00	181.0
54.90	179.0
56.00	772.0
57.00	1169.0
60.10	525.0
61.00	2367.0
62.00	2339.0
63.00	1755.0
64.10	256.0
65.00	386.0
66.90	160.0
68.00	4988.0
69.10	4810.0
70.00	412.0
72.00	310.0
73.00	2377.0
74.10	8535.0
75.10	25592.0
76.00	2399.0
76.90	325.0
77.80	208.0
78.90	1768.0
79.90	578.0
81.00	1809.0
81.90	450.0
86.00	132.0
87.00	2118.0
88.00	1916.0
91.00	215.0
92.00	1527.0
93.00	2574.0
94.00	6387.0
95.00	51664.0
96.00	3368.0
103.90	239.0
105.00	104.0
105.80	311.0
115.80	201.0
116.90	421.0
117.90	281.0
118.90	388.0
128.00	188.0
128.80	134.0
129.90	229.0
130.90	106.0
134.90	154.0
136.80	141.0
140.90	654.0
142.90	724.0
145.00	159.0
147.90	201.0
150.10	115.0
155.10	195.0
156.90	144.0
172.00	678.0
173.00	651.0
174.00	45904.0
175.00	3517.0
176.00	45376.0
177.00	3021.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
36.10	336.0
37.00	1869.0
38.10	2073.0
39.00	817.0
40.00	148.0
44.00	459.0
45.00	347.0
47.00	652.0
48.00	330.0
49.00	1703.0
50.10	8039.0
51.10	2414.0
52.00	127.0
55.00	147.0
56.00	704.0
57.00	1061.0
58.10	100.0
60.00	537.0
61.00	2254.0
62.00	1986.0
63.00	1624.0
64.00	221.0
65.00	384.0
66.90	164.0
68.00	4455.0
69.10	4261.0
70.00	369.0
72.00	251.0
73.00	2198.0
74.10	7821.0
75.10	22832.0
76.00	2005.0
76.90	298.0
77.90	197.0
79.00	1575.0
79.90	519.0
81.00	1630.0
81.90	462.0
86.10	167.0
87.00	1862.0
87.90	1727.0
91.00	226.0
92.00	1342.0
93.00	2378.0
94.00	5640.0
95.00	47368.0
96.00	3076.0
103.90	210.0
105.90	265.0
115.90	184.0
116.90	378.0
117.90	261.0
118.90	341.0
124.10	108.0
128.00	163.0
128.80	128.0
129.90	191.0
134.90	139.0
136.80	145.0
141.00	625.0
141.90	102.0
142.90	714.0
148.00	196.0
155.00	174.0
156.90	131.0
172.00	576.0
172.90	571.0
174.00	41664.0
175.00	3196.0
176.00	42072.0
177.00	2733.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256