




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
Data File : VV024386.D
Acq On : 18 Jan 2022 11:12
Operator : SY/MD
Sample : VV0118WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK302

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/19/2022
Supervised By :Mahesh Dadoda 01/19/2022

Quant Time: Jan 19 01:04:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 19 01:03:04 2022
Response via : Initial Calibration

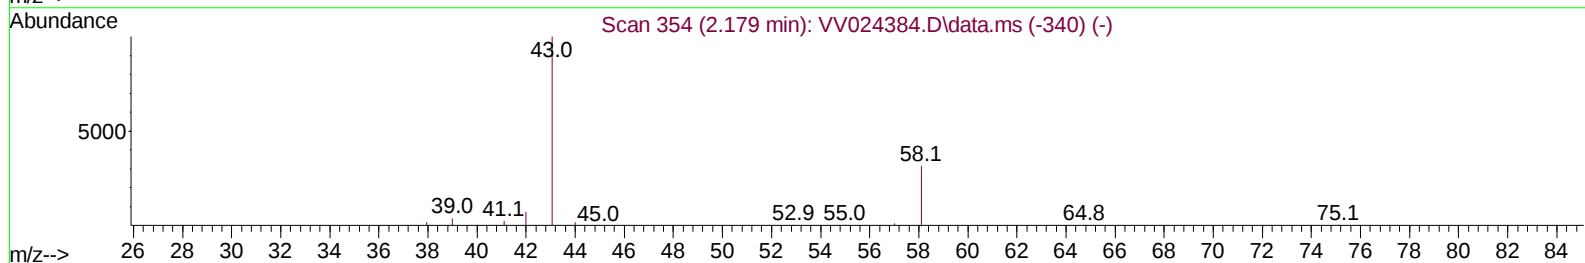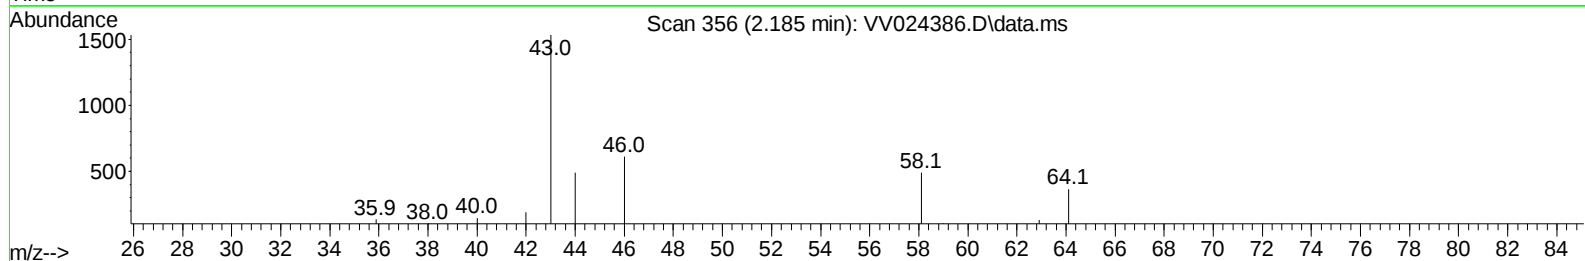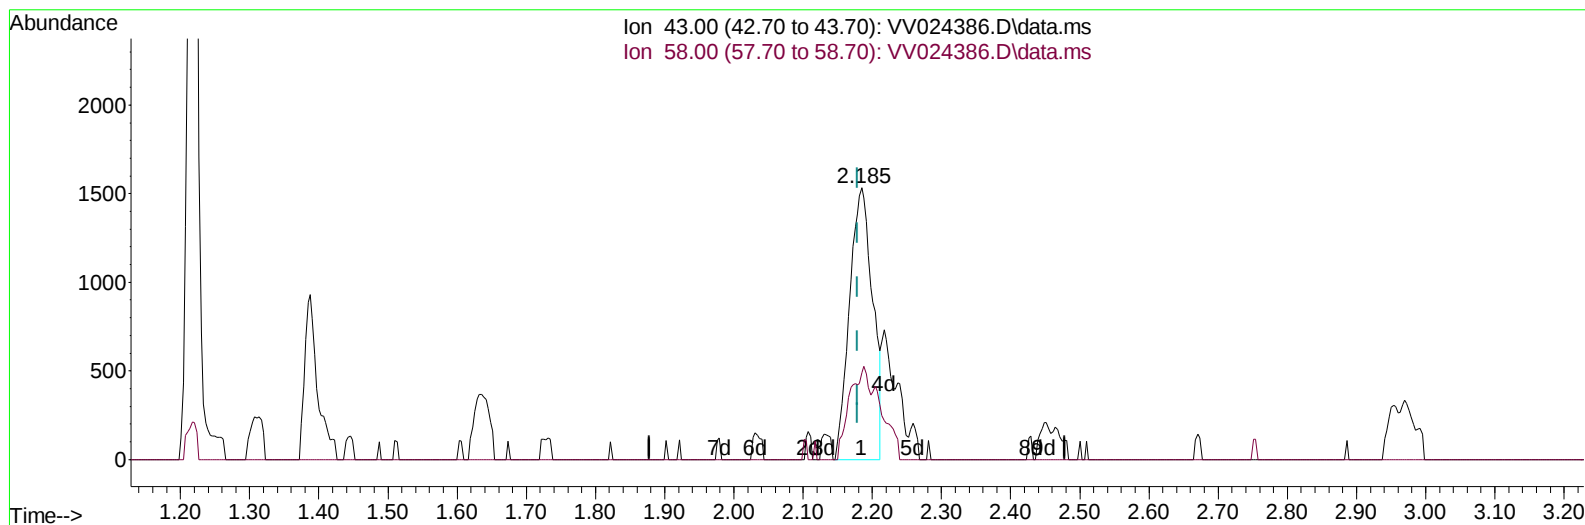

TIC: VV024386.D\data.ms

(13) Acetone (T)

2.185min (+ 0.006) 2.87 ug/L

response 3548

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.50	4.09
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
 Data File : VV024386.D
 Acq On : 18 Jan 2022 11:12
 Operator : SY/MD
 Sample : VV0118WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK302

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/19/2022
 Supervised By :Mahesh Dadoda 01/19/2022

Quant Time: Jan 19 01:04:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 19 01:03:04 2022
 Response via : Initial Calibration

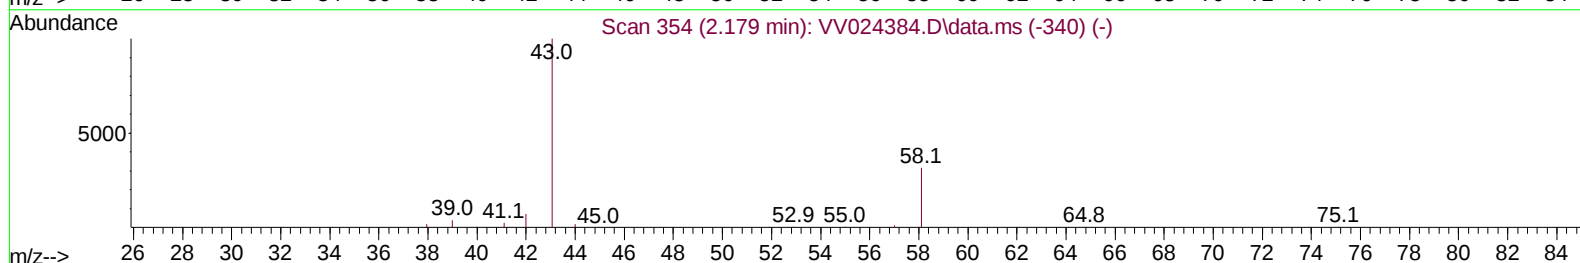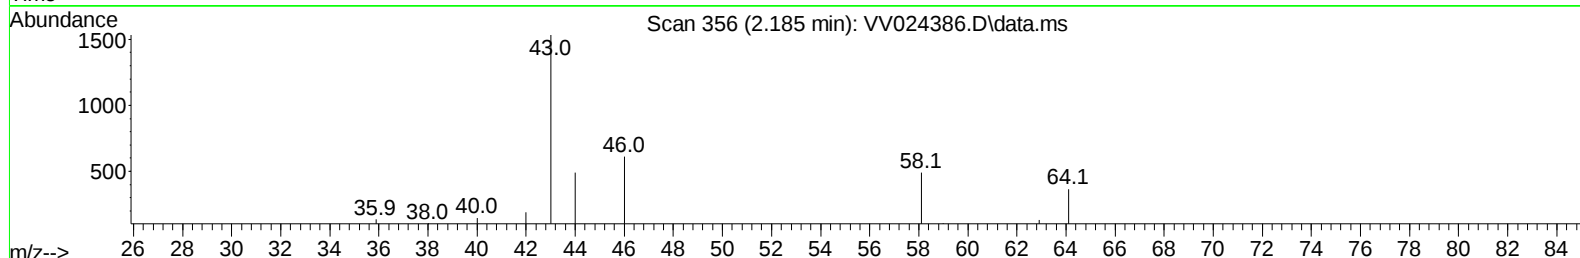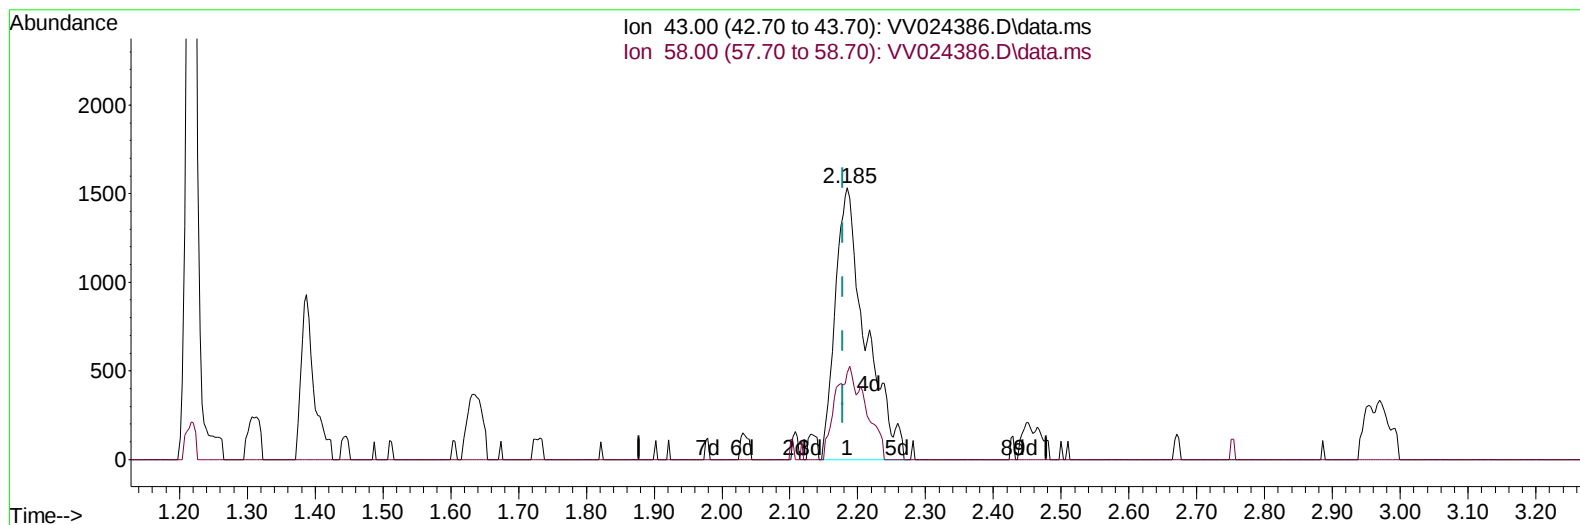

TIC: VV024386.D\data.ms

(13) Acetone (T)

2.185min (+ 0.006) 3.84 ug/L m

response 4754

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.50	3.05
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
 Data File : VV024386.D
 Acq On : 18 Jan 2022 11:12
 Operator : SY/MD
 Sample : VV0118WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK302

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 01/19/2022
 Supervised By : Mahesh Dadoda 01/19/2022

Quant Time: Jan 19 01:04:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 19 01:03:04 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.612	114		312428	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		292162	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		143482	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.307	65		94839	42.179	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery =	84.360%		
7) Chloroethane-d5	1.571	69		78850	46.163	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery =	92.320%		
11) 1,1-Dichloroethene-d2	2.108	63		140859	33.519	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery =	67.040%		
21) 2-Butanone-d5	3.889	46		141991	113.344	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery =	113.340%		
24) Chloroform-d	4.346	84		206921	50.352	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	100.700%		
26) 1,2-Dichloroethane-d4	5.027	65		134564	48.907	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	97.820%		
32) Benzene-d6	5.047	84		415873	54.547	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	109.100%		
36) 1,2-Dichloropropane-d6	6.066	67		126807	59.347	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery =	118.700%		
41) Toluene-d8	7.313	98		392246	53.136	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery =	106.280%		
43) trans-1,3-Dichloroprop...	7.619	79		61803	50.231	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery =	100.460%		
47) 2-Hexanone-d5	8.088	63		91917	99.015	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery =	99.020%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84		154722	50.670	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery =	101.340%		
66) 1,2-Dichlorobenzene-d4	11.622	152		159278	55.692	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery =	111.380%		
Target Compounds							
13) Acetone	2.185	43		4754m	3.844	ug/L	
48) 2-Hexanone	8.146	43		13116	7.167	ug/L #	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
Data File : VV024386.D
Acq On : 18 Jan 2022 11:12
Operator : SY/MD
Sample : VV0118WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK302

Manual IntegrationsAPPROVED

Quant Time: Jan 19 01:04:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 19 01:03:04 2022
Response via : Initial Calibration

Reviewed By :John Carlone 01/19/2022
Supervised By :Mahesh Dadoda 01/19/2022

