




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
Data File : VV024390.D
Acq On : 18 Jan 2022 13:46
Operator : SY/MD
Sample : N1115-13ME
Misc : 6.31g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLS3ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/19/2022
Supervised By :Mahesh Dadoda 01/19/2022

Quant Time: Jan 19 01:04:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 19 01:03:04 2022
Response via : Initial Calibration

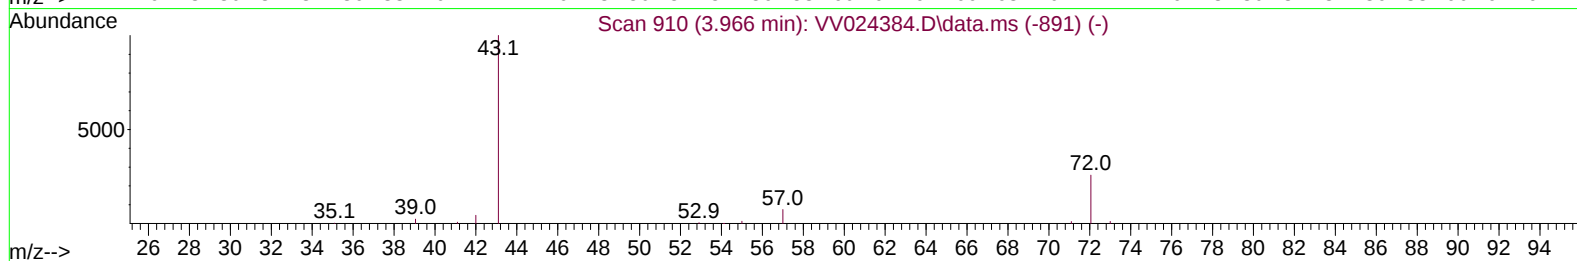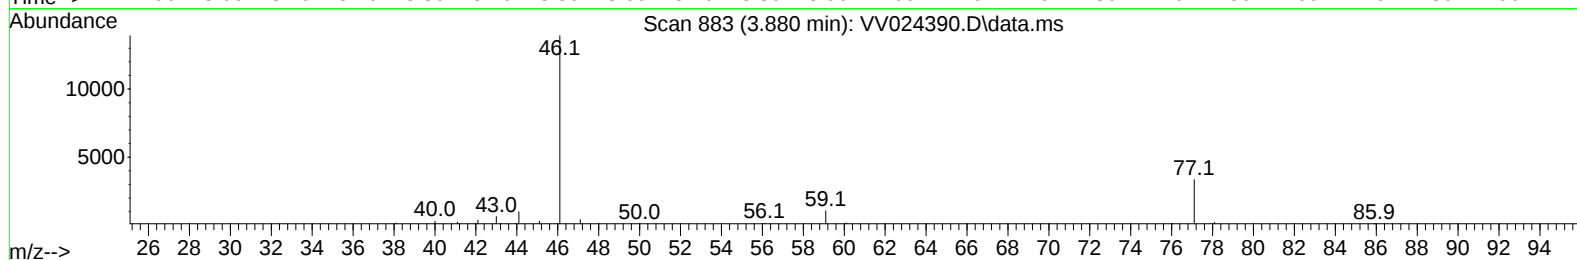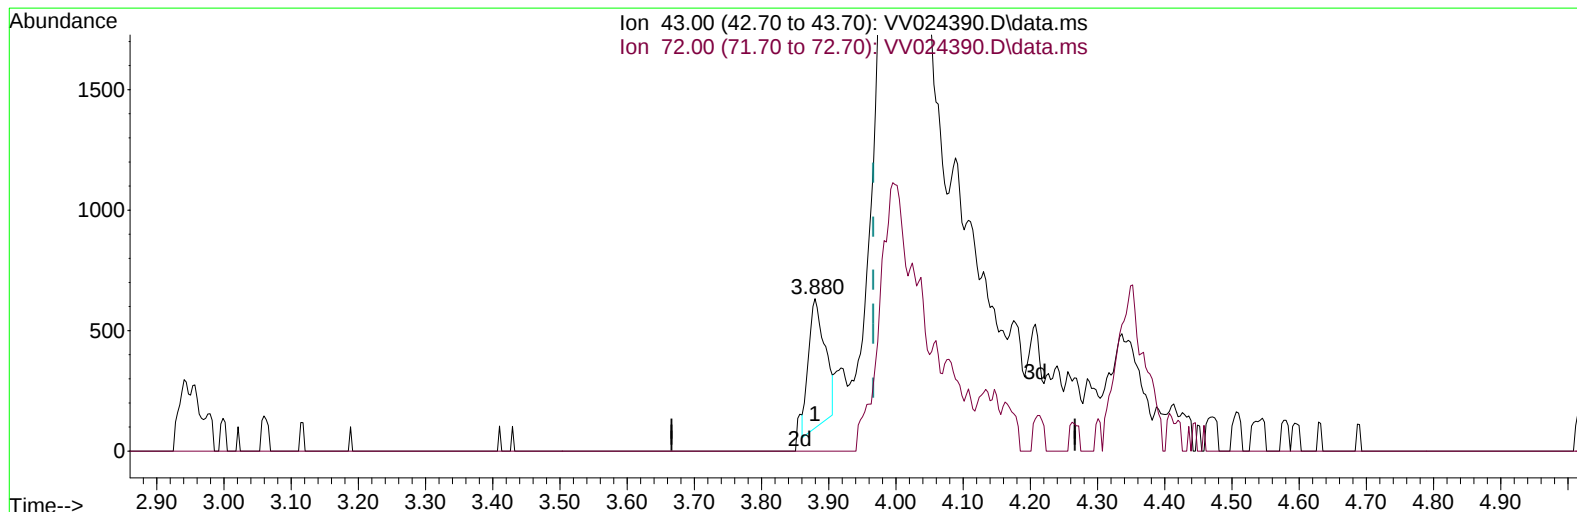

TIC: VV024390.D\data.ms

(22) 2-Butanone (T)

3.880min (-0.087) 0.54 ug/L

response 909

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.90	225.96#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
Data File : VV024390.D
Acq On : 18 Jan 2022 13:46
Operator : SY/MD
Sample : N1115-13ME
Misc : 6.31g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLS3ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/19/2022
Supervised By :Mahesh Dadoda 01/19/2022

Quant Time: Jan 19 01:04:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 19 01:03:04 2022
Response via : Initial Calibration

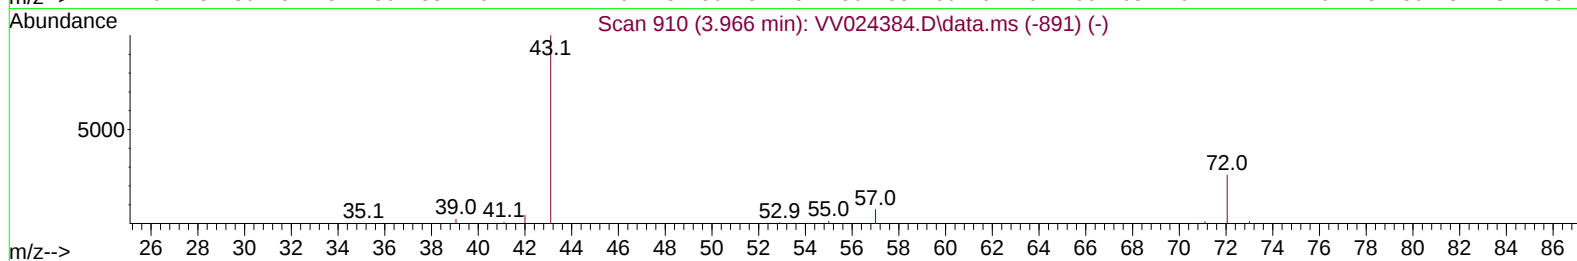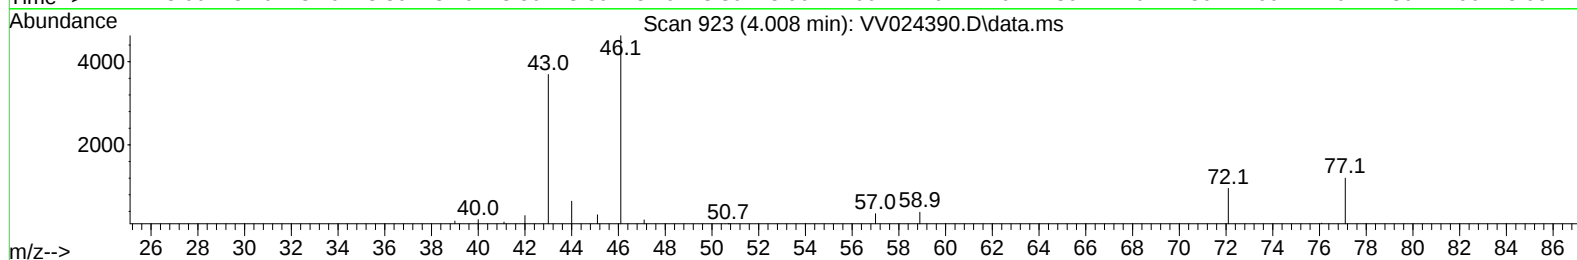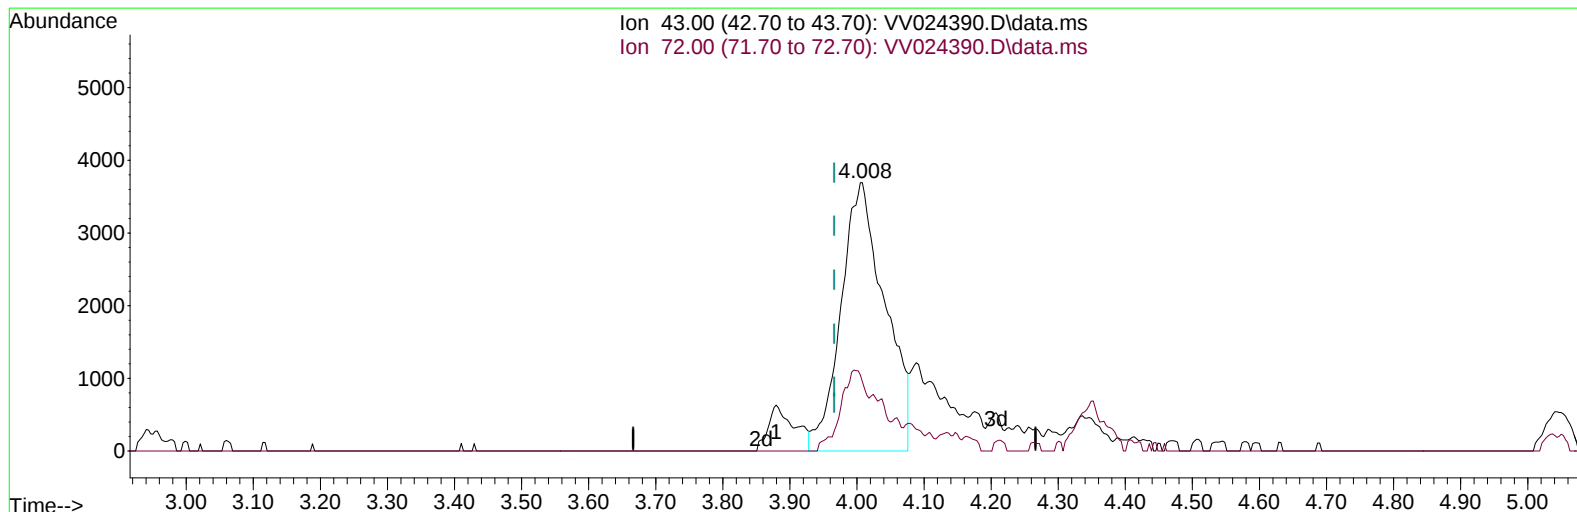

TIC: VV024390.D\data.ms

(22) 2-Butanone (T)

4.008min (+ 0.042) 10.06 ug/L m

response 16777

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.90	12.24#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
Data File : VV024390.D
Acq On : 18 Jan 2022 13:46
Operator : SY/MD
Sample : N1115-13ME
Misc : 6.31g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLS3ME

Manual IntegrationsAPPROVED

Quant Time: Jan 19 01:04:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 19 01:03:04 2022
Response via : Initial Calibration

Reviewed By :John Carlone 01/19/2022
Supervised By :Mahesh Dadoda 01/19/2022

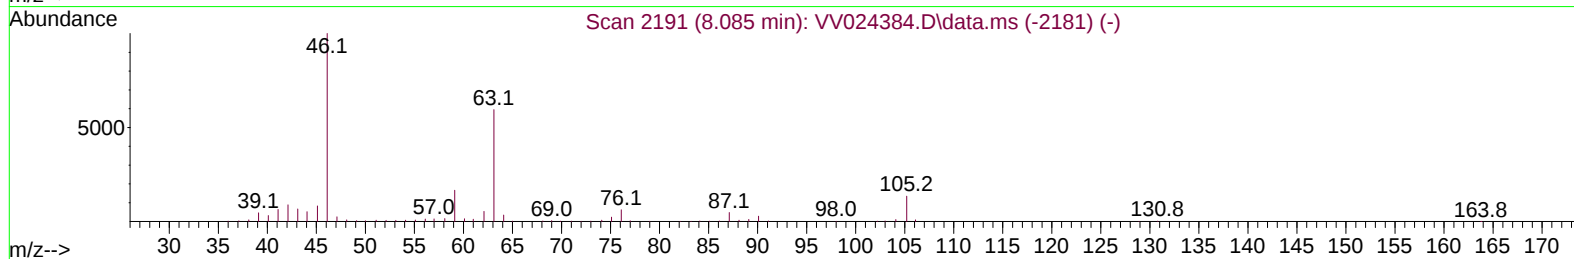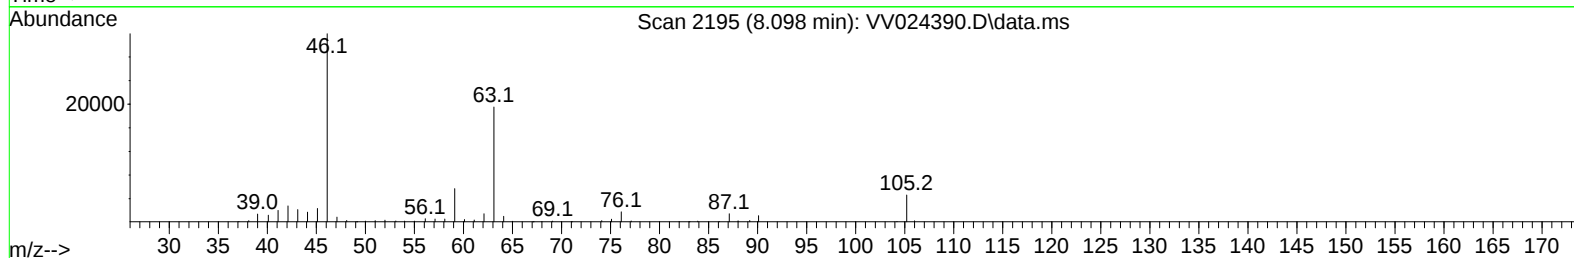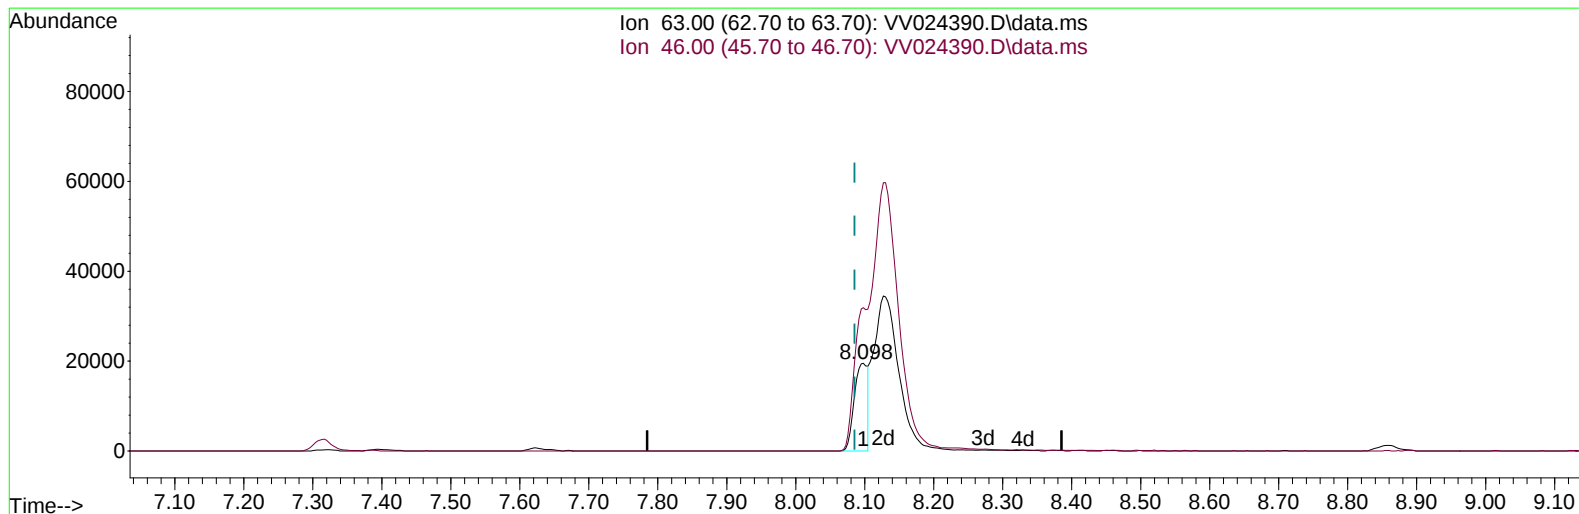

TIC: VV024390.D\data.ms

(47) 2-Hexanone-d5 (S)

8.098min (+ 0.013) 22.61 ug/L

response 26729

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	169.00	141.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
Data File : VV024390.D
Acq On : 18 Jan 2022 13:46
Operator : SY/MD
Sample : N1115-13ME
Misc : 6.31g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLS3ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/19/2022
Supervised By :Mahesh Dadoda 01/19/2022

Quant Time: Jan 19 01:04:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 19 01:03:04 2022
Response via : Initial Calibration

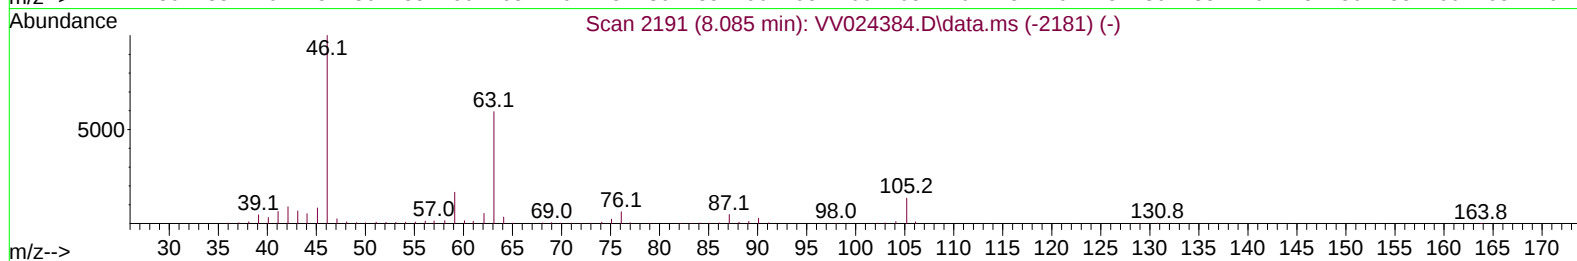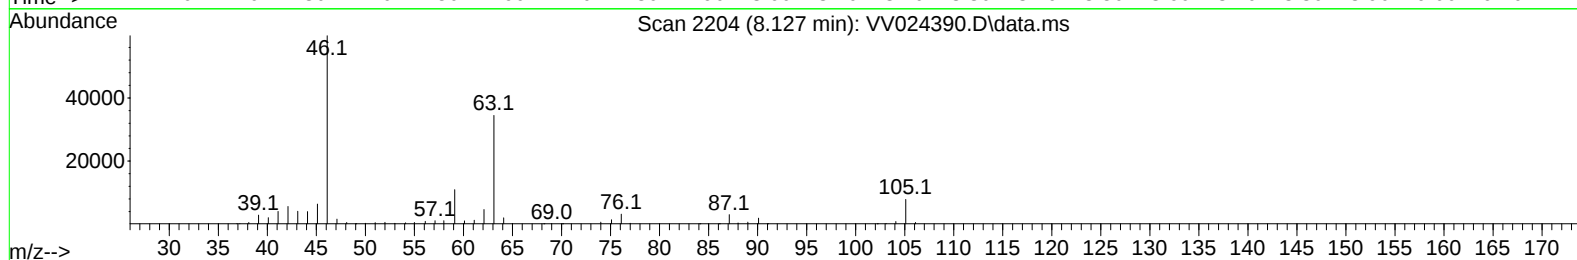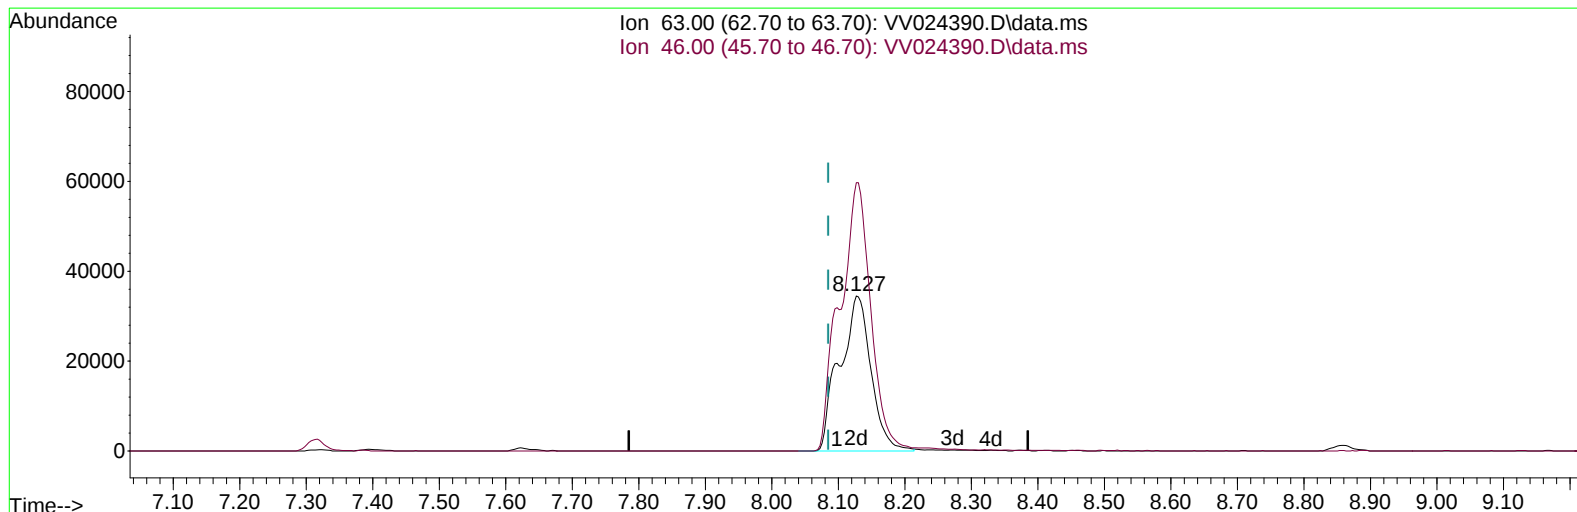

TIC: VV024390.D\data.ms

(47) 2-Hexanone-d5 (S)

8.127min (+ 0.042) 95.80 ug/L m

response 113236

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	169.00	33.45#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011822\
 Data File : VW024390.D
 Acq On : 18 Jan 2022 13:46
 Operator : SY/MD
 Sample : N1115-13ME
 Misc : 6.31g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLS3ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/19/2022
 Supervised By :Mahesh Dadoda 01/19/2022

Quant Time: Jan 19 01:04:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 19 01:03:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	396650	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	372018	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	182111	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	107529	37.668	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	75.340%		
7) Chloroethane-d5	1.568	69	76028	35.059	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	70.120%		
11) 1,1-Dichloroethene-d2	2.092	63	163516	30.648	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	61.300%		
21) 2-Butanone-d5	3.899	46	146199	91.923	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	91.920%		
24) Chloroform-d	4.346	84	242474	46.475	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.960%		
26) 1,2-Dichloroethane-d4	5.027	65	162619	46.554	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.100%		
32) Benzene-d6	5.043	84	494485	50.936	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.880%		
36) 1,2-Dichloropropane-d6	6.066	67	149278	54.867	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	109.740%		
41) Toluene-d8	7.314	98	470959	50.104	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.200%		
43) trans-1,3-Dichloroprop...	7.622	79	77920	49.736	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	99.480%		
47) 2-Hexanone-d5	8.127	63	113236m	95.797	ug/L	0.04
Spiked Amount 100.000	Range 45 - 130		Recovery =	95.800%		
56) 1,1,2,2-Tetrachloroeth...	10.227	84	184216	47.379	ug/L	0.01
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.760%		
66) 1,2-Dichlorobenzene-d4	11.628	152	192153	52.936	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.880%		
Target Compounds					Qvalue	
13) Acetone	2.188	43	4830	3.076	ug/L	64
22) 2-Butanone	4.008	43	16777m	10.058	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
Data File : VV024390.D
Acq On : 18 Jan 2022 13:46
Operator : SY/MD
Sample : N1115-13ME
Misc : 6.31g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLS3ME

Manual IntegrationsAPPROVED

Quant Time: Jan 19 01:04:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 19 01:03:04 2022
Response via : Initial Calibration

Reviewed By :John Carlone 01/19/2022
Supervised By :Mahesh Dadoda 01/19/2022

