

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011822\
 Data File : VW024394.D
 Acq On : 18 Jan 2022 15:21
 Operator : SY/MD
 Sample : N1129-06ME
 Misc : 6.14g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBLZ9ME

Quant Time: Jan 19 01:05:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 19 01:03:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	328246	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	305402	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	151678	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	100823	42.679	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.360%
7) Chloroethane-d5	1.571	69	72670	40.494	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.980%
11) 1,1-Dichloroethene-d2	2.092	63	153269	34.714	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.420%
21) 2-Butanone-d5	3.902	46	133766	101.633	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.630%
24) Chloroform-d	4.346	84	231968	53.727	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.460%
26) 1,2-Dichloroethane-d4	5.027	65	153811	53.209	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.420%
32) Benzene-d6	5.043	84	469260	58.881	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	117.760%
36) 1,2-Dichloropropane-d6	6.066	67	144394	64.648	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	129.300%#
41) Toluene-d8	7.313	98	443486	57.473	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	114.940%
43) trans-1,3-Dichloroprop...	7.622	79	73881	57.444	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	114.880%
47) 2-Hexanone-d5	8.098	63	27199	28.029	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	28.030%#
56) 1,1,2,2-Tetrachloroeth...	10.226	84	178968	56.069	ug/L	0.01
Spiked Amount	50.000	Range	65 - 120	Recovery	=	112.140%
66) 1,2-Dichlorobenzene-d4	11.628	152	181882	60.160	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	120.320%#
Target Compounds					Qvalue	
13) Acetone	2.195	43	5827	4.484	ug/L	65
22) 2-Butanone	3.998	43	12866	9.321	ug/L	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
Data File : VV024394.D
Acq On : 18 Jan 2022 15:21
Operator : SY/MD
Sample : N1129-06ME
Misc : 6.14g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBLZ9ME

Quant Time: Jan 19 01:05:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 19 01:03:04 2022
Response via : Initial Calibration




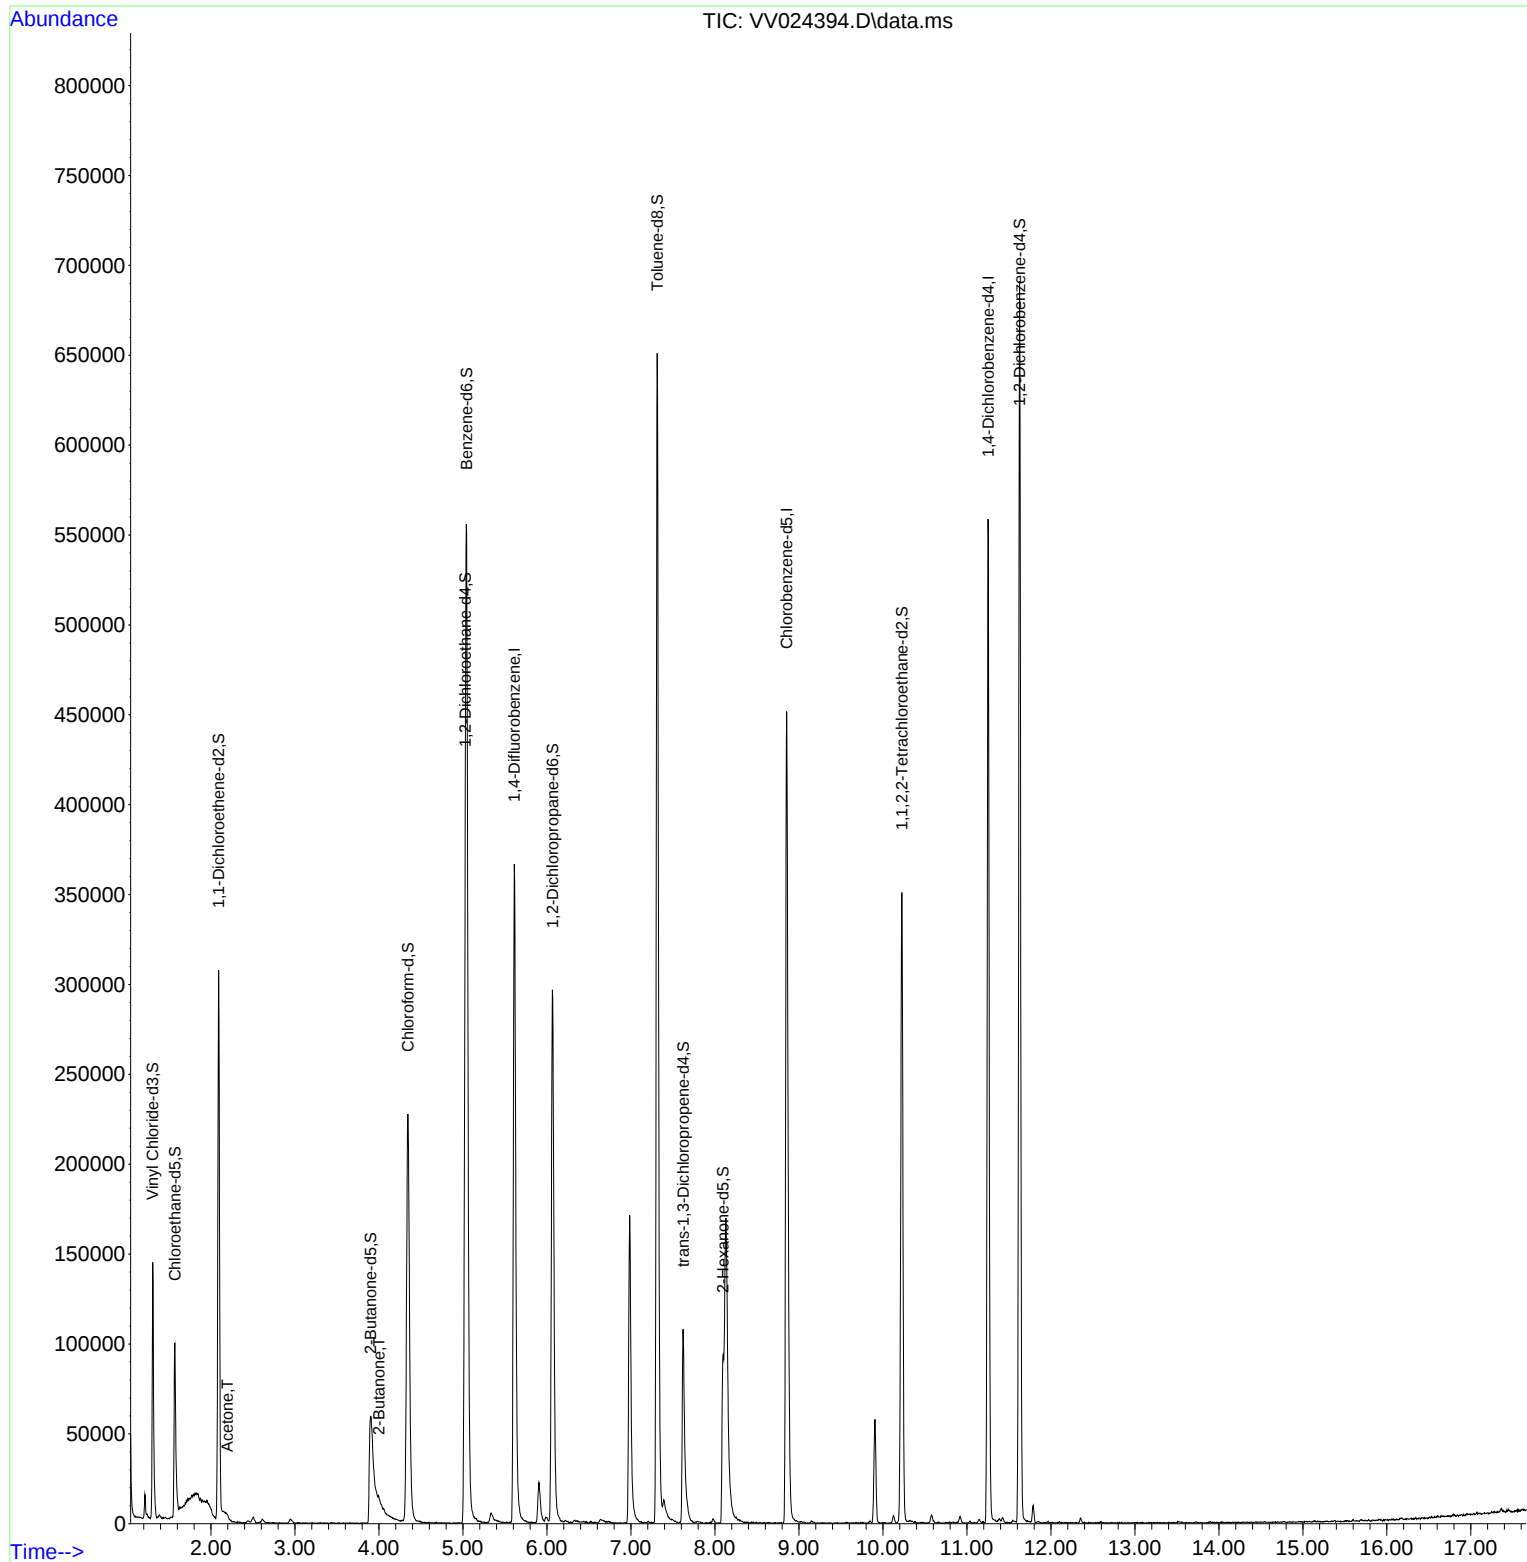


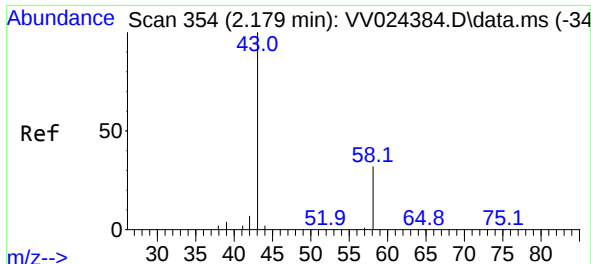

#13
Acetone
Concen: 4.484 ug/L
RT: 2.195 min Scan# 31
Delta R.T. 0.016 min
Lab File: VV024394.D
Acq: 18 Jan 2022 15:21

Instrument :
MSVOA_V
ClientSampleId :
DBLZ9ME

Tgt Ion: 43 Resp: 5827
Ion Ratio Lower Upper
43 100
58 11.9 0.0 63.0

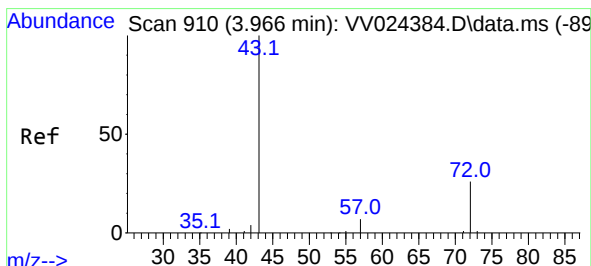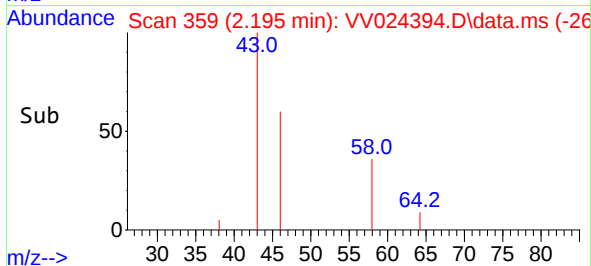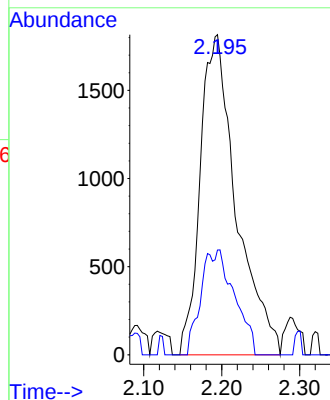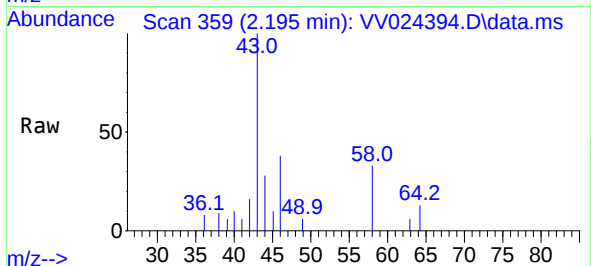

#22
2-Butanone
Concen: 9.321 ug/L
RT: 3.998 min Scan# 920
Delta R.T. 0.032 min
Lab File: VV024394.D
Acq: 18 Jan 2022 15:21

Tgt Ion: 43 Resp: 12866
Ion Ratio Lower Upper
43 100
72 16.6 14.9 44.9

