

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
 Data File : VV024387.D
 Acq On : 18 Jan 2022 12:36
 Operator : SY/MD
 Sample : N1114-20ME
 Misc : 5.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLR2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

Signal : TIC: VV024387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	49	54	59	rBV2	21968	20656	0.23%	0.098%
2	1.307	76	83	100	rVB	153474	188923	2.09%	0.894%
3	1.542	148	156	160	rBV	115537	145683	1.61%	0.689%
4	2.089	316	326	339	rBV2	351338	533282	5.90%	2.522%
5	2.571	470	476	478	rBV3	328	270	0.00%	0.001%
6	2.606	478	487	491	rBV4	2475	3427	0.04%	0.016%
7	2.661	502	504	508	rVB4	631	293	0.00%	0.001%
8	2.690	510	513	514	rBV2	387	205	0.00%	0.001%
9	2.716	518	521	524	rBV3	450	240	0.00%	0.001%
10	2.744	524	530	532	rBV2	1160	1051	0.01%	0.005%
11	2.802	545	548	550	rBV2	321	180	0.00%	0.001%
12	2.941	581	591	607	rVV7	3499	8042	0.09%	0.038%
13	3.021	610	616	618	rVB3	649	574	0.01%	0.003%
14	3.179	653	665	686	rBV	31046	65113	0.72%	0.308%
15	3.326	706	711	713	rBV2	312	239	0.00%	0.001%
16	3.346	713	717	719	rVB	415	285	0.00%	0.001%
17	3.400	732	734	740	rVB2	303	235	0.00%	0.001%
18	3.436	740	745	747	rBV	240	248	0.00%	0.001%
19	3.539	772	777	780	rBV2	343	280	0.00%	0.001%
20	3.770	845	849	853	rBV2	226	201	0.00%	0.001%
21	3.892	873	887	908	rBV	63640	216919	2.40%	1.026%
22	4.339	1012	1026	1057	rVB	226771	591809	6.55%	2.799%
23	4.696	1134	1137	1142	rBV3	260	269	0.00%	0.001%
24	4.757	1153	1156	1159	rBV2	247	146	0.00%	0.001%
25	4.793	1163	1167	1170	rBV3	297	254	0.00%	0.001%
26	4.863	1183	1189	1193	rVV3	444	423	0.00%	0.002%
27	4.879	1193	1194	1197	rVB2	400	186	0.00%	0.001%
28	4.902	1197	1201	1205	rBV3	528	522	0.01%	0.002%
29	5.034	1225	1242	1270	rBV2	590755	1474457	16.32%	6.974%
30	5.291	1319	1322	1324	rBV2	378	285	0.00%	0.001%
31	5.326	1324	1333	1343	rBV7	5437	12558	0.14%	0.059%
32	5.487	1379	1383	1384	rBV2	458	289	0.00%	0.001%
33	5.606	1408	1420	1455	rBV	442604	930173	10.30%	4.400%
34	5.905	1499	1513	1535	rBV	571527	1141079	12.63%	5.397%
35	6.063	1549	1562	1589	rVB	309375	655966	7.26%	3.103%
36	6.548	1712	1713	1715	rBV2	452	171	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011822\
 Data File : VW024387.D
 Acq On : 18 Jan 2022 12:36
 Operator : SY/MD
 Sample : N1114-20ME
 Misc : 5.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLR2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

37	6.632	1732	1739	1740	rBV5	2000	1879	0.02%	0.009%
38	6.844	1801	1805	1807	rVB2	506	281	0.00%	0.001%
39	6.911	1824	1826	1828	rBV	278	201	0.00%	0.001%
40	6.979	1836	1847	1879	rBV	176716	359868	3.98%	1.702%
41	7.172	1904	1907	1910	rBV2	318	259	0.00%	0.001%
42	7.194	1910	1914	1916	rBV2	712	582	0.01%	0.003%
43	7.227	1922	1924	1926	rVB2	472	158	0.00%	0.001%
44	7.243	1926	1929	1930	rBV2	475	242	0.00%	0.001%
45	7.310	1938	1950	1969	rBV	686387	1261623	13.97%	5.967%
46	7.616	2036	2045	2073	rBV	109358	241390	2.67%	1.142%
47	7.780	2093	2096	2099	rBV3	575	465	0.01%	0.002%
48	7.969	2138	2155	2181	rBV	5379354	9032943	100.00%	42.724%
49	8.091	2185	2193	2196	rBV	88524	122093	1.35%	0.577%
50	8.439	2295	2301	2303	rBV4	1253	1324	0.01%	0.006%
51	8.519	2324	2326	2328	rVB2	501	221	0.00%	0.001%
52	8.725	2387	2390	2392	rBV3	278	148	0.00%	0.001%
53	8.744	2393	2396	2400	rBV2	320	288	0.00%	0.001%
54	8.850	2416	2429	2463	rBV	554101	1127629	12.48%	5.333%
55	9.146	2513	2521	2541	rVV2	6822	14420	0.16%	0.068%
56	9.233	2545	2548	2551	rBV2	322	226	0.00%	0.001%
57	9.513	2631	2635	2637	rBV2	320	219	0.00%	0.001%
58	9.554	2641	2648	2658	rVV5	3477	6345	0.07%	0.030%
59	9.609	2662	2665	2671	rVV4	407	309	0.00%	0.001%
60	9.693	2687	2691	2695	rVB4	492	443	0.00%	0.002%
61	9.722	2695	2700	2704	rBV3	246	265	0.00%	0.001%
62	9.760	2710	2712	2715	rBV2	219	145	0.00%	0.001%
63	9.789	2717	2721	2723	rBV	256	190	0.00%	0.001%
64	9.805	2723	2726	2729	rBV4	346	189	0.00%	0.001%
65	9.834	2729	2735	2736	rBV2	898	854	0.01%	0.004%
66	9.934	2763	2766	2768	rBV	458	287	0.00%	0.001%
67	9.995	2781	2785	2786	rBV2	302	213	0.00%	0.001%
68	10.017	2790	2792	2794	rBV3	498	247	0.00%	0.001%
69	10.098	2807	2817	2821	rBV5	6357	10844	0.12%	0.051%
70	10.226	2840	2857	2877	rBV	349109	649617	7.19%	3.073%
71	10.452	2924	2927	2930	rBV3	485	359	0.00%	0.002%
72	10.516	2945	2947	2952	rVB3	372	221	0.00%	0.001%
73	10.554	2952	2959	2960	rBV5	878	1057	0.01%	0.005%
74	10.577	2960	2966	2974	rVV5	3420	5019	0.06%	0.024%
75	10.644	2984	2987	2989	rBV2	459	277	0.00%	0.001%
76	10.712	3003	3008	3010	rBV2	475	397	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011822\
 Data File : VW024387.D
 Acq On : 18 Jan 2022 12:36
 Operator : SY/MD
 Sample : N1114-20ME
 Misc : 5.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLR2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

77	10.866	3052	3056	3059	rBV2	694	645	0.01%	0.003%
78	11.117	3131	3134	3136	rVV	686	441	0.00%	0.002%
79	11.143	3137	3142	3150	rVB5	2228	3290	0.04%	0.016%
80	11.252	3164	3176	3195	rBV	697819	1113134	12.32%	5.265%
81	11.542	3263	3266	3268	rBV	381	276	0.00%	0.001%
82	11.628	3280	3293	3310	rBV	745930	1174428	13.00%	5.555%
83	11.776	3336	3339	3342	rBV2	713	672	0.01%	0.003%
84	11.847	3358	3361	3364	rBV4	516	368	0.00%	0.002%
85	11.889	3372	3374	3378	rBV	445	219	0.00%	0.001%
86	12.050	3421	3424	3427	rBV2	393	290	0.00%	0.001%
87	12.349	3511	3517	3526	rBV7	2902	4491	0.05%	0.021%
88	12.487	3558	3560	3562	rBV	453	176	0.00%	0.001%
89	12.786	3650	3653	3656	rBV2	549	415	0.00%	0.002%
90	12.850	3671	3673	3677	rVB	394	212	0.00%	0.001%
91	12.869	3677	3679	3681	rBV	361	247	0.00%	0.001%
92	13.207	3781	3784	3789	rVB2	344	249	0.00%	0.001%
93	13.513	3873	3879	3886	rBV5	1853	2342	0.03%	0.011%
94	13.554	3890	3892	3894	rBV2	393	185	0.00%	0.001%
95	13.609	3907	3909	3913	rVB2	446	172	0.00%	0.001%
96	13.722	3940	3944	3948	rBV3	310	328	0.00%	0.002%
97	13.831	3974	3978	3982	rBV3	383	332	0.00%	0.002%
98	14.030	4036	4040	4043	rBV4	469	451	0.00%	0.002%
99	14.303	4123	4125	4130	rBV3	335	211	0.00%	0.001%
100	14.892	4307	4308	4310	rBV	583	184	0.00%	0.001%




Sum of corrected areas: 21142428

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
Data File : VV024387.D
Acq On : 18 Jan 2022 12:36
Operator : SY/MD
Sample : N1114-20ME
Misc : 5.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLR2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

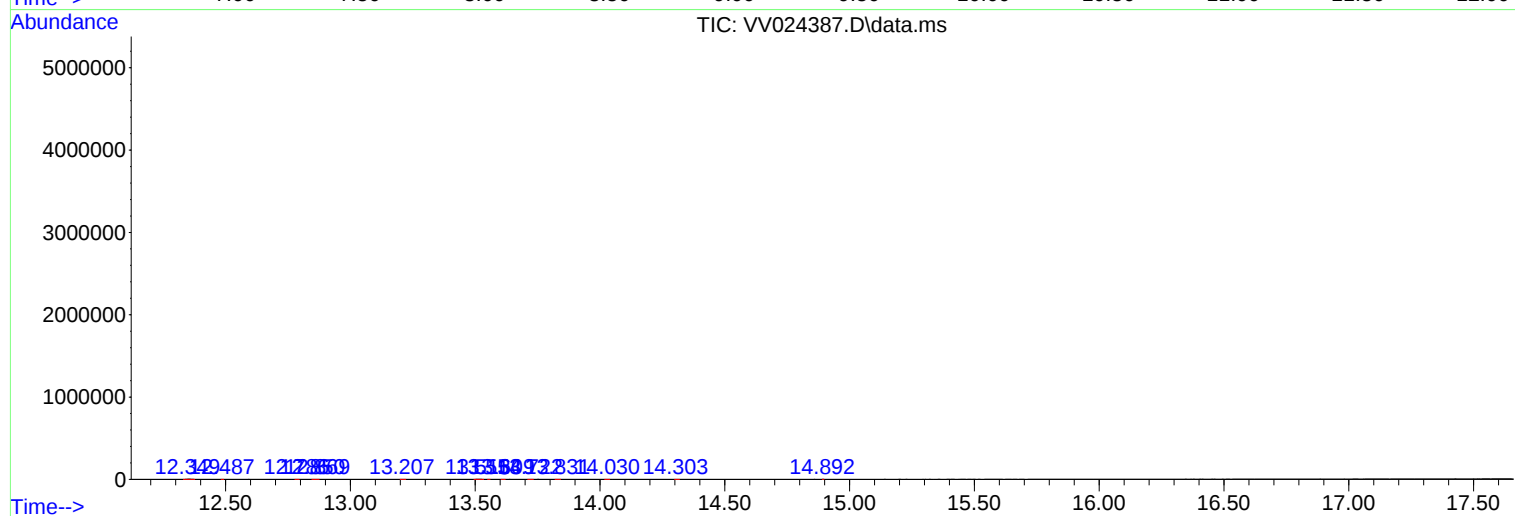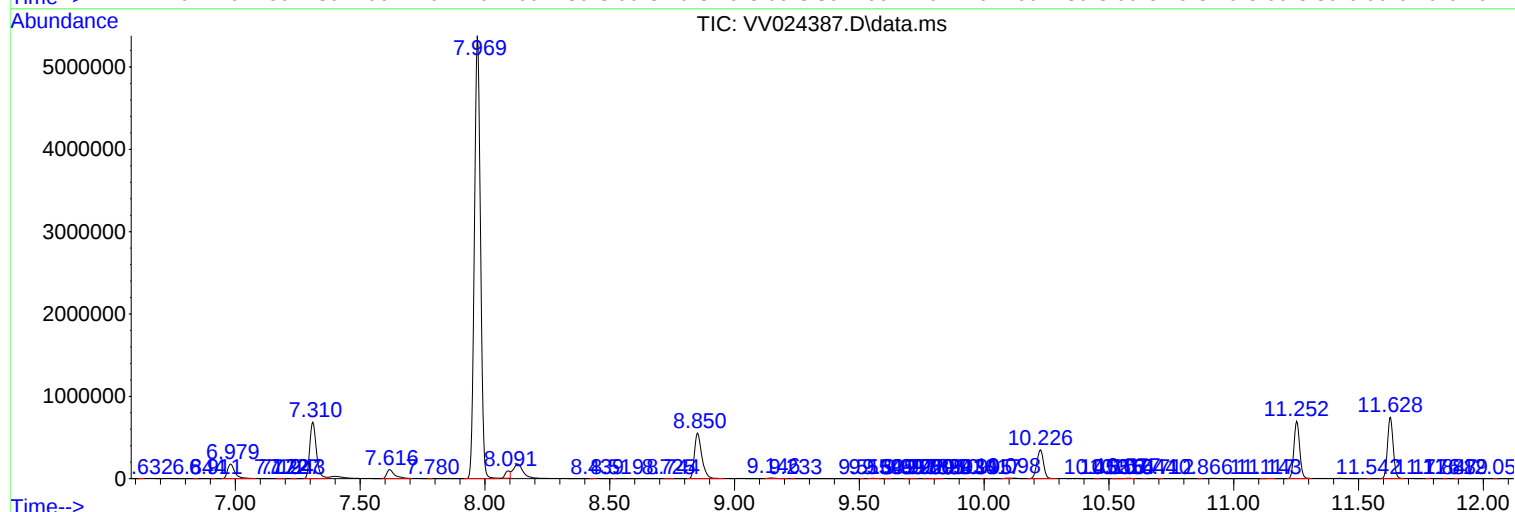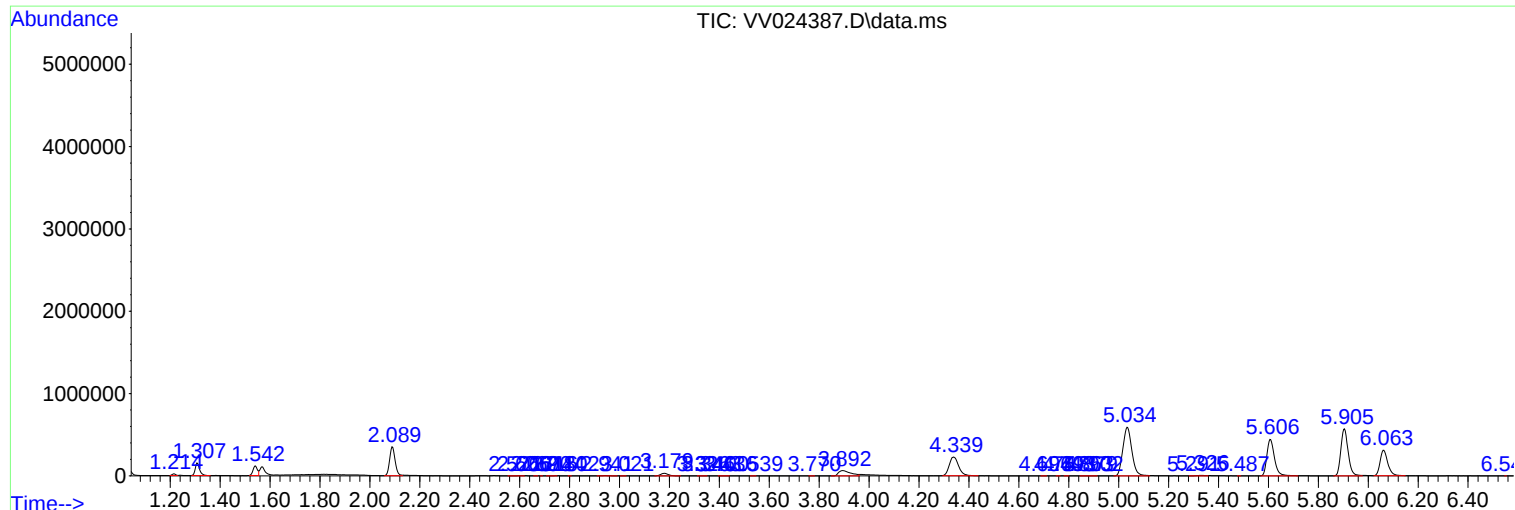

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
Data File : VV024387.D
Acq On : 18 Jan 2022 12:36
Operator : SY/MD
Sample : N1114-20ME
Misc : 5.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLR2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
Data File : VV024387.D
Acq On : 18 Jan 2022 12:36
Operator : SY/MD
Sample : N1114-20ME
Misc : 5.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLR2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------