

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
 Data File : VV024392.D
 Acq On : 18 Jan 2022 14:33
 Operator : SY/MD
 Sample : N1115-12ME 5X
 Misc : 6.05g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLS2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

Signal : TIC: VV024392.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	60	rBV2	13096	11801	0.77%	0.101%
2	1.307	76	83	98	rVB	158386	167528	10.97%	1.427%
3	1.568	158	164	176	rVB	125599	136371	8.93%	1.162%
4	2.108	320	332	351	rBV	299548	460515	30.15%	3.923%
5	2.256	375	378	386	rBV4	580	669	0.04%	0.006%
6	2.548	467	469	471	rBV	265	104	0.01%	0.001%
7	2.577	477	478	480	rBV	350	123	0.01%	0.001%
8	2.622	486	492	498	rVB5	540	750	0.05%	0.006%
9	2.841	558	560	564	rBV2	376	235	0.02%	0.002%
10	2.892	572	576	579	rBV2	275	239	0.02%	0.002%
11	2.957	589	596	604	rBV4	2759	4209	0.28%	0.036%
12	3.040	620	622	626	rVB	261	141	0.01%	0.001%
13	3.073	626	632	634	rBV	598	447	0.03%	0.004%
14	3.118	643	646	650	rVB2	289	225	0.01%	0.002%
15	3.143	650	654	657	rBV	293	236	0.02%	0.002%
16	3.195	657	670	685	rBV2	6325	13773	0.90%	0.117%
17	3.246	685	686	689	rBV2	212	123	0.01%	0.001%
18	3.417	736	739	740	rBV2	277	123	0.01%	0.001%
19	3.458	747	752	754	rBV	224	164	0.01%	0.001%
20	3.507	765	767	770	rVB2	524	305	0.02%	0.003%
21	3.526	770	773	776	rBV	350	256	0.02%	0.002%
22	3.561	780	784	785	rBV	199	136	0.01%	0.001%
23	3.590	790	793	794	rVB	347	132	0.01%	0.001%
24	3.648	807	811	813	rVB	261	168	0.01%	0.001%
25	3.661	813	815	818	rBV2	261	140	0.01%	0.001%
26	3.741	835	840	844	rBV2	347	306	0.02%	0.003%
27	3.764	844	847	850	rBV2	254	171	0.01%	0.001%
28	3.815	860	863	866	rVB2	205	112	0.01%	0.001%
29	3.886	874	885	917	rBV	82361	254472	16.66%	2.168%
30	4.349	1013	1029	1062	rBV	221483	549104	35.95%	4.678%
31	4.667	1125	1128	1131	rBV	368	312	0.02%	0.003%
32	4.851	1183	1185	1187	rBV	388	196	0.01%	0.002%
33	4.886	1193	1196	1198	rBV	211	120	0.01%	0.001%
34	4.928	1204	1209	1212	rBV4	499	498	0.03%	0.004%
35	4.966	1216	1221	1225	rBV3	467	415	0.03%	0.004%
36	5.047	1228	1246	1272	rBV2	515454	1335579	87.44%	11.378%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011822\
 Data File : VW024392.D
 Acq On : 18 Jan 2022 14:33
 Operator : SY/MD
 Sample : N1115-12ME 5X
 Misc : 6.05g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLS2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

37	5.288	1318	1321	1324	rBV2	412	357	0.02%	0.003%
38	5.439	1365	1368	1370	rBV2	507	305	0.02%	0.003%
39	5.616	1411	1423	1459	rBV	362955	731424	47.89%	6.231%
40	5.915	1502	1516	1540	rBV3	110519	244285	15.99%	2.081%
41	6.069	1551	1564	1594	rVB	291706	600619	39.32%	5.117%
42	6.426	1673	1675	1678	rBV	547	272	0.02%	0.002%
43	6.442	1678	1680	1684	rBV	270	191	0.01%	0.002%
44	6.461	1684	1686	1687	rBV	362	132	0.01%	0.001%
45	6.523	1699	1705	1707	rBV3	722	690	0.05%	0.006%
46	6.561	1715	1717	1720	rBV3	281	178	0.01%	0.002%
47	6.600	1727	1729	1731	rBV	301	114	0.01%	0.001%
48	6.645	1735	1743	1744	rBV4	1156	1213	0.08%	0.010%
49	6.706	1760	1762	1764	rBV2	387	192	0.01%	0.002%
50	6.834	1798	1802	1804	rVB2	354	205	0.01%	0.002%
51	6.986	1838	1849	1876	rBV2	169052	314029	20.56%	2.675%
52	7.243	1927	1929	1934	rVB3	462	362	0.02%	0.003%
53	7.269	1934	1937	1939	rBV2	230	137	0.01%	0.001%
54	7.314	1939	1951	1970	rBV	642013	1122134	73.47%	9.560%
55	7.619	2034	2046	2068	rBV	119564	211519	13.85%	1.802%
56	7.973	2143	2156	2179	rBV	908902	1527411	100.00%	13.012%
57	8.092	2183	2193	2227	rVV	263989	585282	38.32%	4.986%
58	8.387	2283	2285	2289	rBV	382	320	0.02%	0.003%
59	8.558	2336	2338	2341	rVB2	520	258	0.02%	0.002%
60	8.571	2341	2342	2346	rBV2	340	213	0.01%	0.002%
61	8.593	2346	2349	2352	rBV	293	238	0.02%	0.002%
62	8.661	2365	2370	2375	rBV3	505	565	0.04%	0.005%
63	8.767	2398	2403	2405	rBV2	349	248	0.02%	0.002%
64	8.799	2412	2413	2415	rBV2	327	149	0.01%	0.001%
65	8.850	2418	2429	2461	rVV	529929	872840	57.15%	7.436%
66	9.146	2515	2521	2522	rBV3	1801	1449	0.09%	0.012%
67	9.330	2575	2578	2580	rBV	457	174	0.01%	0.001%
68	9.407	2599	2602	2604	rBV2	167	136	0.01%	0.001%
69	9.448	2609	2615	2617	rBV2	273	309	0.02%	0.003%
70	9.481	2623	2625	2629	rBV2	280	224	0.01%	0.002%
71	9.657	2674	2680	2683	rBV2	413	525	0.03%	0.004%
72	9.731	2700	2703	2706	rBV2	218	137	0.01%	0.001%
73	9.805	2723	2726	2727	rBV	337	214	0.01%	0.002%
74	9.957	2771	2773	2774	rBV2	269	127	0.01%	0.001%
75	10.095	2811	2816	2818	rBV2	682	641	0.04%	0.005%
76	10.127	2818	2826	2837	rVB5	3325	5538	0.36%	0.047%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
 Data File : VV024392.D
 Acq On : 18 Jan 2022 14:33
 Operator : SY/MD
 Sample : N1115-12ME 5X
 Misc : 6.05g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLS2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

77	10.217	2842	2854	2874	rBV	377390	606722	39.72%	5.169%
78	10.368	2898	2901	2905	rBV3	745	474	0.03%	0.004%
79	10.641	2983	2986	2988	rBV	340	248	0.02%	0.002%
80	10.657	2988	2991	2996	rVB2	755	690	0.05%	0.006%
81	10.680	2996	2998	2999	rBV	336	150	0.01%	0.001%
82	10.792	3031	3033	3037	rVB2	425	245	0.02%	0.002%
83	10.918	3064	3072	3082	rBV5	3393	4932	0.32%	0.042%
84	11.027	3103	3106	3110	rBV5	627	493	0.03%	0.004%
85	11.098	3126	3128	3130	rBV	293	109	0.01%	0.001%
86	11.146	3137	3143	3150	rBV3	1598	2098	0.14%	0.018%
87	11.207	3160	3162	3163	rBV3	362	112	0.01%	0.001%
88	11.249	3163	3175	3193	rBV	569968	874400	57.25%	7.449%
89	11.622	3279	3291	3315	rBV	678898	1079331	70.66%	9.195%
90	11.989	3403	3405	3408	rVB	447	182	0.01%	0.002%
91	12.024	3409	3416	3419	rBV3	473	552	0.04%	0.005%
92	12.046	3421	3423	3426	rBV2	356	159	0.01%	0.001%
93	12.120	3444	3446	3452	rVB3	398	282	0.02%	0.002%
94	12.265	3488	3491	3493	rBV2	456	317	0.02%	0.003%
95	12.323	3506	3509	3511	rBV2	464	295	0.02%	0.003%
96	12.648	3608	3610	3613	rBV	283	151	0.01%	0.001%
97	12.735	3635	3637	3642	rBV3	451	399	0.03%	0.003%
98	12.776	3649	3650	3655	rBV	285	155	0.01%	0.001%
99	12.847	3670	3672	3674	rBV	415	123	0.01%	0.001%
100	12.924	3694	3696	3699	rVB	428	188	0.01%	0.002%

Sum of corrected areas: 11738361




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
Data File : VV024392.D
Acq On : 18 Jan 2022 14:33
Operator : SY/MD
Sample : N1115-12ME 5X
Misc : 6.05g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLS2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

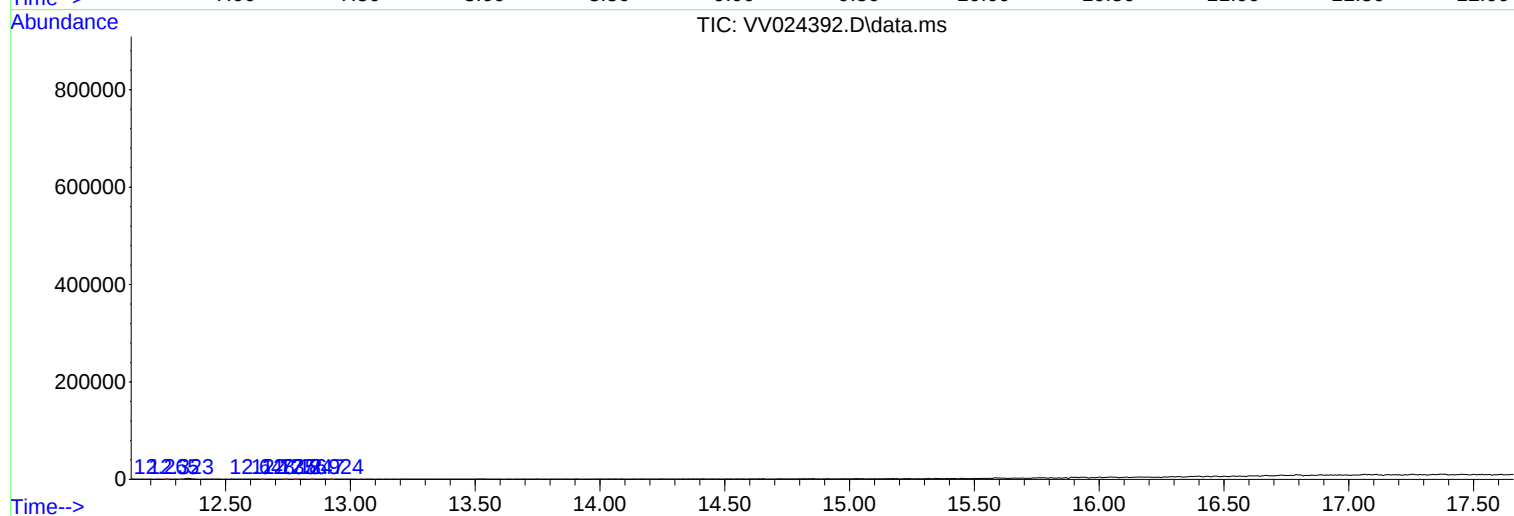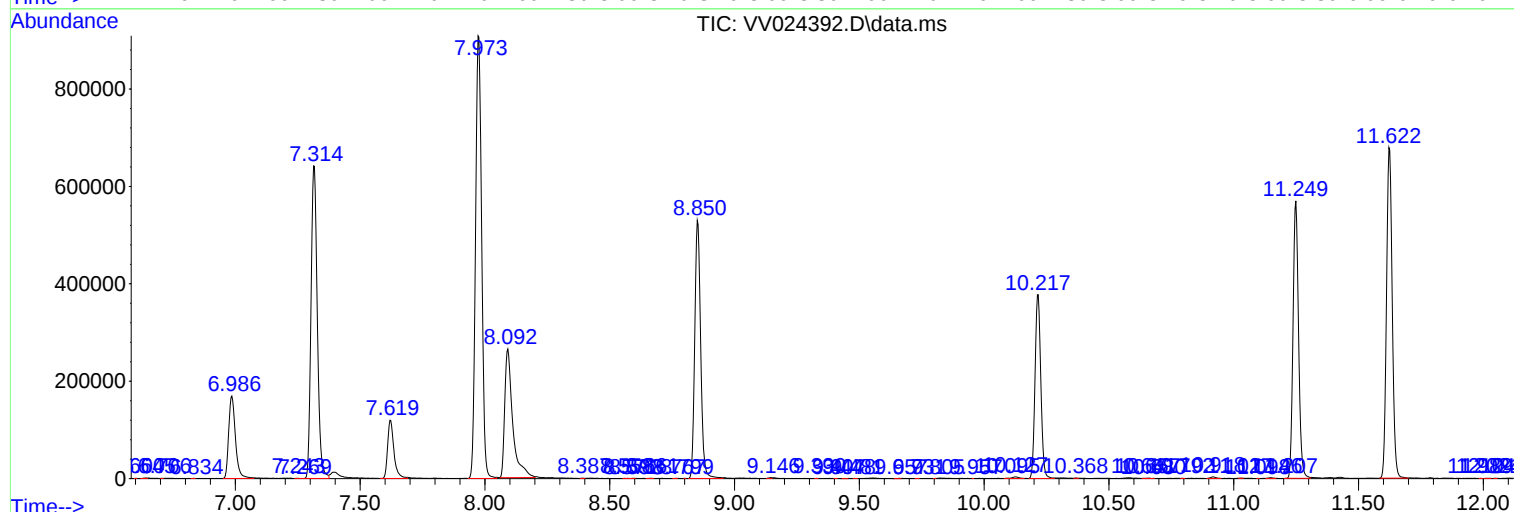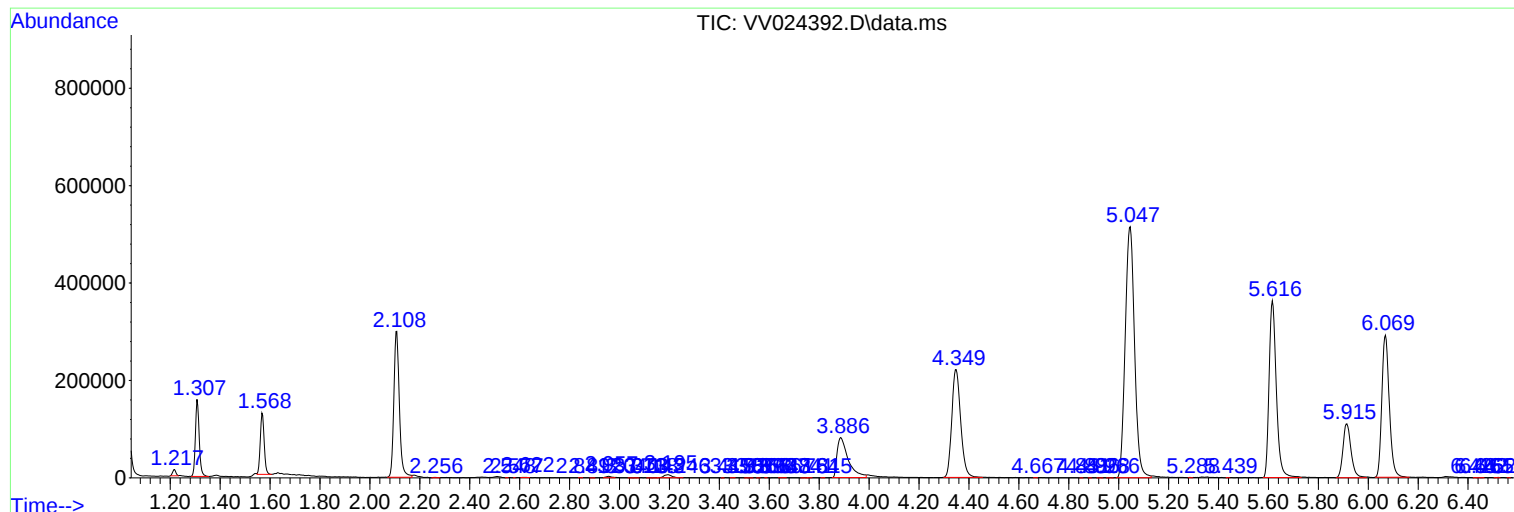

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
Data File : VV024392.D
Acq On : 18 Jan 2022 14:33
Operator : SY/MD
Sample : N1115-12ME 5X
Misc : 6.05g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLS2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
Data File : VV024392.D
Acq On : 18 Jan 2022 14:33
Operator : SY/MD
Sample : N1115-12ME 5X
Misc : 6.05g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLS2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------