


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011822\
 Data File : VV024383.D
 Acq On : 18 Jan 2022 09:36
 Operator : SY/MD
 Sample : BFB257
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB257

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis
 Last Update : Fri Jan 21 00:04:44 2022

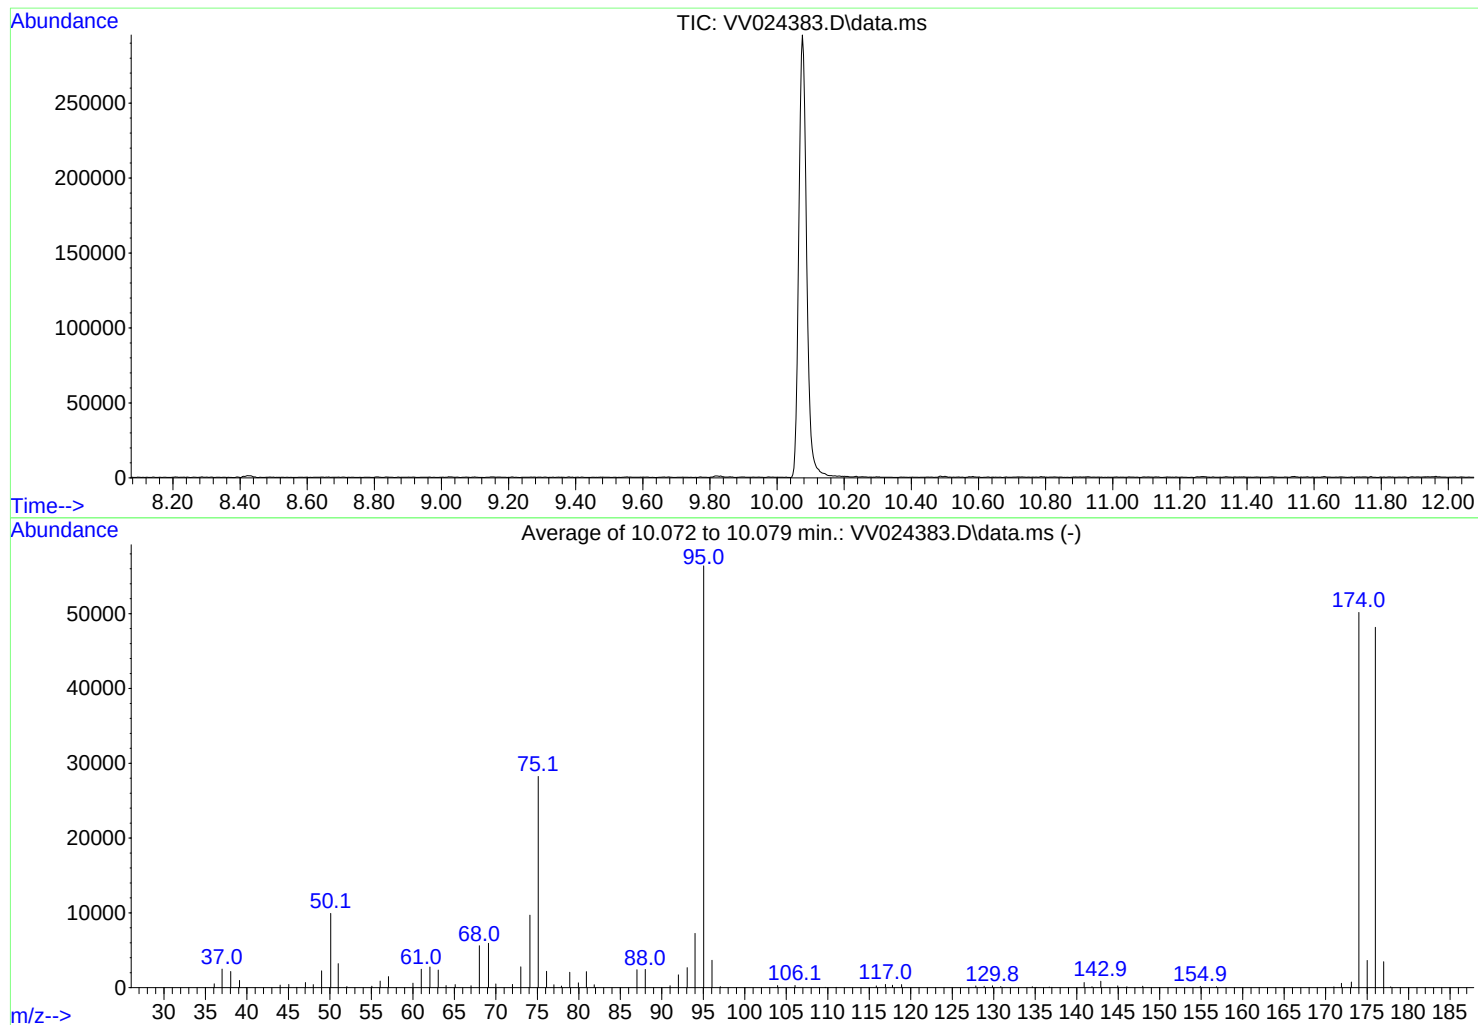

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	9936	PASS
75	95	30	80	50.1	28245	PASS
95	95	100	100	100.0	56389	PASS
96	95	5	9	6.5	3662	PASS
173	174	0.00	2	1.5	760	PASS
174	95	50	120	89.0	50160	PASS
175	174	5	9	7.2	3635	PASS
176	174	95	105	96.0	48168	PASS
177	176	5	10	7.2	3475	PASS

m/z	Abundance
39.90	148.0
44.00	198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

m/z	Abundance
36.10	592.0
37.00	2708.0
38.00	2096.0
39.10	1052.0
40.00	137.0
44.00	532.0
45.10	427.0
47.10	764.0
48.00	451.0
49.00	2282.0
50.10	10184.0
51.00	3343.0
52.10	162.0
55.00	179.0
56.10	927.0
57.10	1440.0
60.00	574.0
61.00	2450.0
62.10	2767.0
63.00	2366.0
64.00	283.0
65.10	417.0
67.00	285.0
68.00	5376.0
69.10	6047.0
70.00	402.0
72.00	442.0
73.00	2785.0
74.10	9858.0
75.10	27992.0
76.10	2306.0
77.00	383.0
77.90	223.0
78.90	2026.0
80.00	639.0
80.90	2099.0
81.90	409.0
87.00	2377.0
88.00	2403.0
91.00	242.0
92.00	1766.0
93.10	2567.0
94.00	7239.0
95.00	55456.0
96.00	3625.0
97.10	157.0
103.90	325.0
106.00	320.0
115.90	243.0
116.90	428.0
117.80	342.0
118.90	381.0
127.90	227.0
128.80	197.0
129.80	256.0
130.80	126.0
134.60	122.0
137.00	146.0
140.90	682.0
141.80	134.0
142.90	868.0
144.90	220.0
146.10	145.0
147.90	173.0
154.90	212.0
156.90	122.0
171.00	167.0
171.90	598.0
173.10	667.0
174.00	47976.0
175.00	3546.0
176.00	46520.0
177.00	3550.0
177.80	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

m/z	Abundance
36.00	517.0
37.00	2570.0
38.10	2221.0
39.10	976.0
39.90	170.0
44.00	560.0
45.10	449.0
47.10	688.0
48.00	432.0
49.00	2341.0
50.10	10225.0
51.00	3279.0
52.00	154.0
55.10	196.0
56.10	892.0
57.00	1501.0
60.00	595.0
61.00	2498.0
62.10	2809.0
63.00	2449.0
64.00	287.0
65.10	447.0
67.00	288.0
68.00	5724.0
69.10	6089.0
70.00	518.0
72.00	448.0
73.00	2897.0
74.10	10084.0
75.10	29088.0
76.10	2246.0
77.00	403.0
77.90	213.0
78.90	2139.0
80.00	651.0
80.90	2209.0
81.90	379.0
87.00	2497.0
88.00	2546.0
91.00	262.0
92.00	1800.0
93.00	2785.0
94.00	7562.0
95.10	58112.0
96.10	3687.0
97.10	132.0
104.00	280.0
106.00	292.0
109.70	108.0
115.90	248.0
117.00	442.0
117.80	344.0
118.90	419.0
127.80	252.0
128.80	188.0
129.80	252.0
130.90	176.0
134.70	153.0
135.10	111.0
136.70	134.0
140.90	705.0
141.90	152.0
142.90	889.0
145.00	230.0
146.10	143.0
147.90	203.0
154.90	177.0
156.80	152.0
171.00	140.0
171.90	599.0
173.10	776.0
174.00	51696.0
175.00	3734.0
176.00	49664.0
177.00	3629.0
177.90	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

m/z	Abundance
36.00	460.0
37.00	2199.0
38.10	2144.0
39.10	841.0
39.90	198.0
44.00	542.0
45.00	421.0
46.00	138.0
47.00	596.0
48.00	369.0
49.00	2119.0
50.10	9399.0
51.00	3028.0
52.00	131.0
55.10	182.0
56.00	795.0
57.00	1468.0
60.00	614.0
61.00	2408.0
62.00	2736.0
63.10	2260.0
64.00	287.0
65.10	382.0
67.00	235.0
68.00	5708.0
69.10	5671.0
70.00	567.0
72.00	406.0
73.00	2666.0
74.10	9104.0
75.10	27656.0
76.10	2017.0
77.00	365.0
77.90	203.0
78.90	1980.0
79.90	606.0
80.90	2123.0
81.80	373.0
87.00	2300.0
88.00	2366.0
91.00	244.0
92.00	1596.0
93.00	2649.0
94.00	6953.0
95.00	55600.0
96.10	3674.0
97.00	113.0
104.00	245.0
106.10	299.0
111.00	113.0
115.80	236.0
117.00	416.0
117.80	301.0
118.90	437.0
127.80	249.0
128.90	167.0
129.90	258.0
130.90	153.0
134.70	136.0
136.70	117.0
140.90	697.0
141.90	124.0
142.90	831.0
145.00	238.0
146.00	115.0
148.00	201.0
154.90	143.0
156.80	139.0
171.90	525.0
173.10	838.0
174.00	50808.0
175.00	3625.0
176.00	48320.0
177.00	3246.0
177.90	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257