


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011922\
Data File : VV024404.D
Acq On : 19 Jan 2022 10:46
Operator : SY/MD
Sample : VV0119WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK304

Manual IntegrationsAPPROVED

Quant Time: Jan 20 01:02:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 20 01:01:42 2022
Response via : Initial Calibration

Reviewed By :John Carlone 01/20/2022
Supervised By :Mahesh Dadoda 01/20/2022

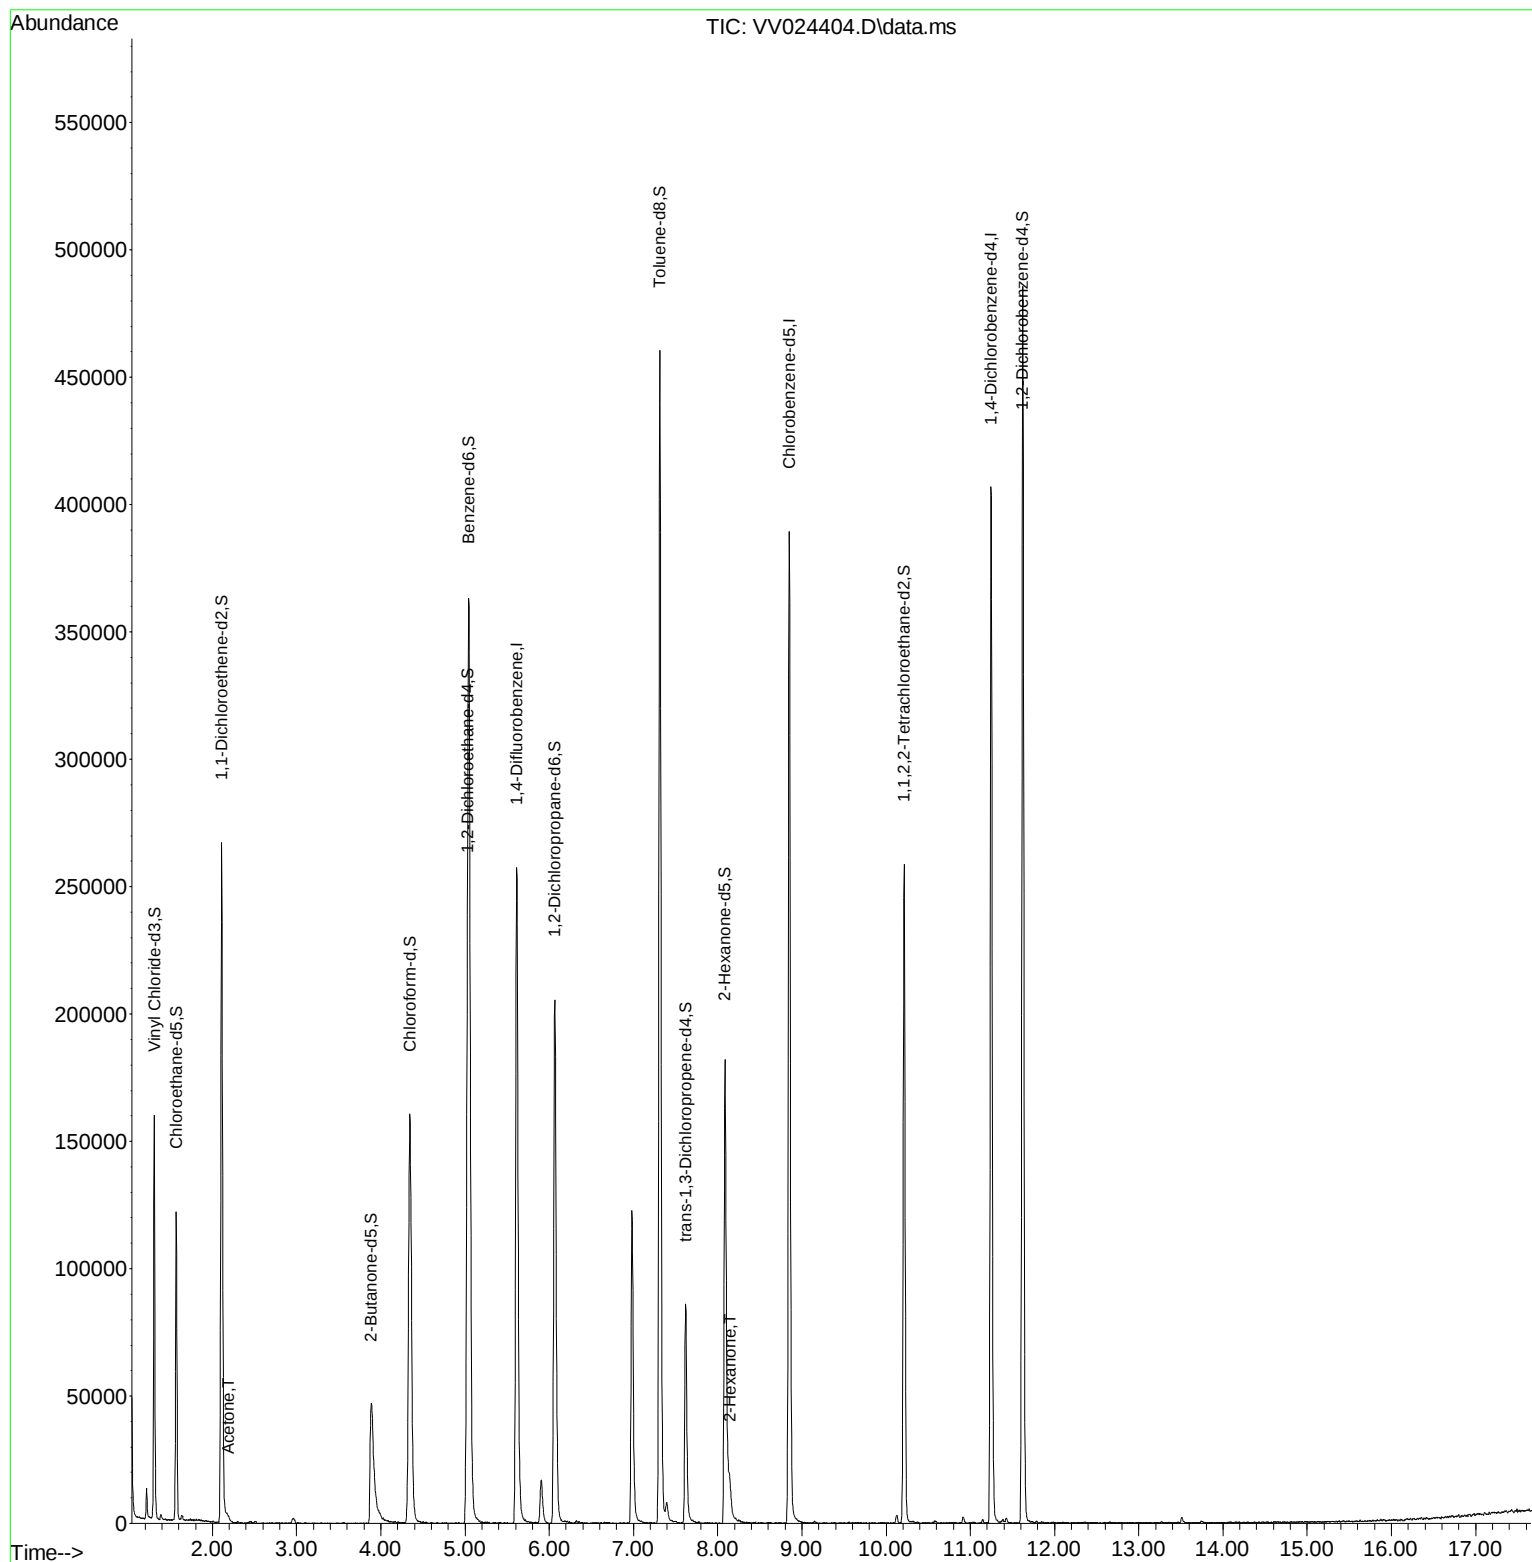




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011922\
 Data File : VV024404.D
 Acq On : 19 Jan 2022 10:46
 Operator : SY/MD
 Sample : VV0119WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK304

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/20/2022
 Supervised By :Mahesh Dadoda 01/20/2022

Quant Time: Jan 20 01:02:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 20 01:01:42 2022
 Response via : Initial Calibration

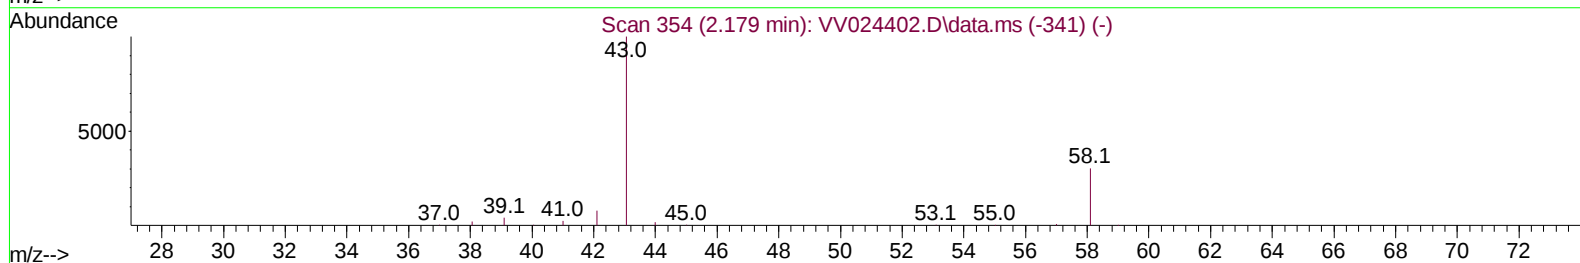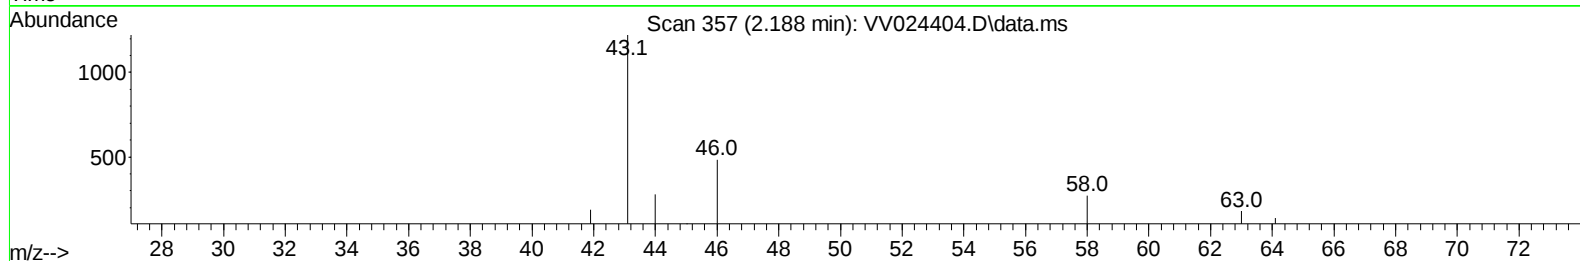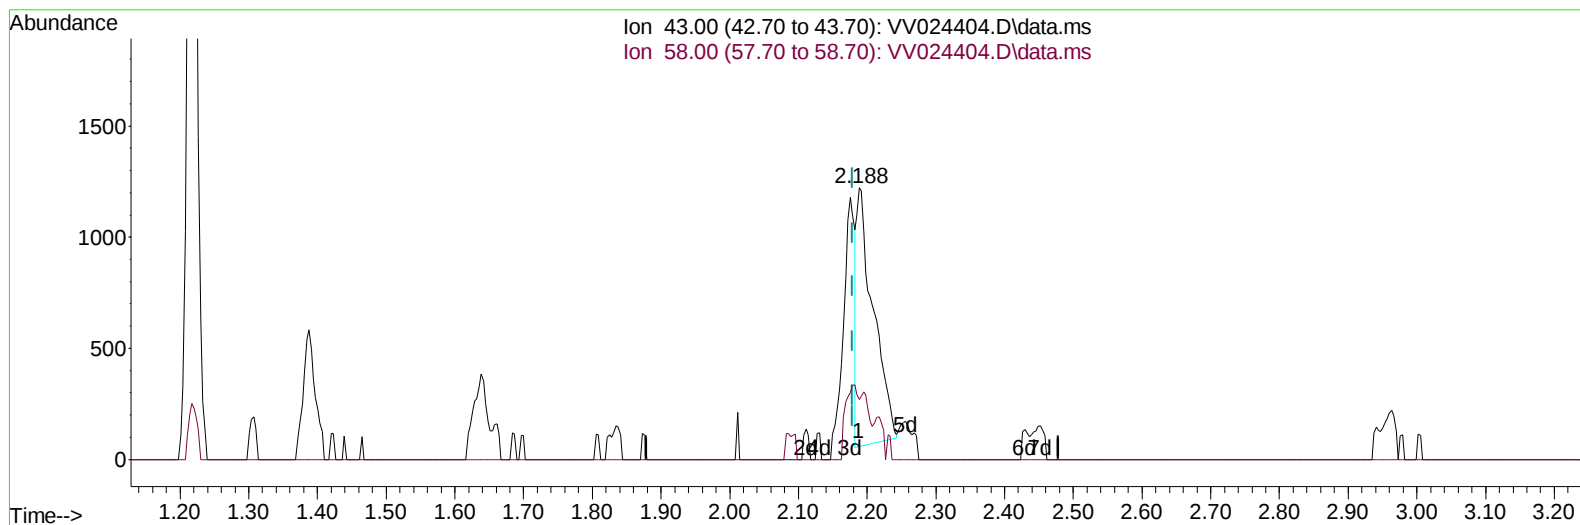

TIC: VV024404.D\data.ms

(13) Acetone (T)

2.188min (+ 0.010) 2.17 ug/L

response 1961

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.50	22.28
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011922\
 Data File : VV024404.D
 Acq On : 19 Jan 2022 10:46
 Operator : SY/MD
 Sample : VV0119WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK304

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/20/2022
 Supervised By :Mahesh Dadoda 01/20/2022

Quant Time: Jan 20 01:02:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 20 01:01:42 2022
 Response via : Initial Calibration

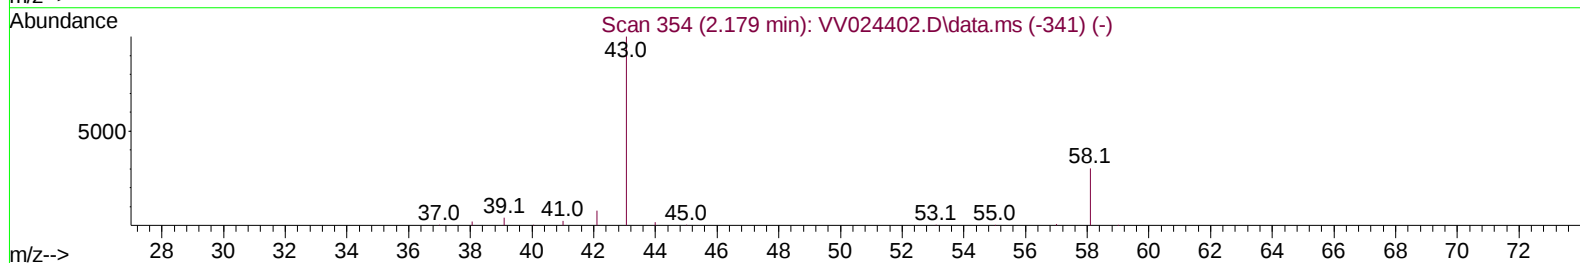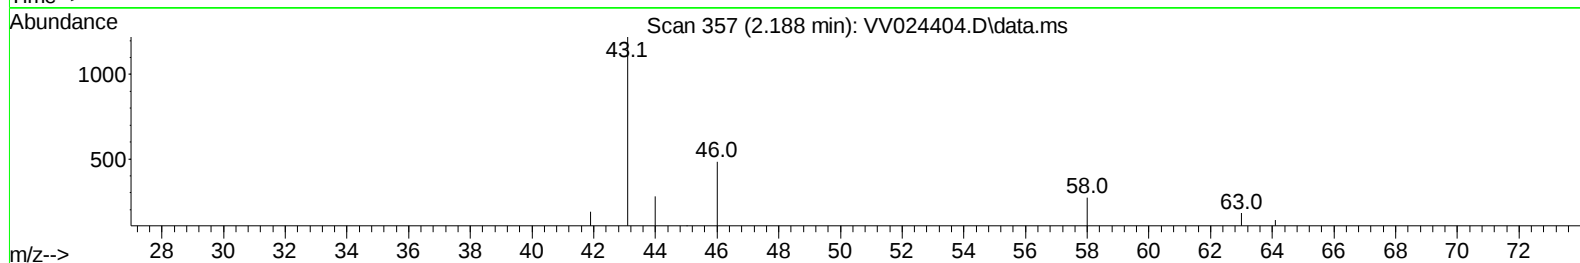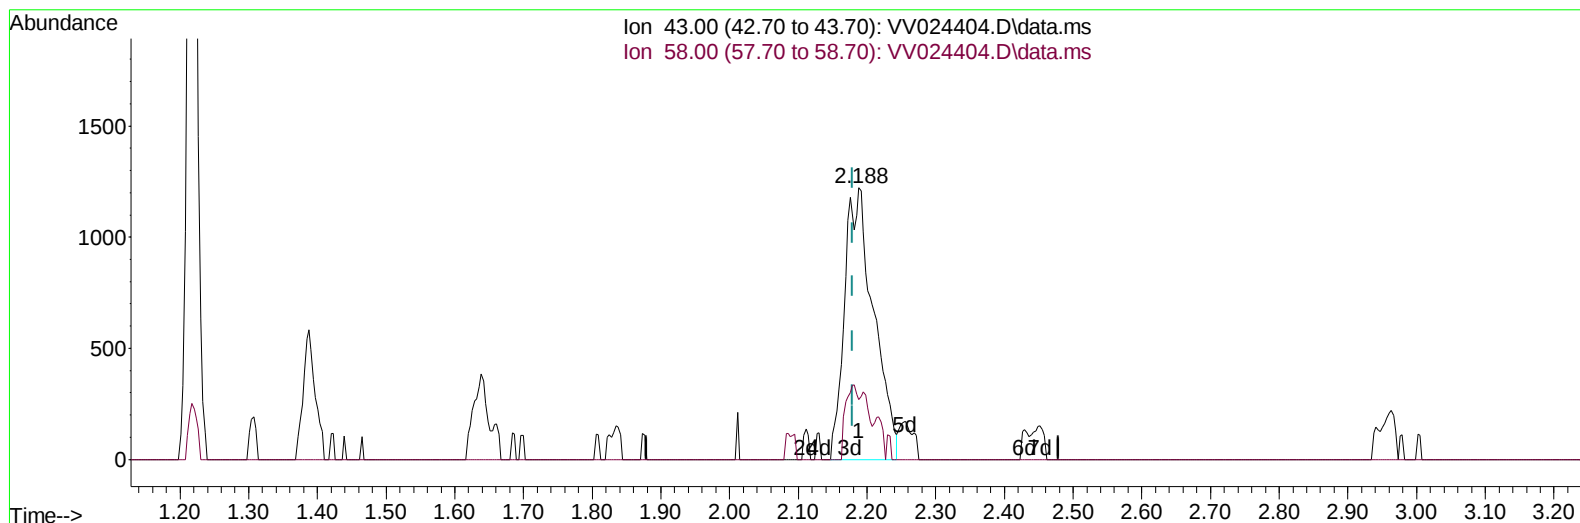

TIC: VV024404.D\data.ms

(13) Acetone (T)

2.188min (+ 0.010) 3.98 ug/L m

response 3591

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.50	12.17
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011922\
 Data File : VV024404.D
 Acq On : 19 Jan 2022 10:46
 Operator : SY/MD
 Sample : VV0119WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK304

Manual IntegrationsAPPROVED

Quant Time: Jan 20 01:02:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 20 01:01:42 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 01/20/2022
 Supervised By : Mahesh Dadoda 01/20/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	228079	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	213942	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	112399	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	96157	58.580	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	117.160%	
7) Chloroethane-d5	1.571	69	72253	57.944	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	115.880%	
11) 1,1-Dichloroethene-d2	2.108	63	134088	43.708	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	87.420%	
21) 2-Butanone-d5	3.886	46	90506	98.965	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	98.960%	
24) Chloroform-d	4.346	84	162471	54.157	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	108.320%	
26) 1,2-Dichloroethane-d4	5.027	65	109975	54.753	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	109.500%	
32) Benzene-d6	5.047	84	318467	57.043	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	114.080%	
36) 1,2-Dichloropropane-d6	6.066	67	90104	57.587	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	115.180%	
41) Toluene-d8	7.313	98	306908	56.777	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	113.560%	
43) trans-1,3-Dichloroprop...	7.619	79	47834	53.092	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	106.180%	
47) 2-Hexanone-d5	8.085	63	60791	89.428	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	89.430%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	108575	48.558	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	97.120%	
66) 1,2-Dichlorobenzene-d4	11.622	152	127910	57.093	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	114.180%	
Target Compounds						
13) Acetone	2.188	43	3591m	3.977	ug/L	
48) 2-Hexanone	8.149	43	9385	7.003	ug/L #	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed