


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012122\
 Data File : VV024419.D
 Acq On : 21 Jan 2022 09:03
 Operator : SY/MD
 Sample : BFB260
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB260

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012122WMA.M
 Title : VOC Analysis
 Last Update : Mon Jan 24 03:05:41 2022

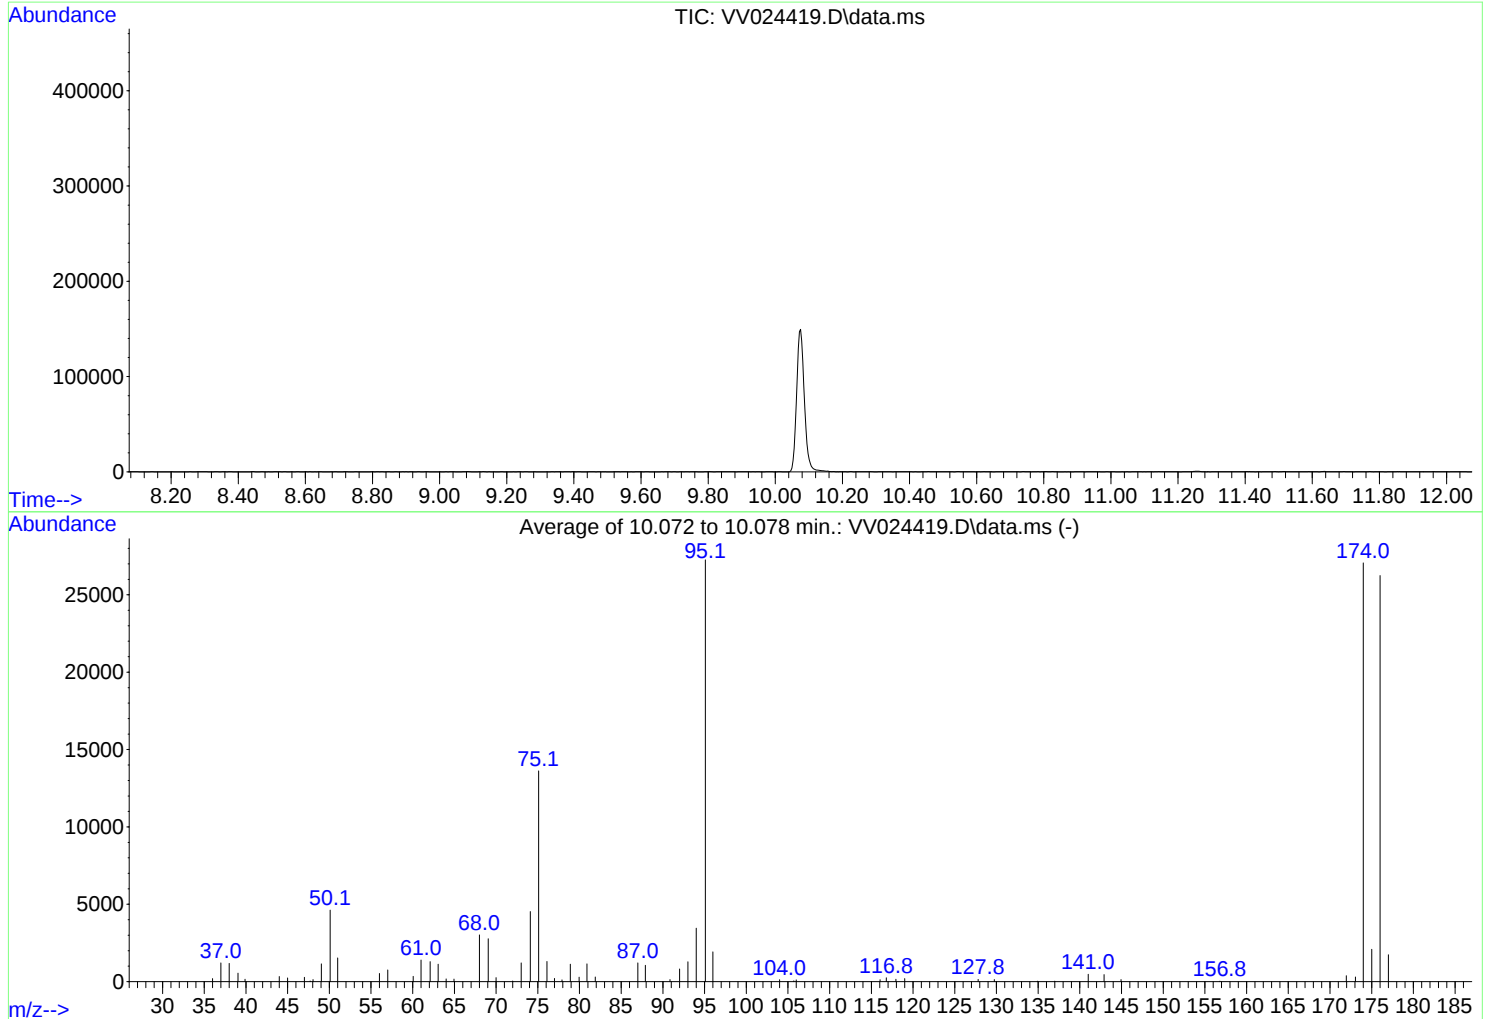

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	4626	PASS
75	95	30	80	50.0	13623	PASS
95	95	100	100	100.0	27259	PASS
96	95	5	9	7.1	1922	PASS
173	174	0.00	2	1.1	297	PASS
174	95	50	120	99.3	27061	PASS
175	174	5	9	7.7	2094	PASS
176	174	95	105	97.0	26248	PASS
177	176	5	10	6.6	1734	PASS

m/z Abundance

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
36.00	190.0
37.00	1272.0
38.00	1211.0
39.00	580.0
39.80	172.0
44.00	373.0
45.00	233.0
46.90	270.0
48.10	163.0
49.00	1076.0
50.10	4760.0
51.00	1538.0
56.00	546.0
57.00	823.0
60.00	370.0
61.00	1504.0
62.10	1241.0
63.10	1199.0
64.00	175.0
64.90	146.0
68.00	2943.0
69.00	2702.0
70.00	287.0
72.00	116.0
73.00	1190.0
74.10	4688.0
75.10	13895.0
76.10	1415.0
77.00	191.0
77.90	121.0
78.90	1092.0
80.00	300.0
80.90	1142.0
81.90	303.0
87.00	1244.0
87.90	1210.0
91.00	127.0
92.00	820.0
93.00	1377.0
94.00	3581.0
95.10	27632.0
96.00	2045.0
104.00	112.0
105.70	155.0
106.00	104.0
116.10	112.0
116.80	231.0
117.90	162.0
119.00	181.0
127.80	120.0
129.80	123.0
134.90	107.0
141.00	487.0
142.90	444.0
145.00	128.0
172.00	381.0
173.00	453.0
174.00	27144.0
175.00	2086.0
176.00	26432.0
177.00	1857.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
36.00	205.0
37.00	1261.0
38.00	1218.0
39.10	578.0
39.90	151.0
44.00	334.0
45.00	250.0
47.00	249.0
47.70	136.0
48.10	140.0
49.00	1201.0
50.10	4774.0
51.00	1569.0
56.00	570.0
57.00	791.0
60.00	355.0
61.00	1466.0
62.10	1376.0
63.10	1153.0
64.00	184.0
64.90	169.0
68.00	3120.0
69.10	2852.0
70.00	254.0
73.00	1256.0
74.10	4602.0
75.10	14009.0
76.10	1337.0
77.00	216.0
77.90	118.0
78.90	1159.0
80.00	297.0
80.90	1177.0
81.90	323.0
87.00	1230.0
87.90	1103.0
90.80	132.0
92.00	820.0
93.00	1351.0
94.00	3569.0
95.10	28160.0
96.00	1990.0
104.00	131.0
106.00	135.0
116.00	128.0
116.80	251.0
117.90	164.0
119.00	193.0
127.80	157.0
129.80	142.0
137.00	107.0
141.00	499.0
142.90	465.0
144.90	141.0
172.00	390.0
173.10	439.0
174.00	28080.0
175.00	2184.0
176.00	27040.0
177.00	1770.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
36.00	206.0
37.00	1098.0
38.00	1124.0
39.10	486.0
40.00	137.0
44.00	273.0
45.00	216.0
47.10	306.0
48.00	114.0
49.10	1161.0
50.10	4344.0
51.00	1499.0
56.00	456.0
57.00	647.0
60.10	301.0
61.00	1226.0
62.10	1272.0
63.00	1035.0
64.00	183.0
65.00	182.0
68.00	2982.0
69.10	2765.0
70.00	237.0
73.00	1184.0
74.10	4294.0
75.10	12966.0
76.10	1157.0
77.00	219.0
77.90	109.0
78.90	1119.0
79.90	270.0
80.90	1137.0
81.90	275.0
87.00	1162.0
87.90	864.0
90.80	140.0
92.00	825.0
93.00	1119.0
94.00	3212.0
95.10	25984.0
96.00	1731.0
104.00	116.0
106.00	118.0
116.00	140.0
116.80	263.0
118.00	147.0
119.00	216.0
127.80	158.0
129.70	124.0
141.00	438.0
142.90	448.0
144.90	130.0
156.80	101.0
171.90	375.0
174.00	25960.0
175.00	2013.0
176.00	25272.0
177.00	1576.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260