

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024483.D
 Acq On : 28 Jan 2022 13:18
 Operator : SY/MD
 Sample : N1318-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jan 29 02:25:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jan 29 02:05:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	131438	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	143552	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	71721	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	46515	4.040	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.800%
7) Chloroethane-d5	1.568	69	46534	4.633	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.600%
11) 1,1-Dichloroethene-d2	2.108	63	73877	3.357	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.200%
20) 2-Butanone-d5	3.915	46	64462	35.124	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	70.240%
24) Chloroform-d	4.346	84	107555	4.922	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.400%
26) 1,2-Dichloroethane-d4	5.030	65	52822	5.338	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.800%
32) Benzene-d6	5.047	84	196870	4.592	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.800%
36) 1,2-Dichloropropane-d6	6.066	67	65210	4.830	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.600%
41) Toluene-d8	7.313	98	159106	4.045	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.800%
43) trans-1,3-Dichloroprop...	7.622	79	19637	4.236	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.800%
46) 2-Hexanone-d5	8.088	63	71588	45.161	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.320%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	39518	4.918	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	61537	5.004	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.000%
Target Compounds					Qvalue	
25) Chloroform	4.371	83	5162	0.257	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024483.D
Acq On : 28 Jan 2022 13:18
Operator : SY/MD
Sample : N1318-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Jan 29 02:25:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jan 29 02:05:31 2022
Response via : Initial Calibration

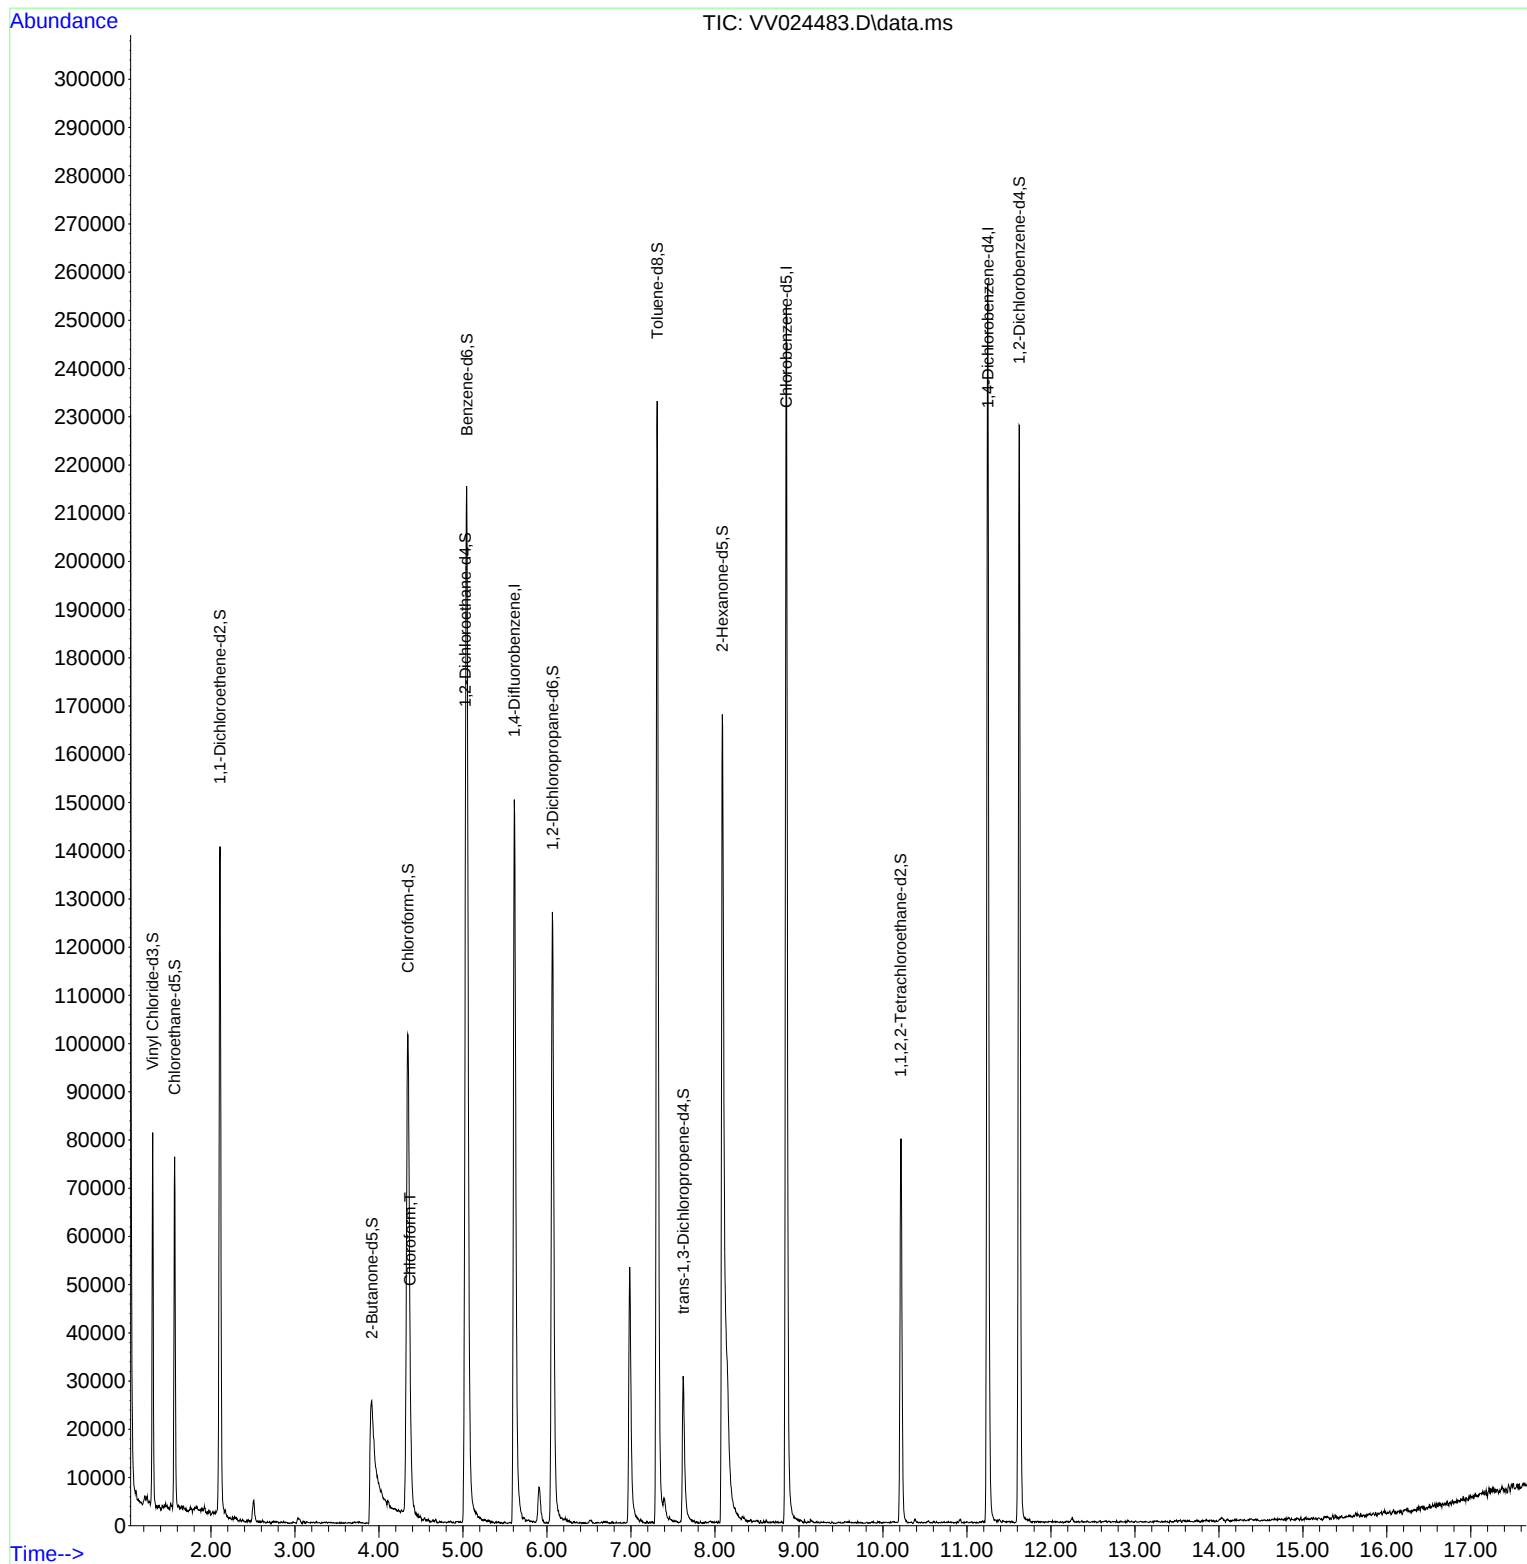

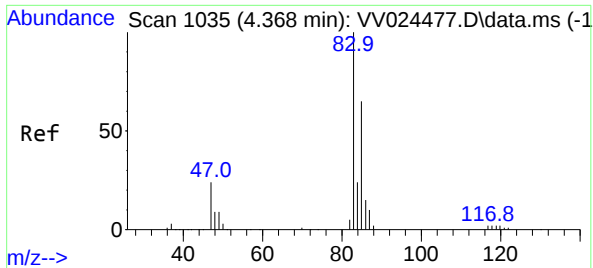

#25
Chloroform
Concen: 0.257 ug/L
RT: 4.371 min Scan# 10
Delta R.T. 0.003 min
Lab File: VV024483.D
Acq: 28 Jan 2022 13:18

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 83 Resp: 5162
Ion Ratio Lower Upper
83 100
85 67.8 45.2 84.0

