

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024480.D
 Acq On : 28 Jan 2022 11:52
 Operator : SY/MD
 Sample : N1317-01DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	34	rVB3	11605	12681	2.26%	0.246%
2	1.204	46	51	59	rVB	14163	13655	2.43%	0.265%
3	1.307	74	83	91	rBV	75353	81102	14.45%	1.571%
4	1.568	157	164	177	rBV	74816	88255	15.72%	1.710%
5	2.108	321	332	347	rBV	137413	203227	36.20%	3.938%
6	2.506	449	456	471	rVB8	3339	6608	1.18%	0.128%
7	3.902	880	890	942	rBV2	50601	201794	35.95%	3.910%
8	4.349	1010	1029	1056	rBV	101479	263884	47.01%	5.113%
9	5.047	1230	1246	1273	rBV3	222182	561366	100.00%	10.877%
10	5.619	1411	1424	1447	rBV	163609	343112	61.12%	6.648%
11	5.915	1503	1516	1529	rBV7	7006	14013	2.50%	0.272%
12	6.069	1552	1564	1582	rBV	128867	268695	47.86%	5.206%
13	6.548	1710	1713	1722	rVB	9746	7345	1.31%	0.142%
14	6.989	1840	1850	1873	rBV2	54797	106126	18.90%	2.056%
15	7.317	1941	1952	1964	rBV	244682	429324	76.48%	8.319%
16	7.387	1964	1974	1998	rVB	295951	522223	93.03%	10.119%
17	7.625	2039	2048	2069	rBV2	32723	62013	11.05%	1.202%
18	7.940	2135	2146	2159	rBV3	7224	13290	2.37%	0.258%
19	8.095	2183	2194	2232	rBV	205687	479607	85.44%	9.293%
20	8.854	2418	2430	2453	rBV	276147	458987	81.76%	8.893%
21	10.217	2842	2854	2872	rBV	86837	138754	24.72%	2.689%
22	10.381	2894	2905	2917	rVB2	16554	26216	4.67%	0.508%
23	11.249	3164	3175	3194	rBV	291948	457438	81.49%	8.863%
24	11.625	3280	3292	3309	rBV	244248	387049	68.95%	7.500%
25	12.252	3477	3487	3496	rVB2	4951	7445	1.33%	0.144%
26	14.040	4034	4043	4053	rVB2	4194	6785	1.21%	0.131%




Sum of corrected areas: 5160994

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024480.D
Acq On : 28 Jan 2022 11:52
Operator : SY/MD
Sample : N1317-01DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

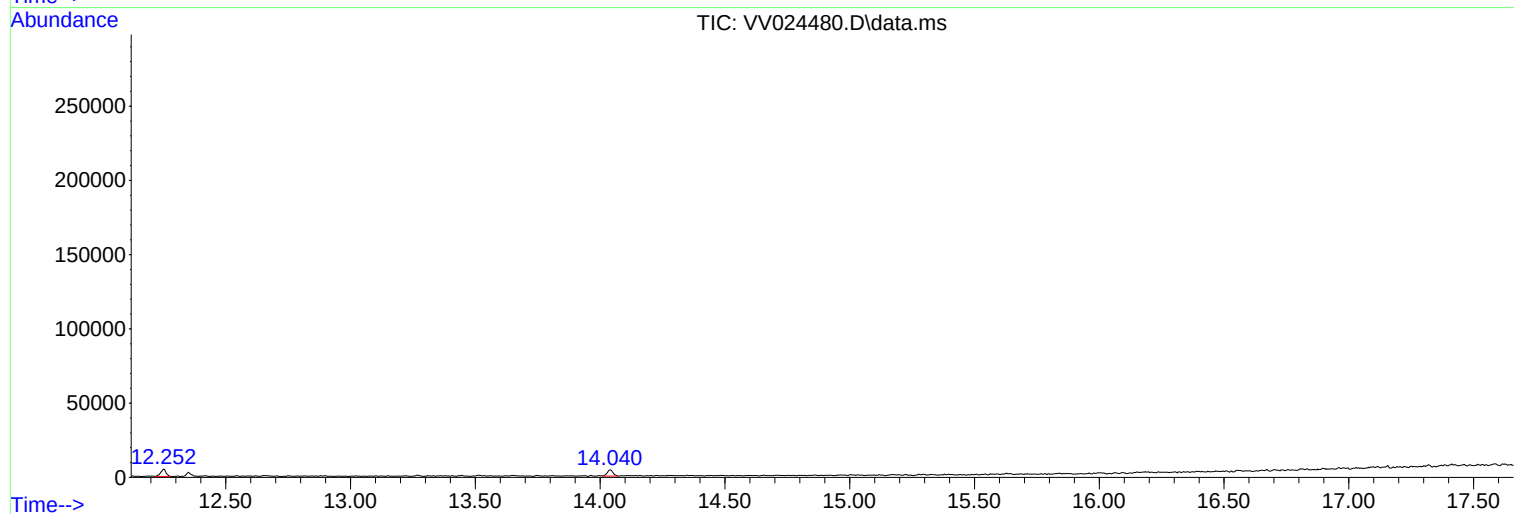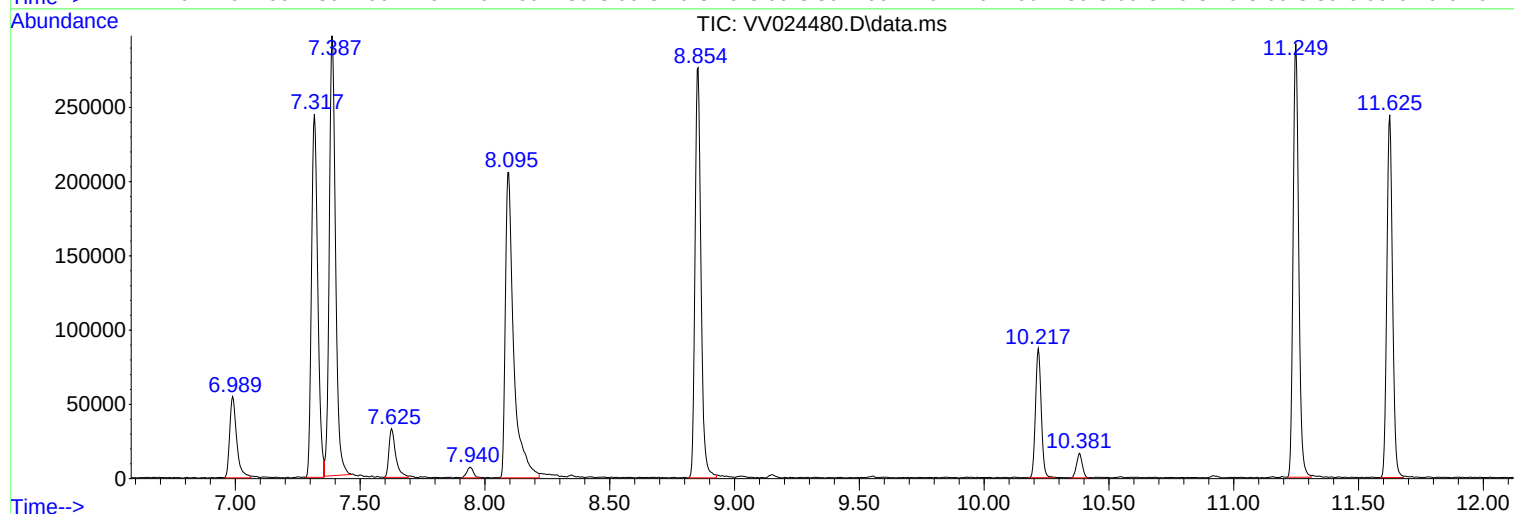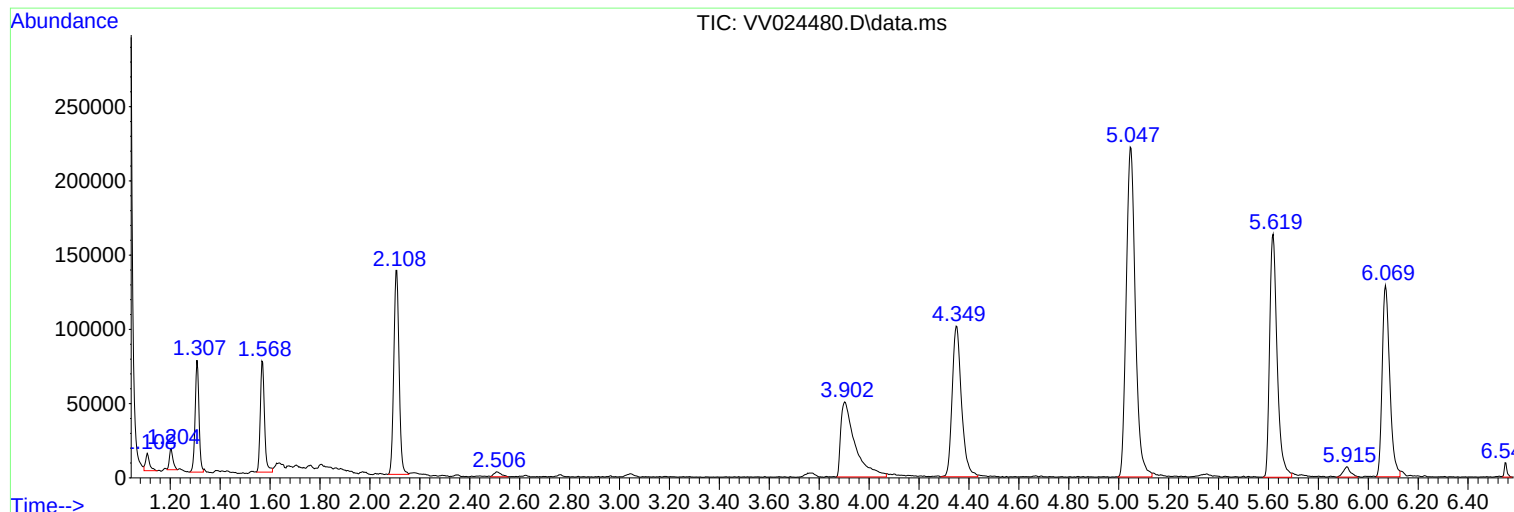

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024480.D
Acq On : 28 Jan 2022 11:52
Operator : SY/MD
Sample : N1317-01DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024480.D
Acq On : 28 Jan 2022 11:52
Operator : SY/MD
Sample : N1317-01DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------