

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024481.D
 Acq On : 28 Jan 2022 12:15
 Operator : SY/MD
 Sample : N1317-03DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024481.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	94	rVB	73809	76567	10.25%	1.441%
2	1.568	157	164	175	rBV	75357	86828	11.63%	1.634%
3	2.108	319	332	345	rBV	140583	208030	27.85%	3.915%
4	2.513	448	458	471	rVB7	4848	8986	1.20%	0.169%
5	3.040	612	622	636	rBV7	5219	12025	1.61%	0.226%
6	3.764	835	847	861	rVB4	5217	12699	1.70%	0.239%
7	3.902	879	890	932	rBV	52032	202471	27.11%	3.810%
8	4.349	1014	1029	1055	rBV	104010	265600	35.56%	4.998%
9	5.050	1230	1247	1283	rBV3	221403	571913	76.57%	10.763%
10	5.619	1412	1424	1449	rBV	158760	327047	43.79%	6.155%
11	5.918	1505	1517	1532	rBV7	5996	13018	1.74%	0.245%
12	6.069	1550	1564	1590	rBV	133029	277701	37.18%	5.226%
13	6.989	1837	1850	1872	rBV	54838	107390	14.38%	2.021%
14	7.317	1941	1952	1964	rBV	250121	437824	58.62%	8.240%
15	7.387	1964	1974	1998	rVB	431968	746890	100.00%	14.056%
16	7.625	2038	2048	2065	rBV2	34277	63715	8.53%	1.199%
17	8.091	2182	2193	2236	rBV	222412	490305	65.65%	9.227%
18	8.854	2417	2430	2462	rBV	261788	441789	59.15%	8.314%
19	10.217	2843	2854	2879	rVB2	85180	137702	18.44%	2.591%
20	11.249	3164	3175	3194	rBV	275417	430266	57.61%	8.097%
21	11.625	3280	3292	3308	rBV	249129	394932	52.88%	7.432%




Sum of corrected areas: 5313698

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024481.D
Acq On : 28 Jan 2022 12:15
Operator : SY/MD
Sample : N1317-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

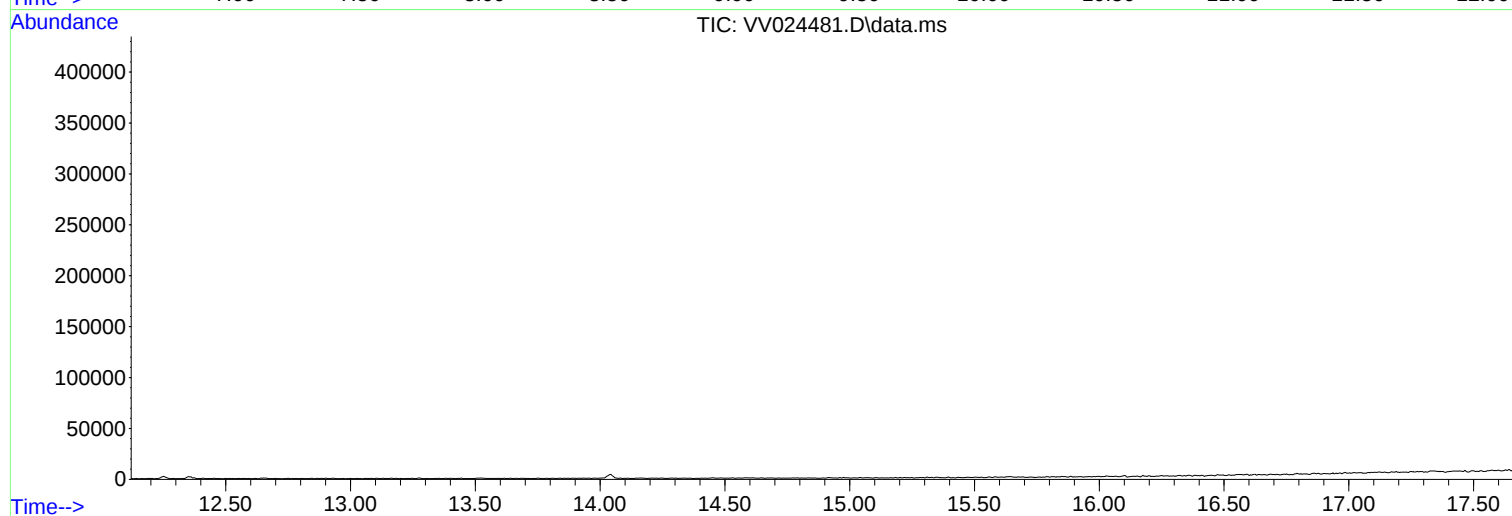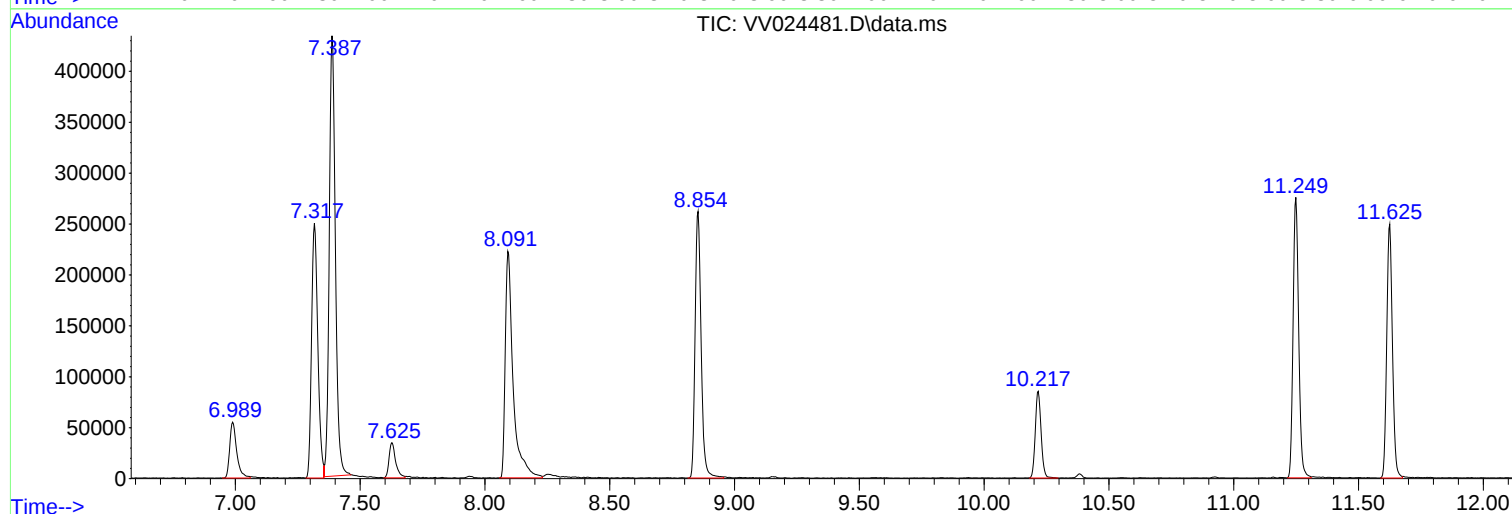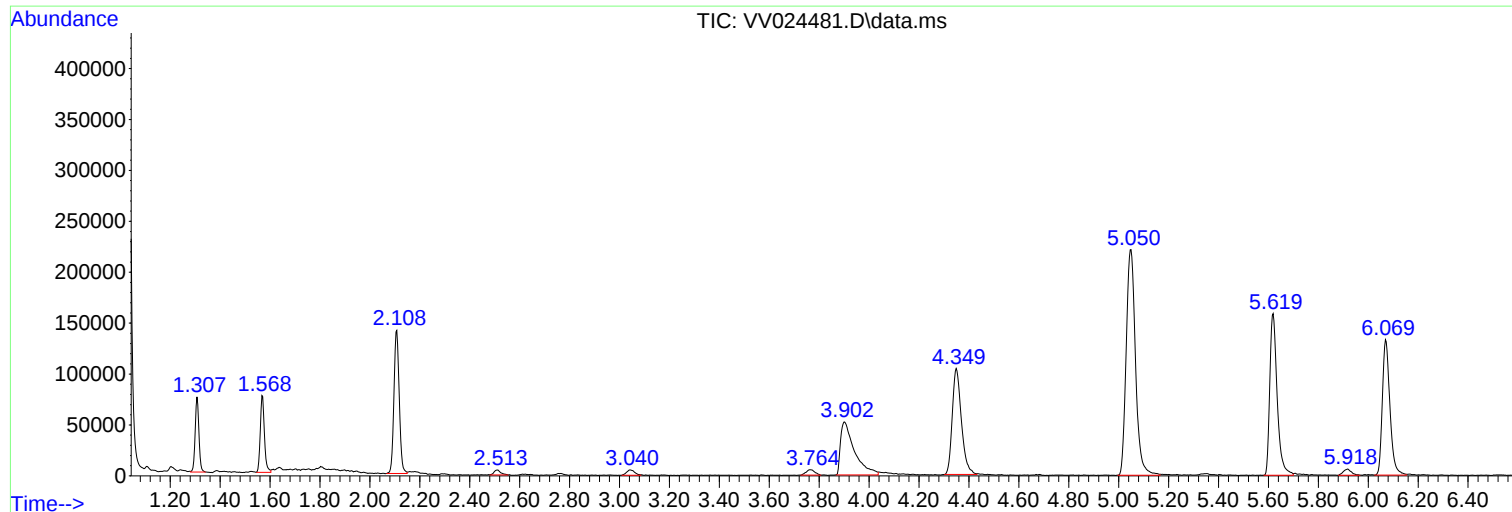

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024481.D
Acq On : 28 Jan 2022 12:15
Operator : SY/MD
Sample : N1317-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024481.D
Acq On : 28 Jan 2022 12:15
Operator : SY/MD
Sample : N1317-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc