

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024484.D
 Acq On : 28 Jan 2022 14:04
 Operator : SY/MD
 Sample : N1328-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COHN9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024484.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.076	8	11	18	rVB	36682	30340	4.80%	0.652%
2	1.243	58	63	72	rVB	9841	10605	1.68%	0.228%
3	1.307	76	83	93	rVB	73909	75160	11.88%	1.616%
4	1.568	157	164	175	rBV	73468	83310	13.17%	1.791%
5	2.108	321	332	344	rBV	134683	197953	31.29%	4.255%
6	3.738	823	839	855	rBV4	7321	20866	3.30%	0.449%
7	3.889	875	886	930	rBV	49471	184696	29.20%	3.970%
8	4.343	1008	1027	1053	rBV2	102189	263806	41.70%	5.670%
9	5.043	1229	1245	1268	rBV3	212993	535148	84.60%	11.503%
10	5.613	1410	1422	1446	rBV	152452	318355	50.33%	6.843%
11	5.905	1503	1513	1528	rVB3	6092	13822	2.19%	0.297%
12	6.066	1546	1563	1593	rBV	127804	273718	43.27%	5.883%
13	6.564	1708	1718	1739	rBV5	5112	12561	1.99%	0.270%
14	6.986	1838	1849	1869	rBV	50283	98174	15.52%	2.110%
15	7.130	1884	1894	1907	rVB5	8798	17136	2.71%	0.368%
16	7.313	1939	1951	1970	rBV	229341	407904	64.48%	8.768%
17	7.394	1972	1976	1991	rVB5	5218	9983	1.58%	0.215%
18	7.622	2037	2047	2068	rBV2	28937	56872	8.99%	1.222%
19	8.085	2174	2191	2231	rBV3	292567	632570	100.00%	13.597%
20	8.850	2418	2429	2465	rBV	262201	435942	68.92%	9.370%
21	10.137	2818	2829	2837	rBV2	6362	9597	1.52%	0.206%
22	10.214	2842	2853	2871	rBV	81691	130388	20.61%	2.803%
23	10.381	2897	2905	2916	rVB2	11497	19433	3.07%	0.418%
24	11.249	3164	3175	3198	rBV	267286	418797	66.21%	9.002%
25	11.532	3252	3263	3271	rBV3	8635	15475	2.45%	0.333%
26	11.622	3280	3291	3311	rVB	230268	369281	58.38%	7.938%
27	14.664	4228	4237	4248	rBV2	6614	10463	1.65%	0.225%




Sum of corrected areas: 4652355

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024484.D
Acq On : 28 Jan 2022 14:04
Operator : SY/MD
Sample : N1328-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COHN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

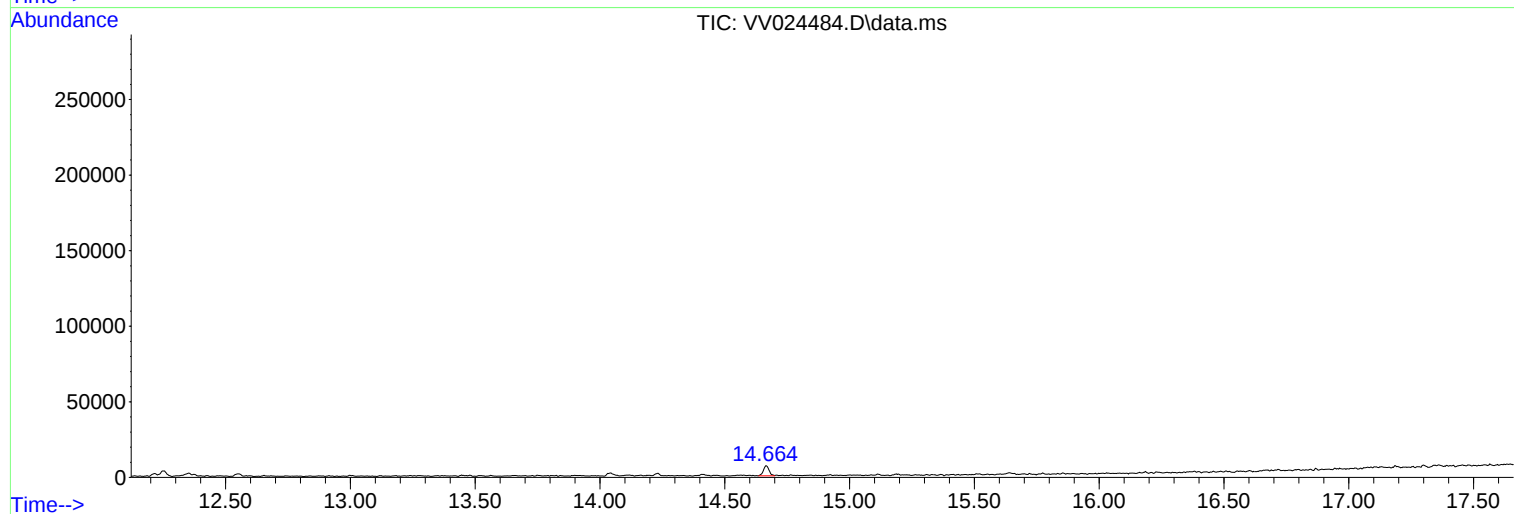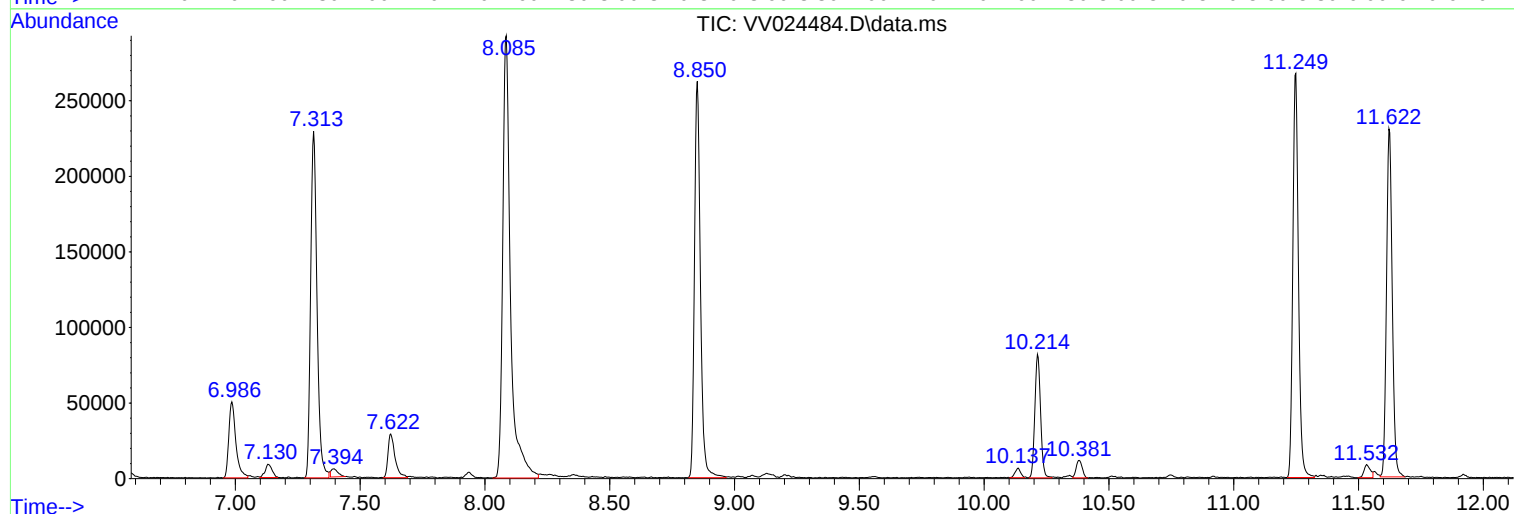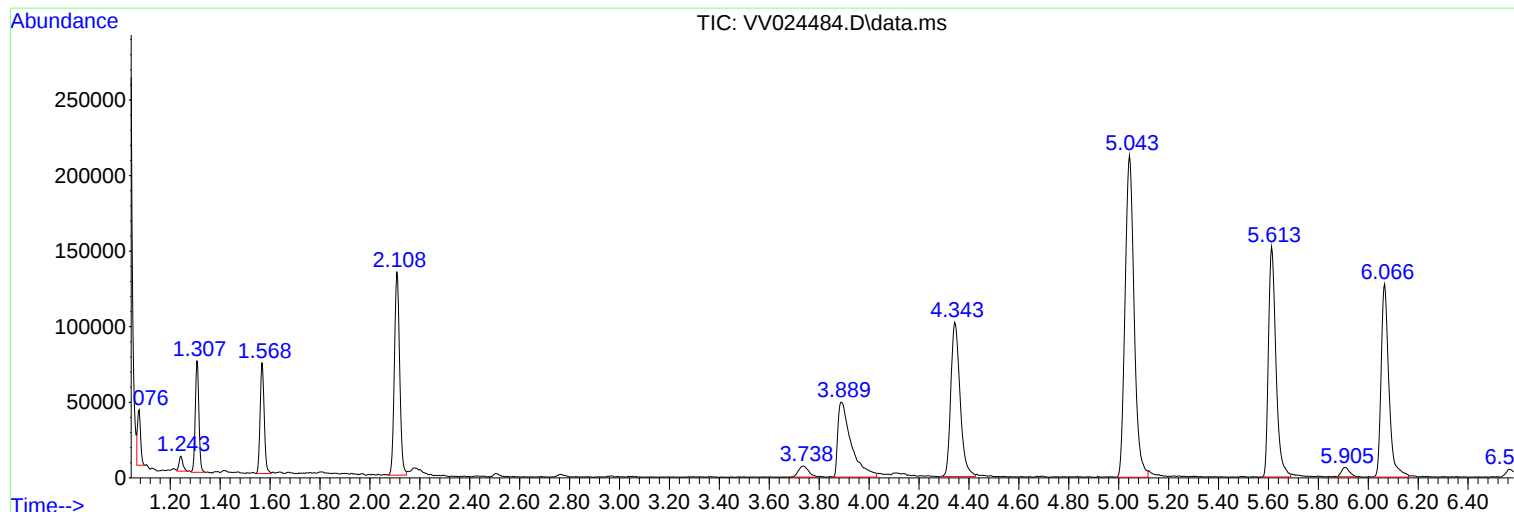

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024484.D
Acq On : 28 Jan 2022 14:04
Operator : SY/MD
Sample : N1328-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024484.D
Acq On : 28 Jan 2022 14:04
Operator : SY/MD
Sample : N1328-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
