

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024487.D
 Acq On : 28 Jan 2022 15:16
 Operator : SY/MD
 Sample : VIBLK243
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK250

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	74800	74763	13.55%	1.529%
2	1.568	156	164	176	rBV	73311	83659	15.17%	1.711%
3	2.111	321	333	354	rVB2	150104	241116	43.71%	4.931%
4	3.918	883	895	921	rBV2	41664	168593	30.57%	3.448%
5	4.352	1011	1030	1053	rBV	102551	264829	48.01%	5.416%
6	5.050	1232	1247	1278	rBV2	216599	551580	100.00%	11.279%
7	5.619	1412	1424	1448	rBV	153416	318149	57.68%	6.506%
8	5.918	1503	1517	1541	rBV2	94020	197919	35.88%	4.047%
9	6.072	1549	1565	1586	rBV	128938	272910	49.48%	5.581%
10	6.989	1839	1850	1869	rBV	54102	104177	18.89%	2.130%
11	7.317	1941	1952	1972	rBV	233338	416323	75.48%	8.513%
12	7.404	1975	1979	1993	rVB7	3669	6194	1.12%	0.127%
13	7.625	2037	2048	2065	rBV2	30070	58108	10.53%	1.188%
14	7.976	2136	2157	2176	rBV	162118	291045	52.77%	5.952%
15	8.092	2183	2193	2228	rBV	213321	465059	84.31%	9.510%
16	8.854	2417	2430	2447	rBV	257640	427389	77.48%	8.740%
17	10.217	2843	2854	2869	rBV2	85609	139553	25.30%	2.854%
18	10.381	2894	2905	2914	rBV	11463	18872	3.42%	0.386%
19	11.249	3161	3175	3195	rBV	264803	414048	75.07%	8.467%
20	11.625	3279	3292	3315	rBV	234876	375885	68.15%	7.687%




Sum of corrected areas: 4890171

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024487.D
Acq On : 28 Jan 2022 15:16
Operator : SY/MD
Sample : VIBLK243
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

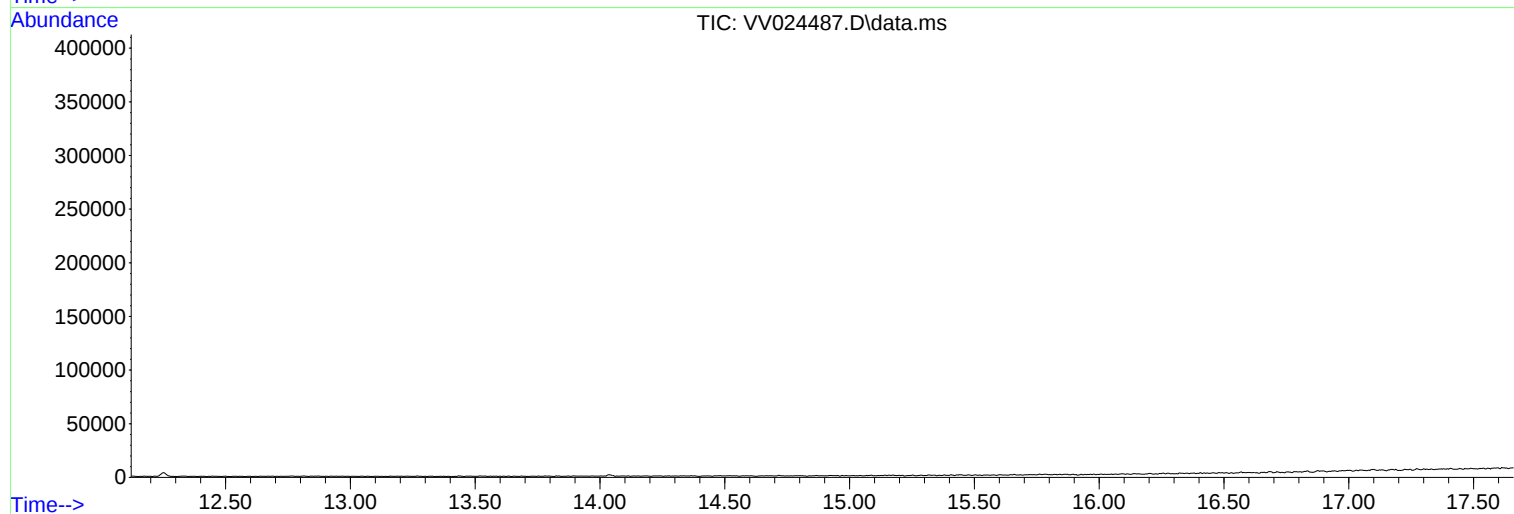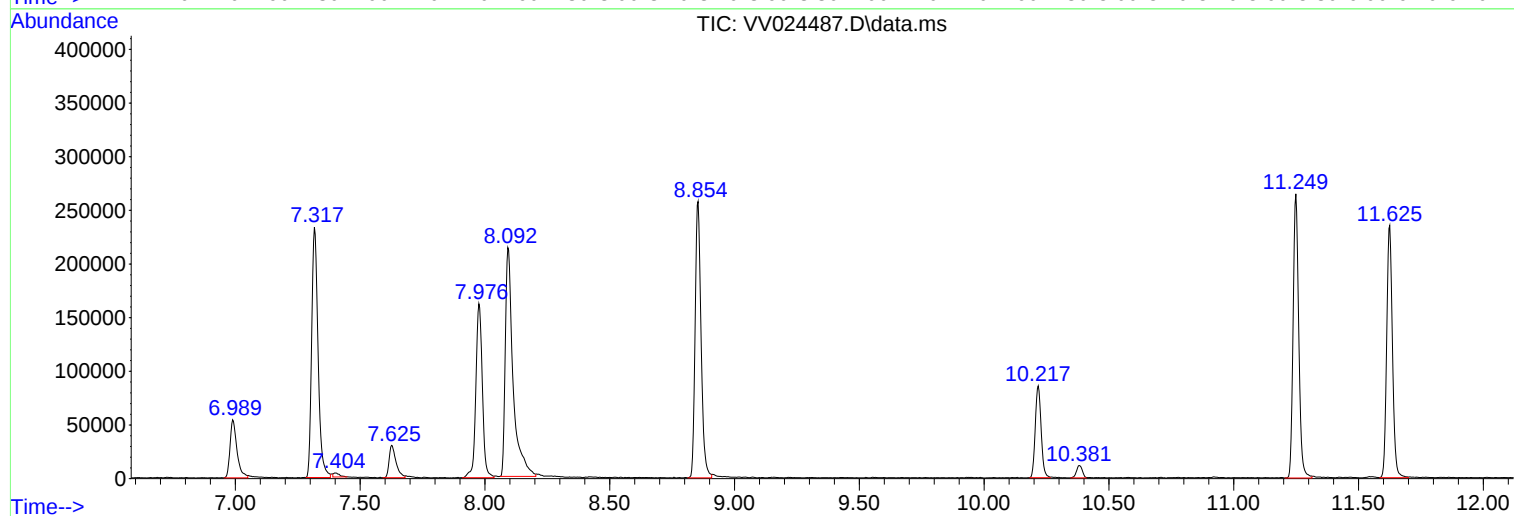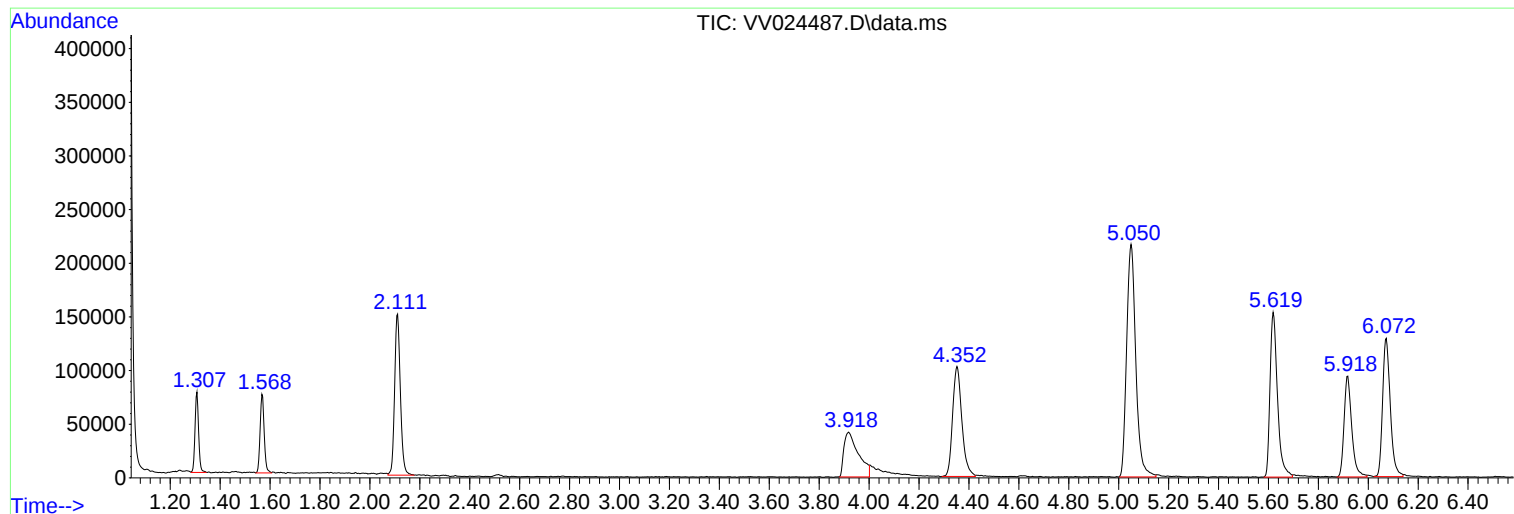

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024487.D
Acq On : 28 Jan 2022 15:16
Operator : SY/MD
Sample : VIBLK243
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024487.D
Acq On : 28 Jan 2022 15:16
Operator : SY/MD
Sample : VIBLK243
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------