

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024490.D
 Acq On : 28 Jan 2022 16:47
 Operator : SY/MD
 Sample : VV0128WBL03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK300

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	68266	70542	13.91%	1.798%
2	1.568	156	164	175	rBV	66951	75524	14.89%	1.925%
3	2.105	321	331	344	rBV	128219	186966	36.87%	4.764%
4	2.507	445	456	468	rBV2	9134	15185	2.99%	0.387%
5	3.918	884	895	898	rBV2	23259	40809	8.05%	1.040%
6	4.346	1013	1028	1054	rVB	96712	243789	48.07%	6.212%
7	5.043	1230	1245	1272	rBV2	200477	507118	100.00%	12.923%
8	5.613	1411	1422	1443	rBV	148541	303696	59.89%	7.739%
9	5.915	1503	1516	1534	rBV8	16551	39958	7.88%	1.018%
10	6.066	1550	1563	1586	rBV2	116819	252459	49.78%	6.433%
11	6.985	1839	1849	1867	rBV2	48292	93486	18.43%	2.382%
12	7.313	1940	1951	1972	rBV	208078	370364	73.03%	9.438%
13	7.625	2039	2048	2074	rBV	26756	54346	10.72%	1.385%
14	7.976	2149	2157	2170	rVB4	10993	19438	3.83%	0.495%
15	8.092	2181	2193	2237	rBV	160077	424458	83.70%	10.816%
16	8.419	2283	2295	2305	rBV3	5581	10224	2.02%	0.261%
17	8.850	2419	2429	2459	rBV	244225	404709	79.81%	10.313%
18	10.217	2839	2854	2877	rBV	78448	128449	25.33%	3.273%
19	11.249	3164	3175	3194	rBV	226774	361106	71.21%	9.202%
20	11.622	3280	3291	3317	rBV	198888	321572	63.41%	8.195%




Sum of corrected areas: 3924198

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024490.D
Acq On : 28 Jan 2022 16:47
Operator : SY/MD
Sample : VV0128WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK300

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

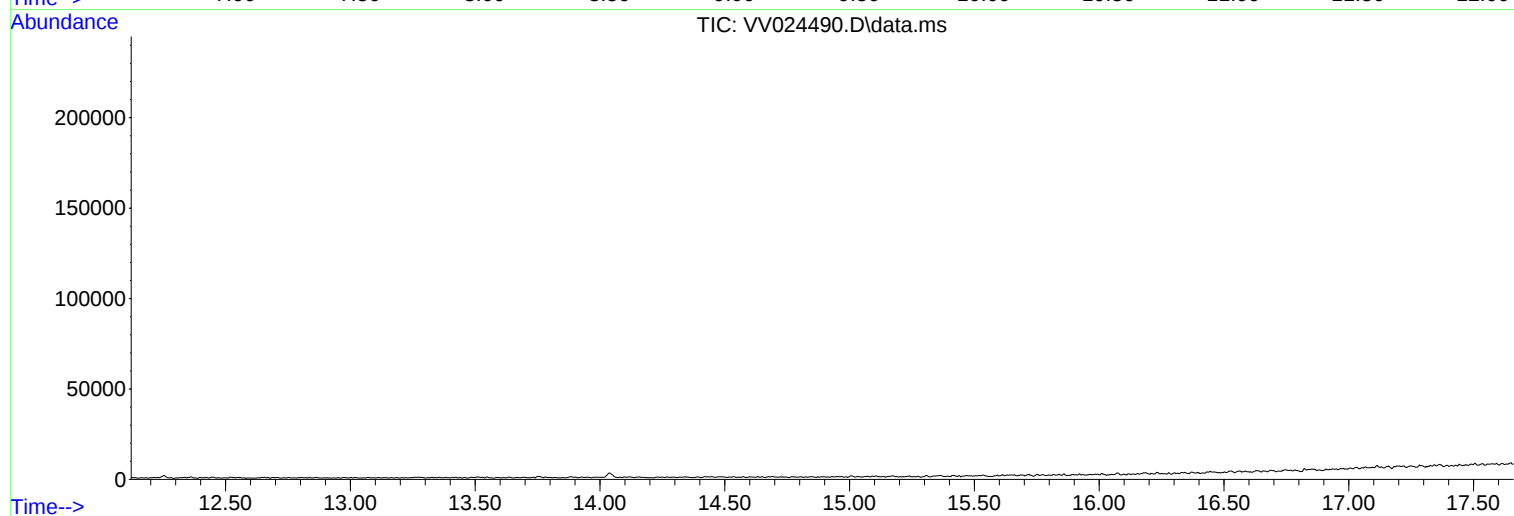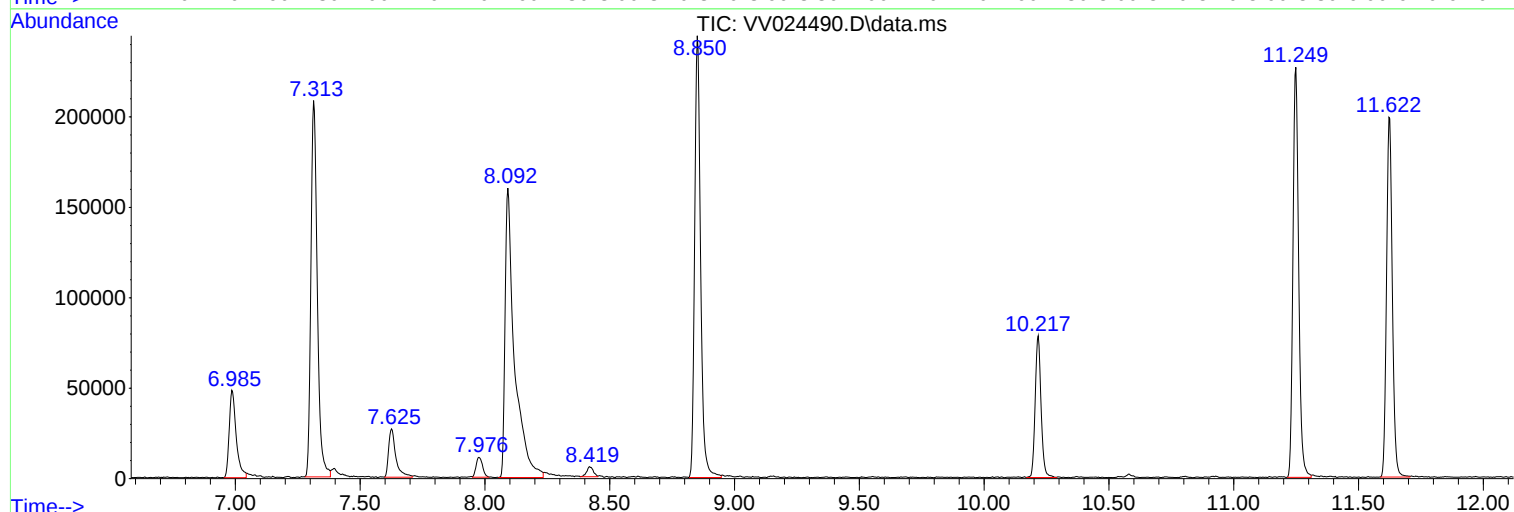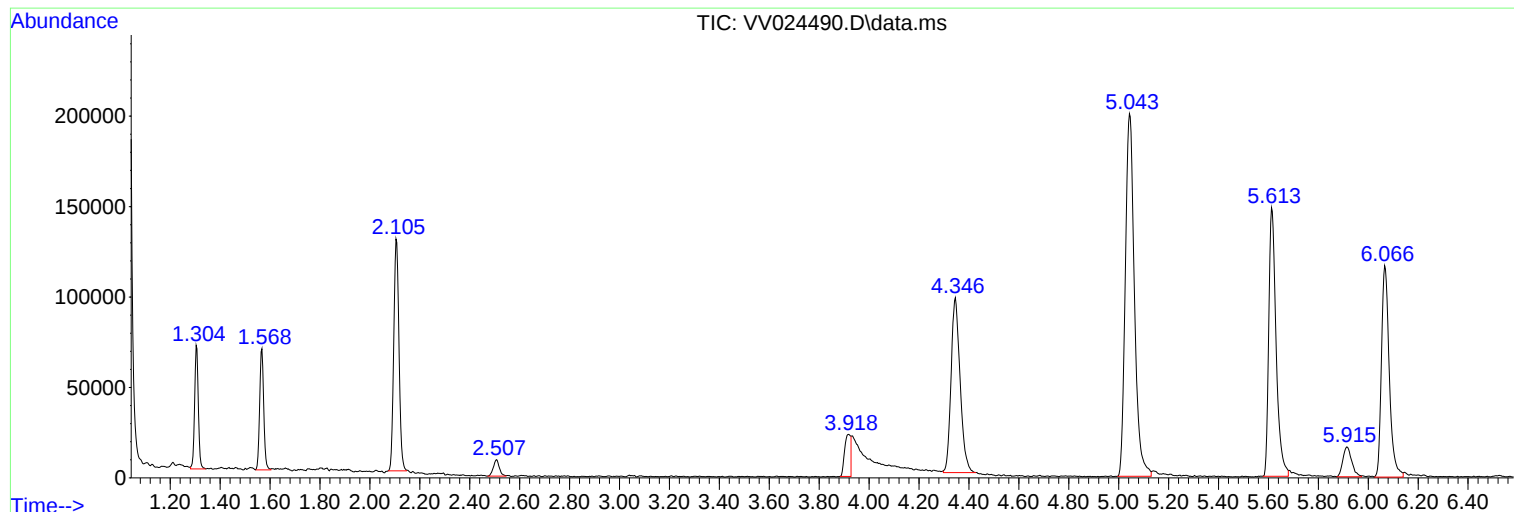

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024490.D
Acq On : 28 Jan 2022 16:47
Operator : SY/MD
Sample : VV0128WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK300

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024490.D
Acq On : 28 Jan 2022 16:47
Operator : SY/MD
Sample : VV0128WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK300

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc