

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024492.D
 Acq On : 28 Jan 2022 17:38
 Operator : SY/MD
 Sample : N1328-02DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0HM1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	63827	65862	3.93%	1.047%
2	1.568	155	164	178	rBV	68382	76352	4.56%	1.214%
3	2.111	322	333	352	rVB4	181247	308360	18.40%	4.903%
4	3.915	881	894	926	rBV2	89277	272442	16.25%	4.332%
5	4.349	1015	1029	1054	rVB2	93083	234209	13.97%	3.724%
6	4.609	1092	1110	1131	rBV3	23239	58455	3.49%	0.929%
7	5.050	1230	1247	1270	rBV3	194008	487944	29.11%	7.758%
8	5.619	1412	1424	1446	rBV	142716	299742	17.88%	4.766%
9	5.915	1503	1516	1545	rBV	210675	430069	25.66%	6.838%
10	6.072	1552	1565	1589	rBV	118042	245247	14.63%	3.899%
11	6.989	1840	1850	1872	rBV	46937	92864	5.54%	1.477%
12	7.317	1939	1952	1970	rBV	203061	360305	21.50%	5.729%
13	7.625	2039	2048	2064	rBV	26900	50479	3.01%	0.803%
14	7.976	2140	2157	2182	rBV	993683	1676216	100.00%	26.652%
15	8.092	2184	2193	2224	rBV	169692	407795	24.33%	6.484%
16	8.854	2417	2430	2450	rBV	243037	403359	24.06%	6.414%
17	10.217	2838	2854	2872	rBV	76830	126204	7.53%	2.007%
18	11.249	3163	3175	3197	rBV	237224	373488	22.28%	5.939%
19	11.625	3280	3292	3313	rBV	199780	319803	19.08%	5.085%




Sum of corrected areas: 6289195

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024492.D
Acq On : 28 Jan 2022 17:38
Operator : SY/MD
Sample : N1328-02DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

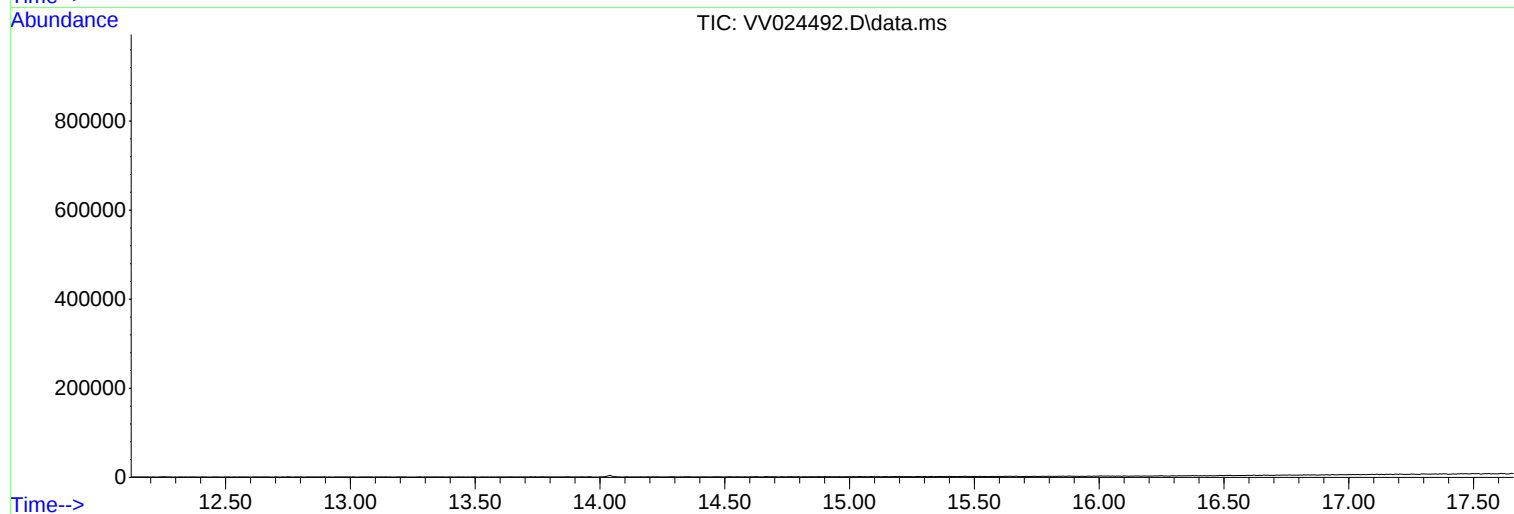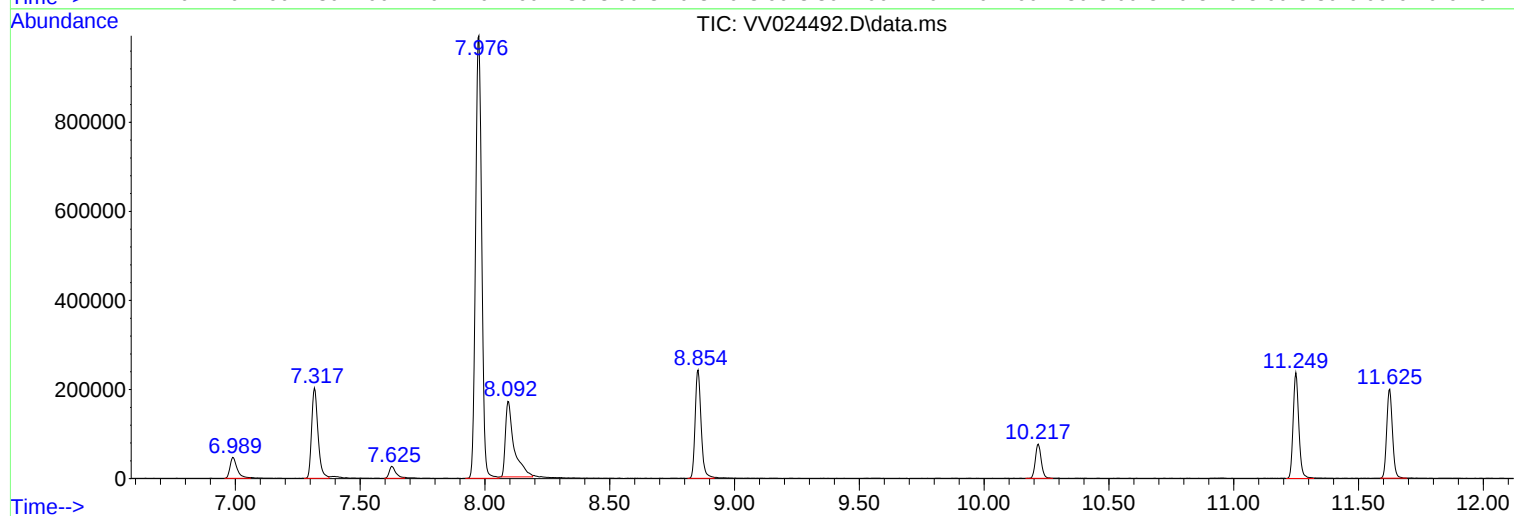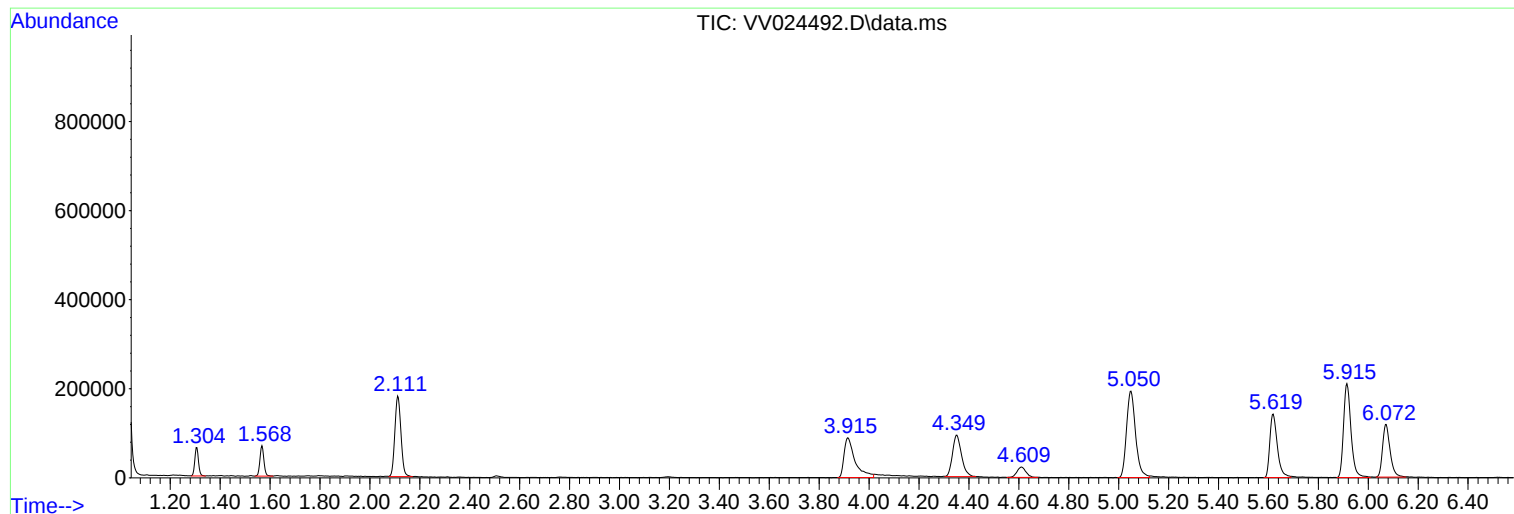

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024492.D
Acq On : 28 Jan 2022 17:38
Operator : SY/MD
Sample : N1328-02DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024492.D
Acq On : 28 Jan 2022 17:38
Operator : SY/MD
Sample : N1328-02DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------