

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024494.D
 Acq On : 28 Jan 2022 18:25
 Operator : SY/MD
 Sample : N1328-04 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0HM3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	93	rBV2	95909	107356	3.50%	1.137%
2	1.568	156	164	176	rBV	67567	78213	2.55%	0.829%
3	2.114	322	334	357	rVB3	238051	407974	13.32%	4.322%
4	3.912	876	893	936	rBV	692104	1747958	57.06%	18.518%
5	4.352	1015	1030	1060	rVB2	94954	247237	8.07%	2.619%
6	4.609	1098	1110	1130	rVB3	17439	44131	1.44%	0.468%
7	5.050	1229	1247	1273	rBV2	200005	509522	16.63%	5.398%
8	5.619	1410	1424	1446	rBV	145658	305913	9.99%	3.241%
9	5.912	1500	1515	1551	rBV	1569837	3063219	100.00%	32.452%
10	6.069	1553	1564	1588	rVB2	122476	259074	8.46%	2.745%
11	6.992	1840	1851	1874	rBV	48188	95823	3.13%	1.015%
12	7.317	1940	1952	1973	rBV	212242	373451	12.19%	3.956%
13	7.625	2038	2048	2065	rBV	28060	53517	1.75%	0.567%
14	7.976	2141	2157	2174	rBV	282293	471733	15.40%	4.998%
15	8.092	2184	2193	2236	rBV	166922	429500	14.02%	4.550%
16	8.854	2416	2430	2455	rBV	242872	410922	13.41%	4.353%
17	10.217	2843	2854	2872	rBV	80944	128942	4.21%	1.366%
18	11.249	3164	3175	3201	rBV	242140	378297	12.35%	4.008%
19	11.625	3279	3292	3313	rBV	204433	326527	10.66%	3.459%




Sum of corrected areas: 9439309

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024494.D
Acq On : 28 Jan 2022 18:25
Operator : SY/MD
Sample : N1328-04 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

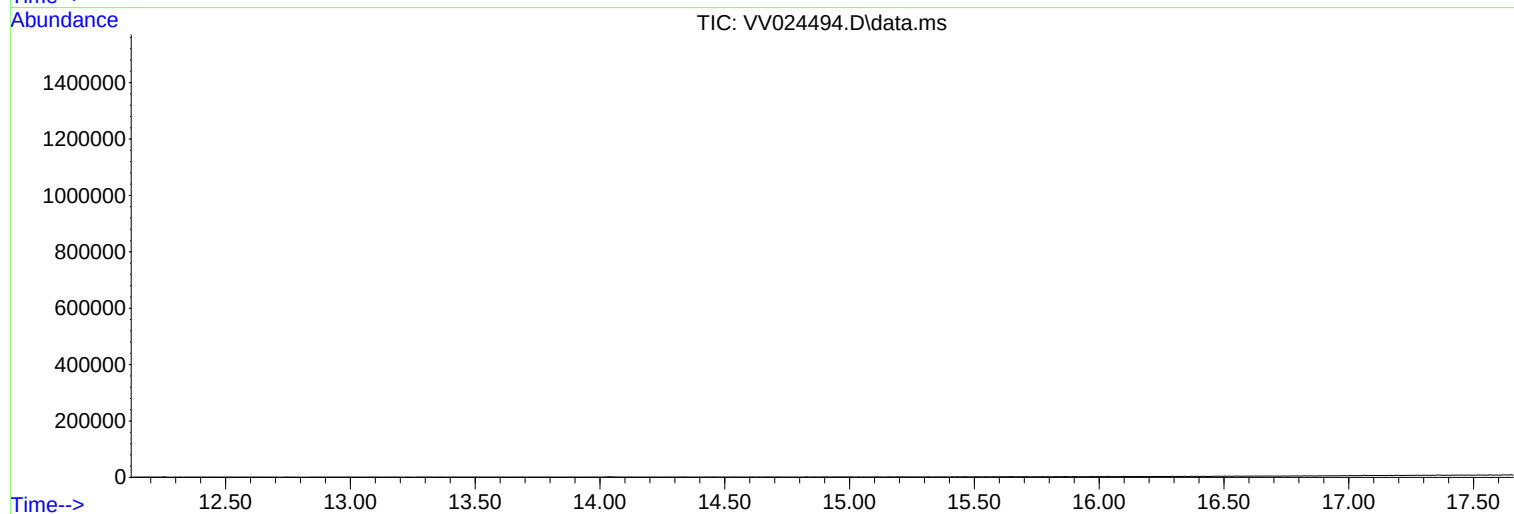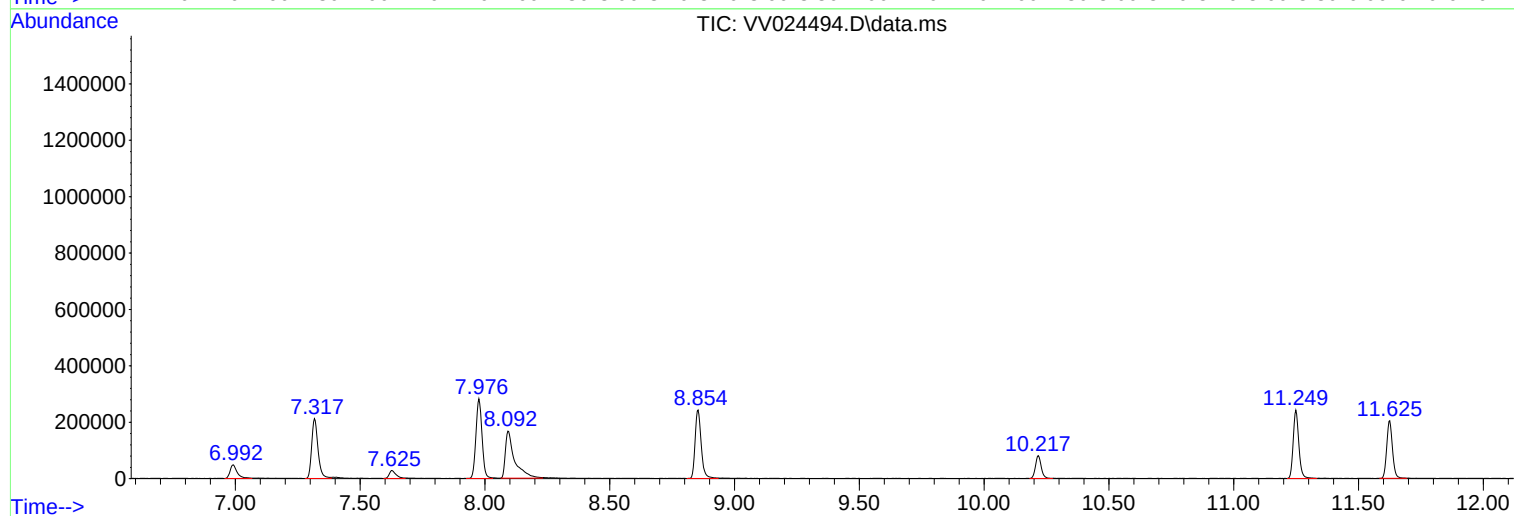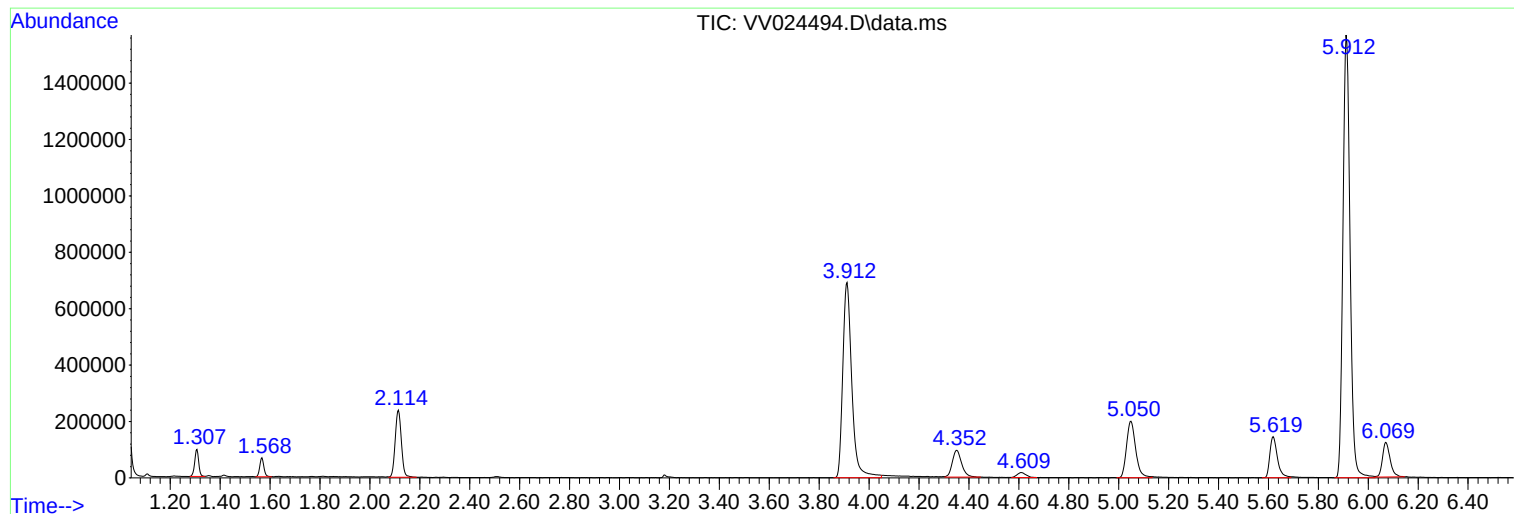

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024494.D
Acq On : 28 Jan 2022 18:25
Operator : SY/MD
Sample : N1328-04 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024494.D
Acq On : 28 Jan 2022 18:25
Operator : SY/MD
Sample : N1328-04 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc