

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024496.D
 Acq On : 28 Jan 2022 19:11
 Operator : SY/MD
 Sample : N1328-06 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0HM5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	70295	71277	3.60%	1.214%
2	1.564	155	163	177	rBV	68620	77826	3.93%	1.325%
3	2.108	322	332	351	rVB2	139787	219944	11.10%	3.746%
4	3.915	882	894	908	rBV2	26709	87626	4.42%	1.492%
5	4.349	1013	1029	1056	rVB	91404	238234	12.02%	4.057%
6	4.609	1100	1110	1125	rVB2	7713	20164	1.02%	0.343%
7	5.047	1231	1246	1279	rBV2	191430	489489	24.70%	8.336%
8	5.619	1412	1424	1450	rBV	132346	278892	14.07%	4.749%
9	5.918	1503	1517	1540	rVB6	36007	82255	4.15%	1.401%
10	6.069	1548	1564	1592	rBV2	119142	255728	12.90%	4.355%
11	6.989	1840	1850	1876	rBV2	45708	92684	4.68%	1.578%
12	7.317	1941	1952	1974	rBV	197327	351486	17.74%	5.986%
13	7.628	2037	2049	2065	rBV2	26767	53014	2.68%	0.903%
14	7.972	2142	2156	2184	rBV	1184963	1981818	100.00%	33.750%
15	8.091	2184	2193	2233	rVV	169508	429433	21.67%	7.313%
16	8.853	2417	2430	2452	rBV	224668	379721	19.16%	6.467%
17	10.217	2843	2854	2867	rBV	77110	125529	6.33%	2.138%
18	11.249	3165	3175	3194	rBV	212016	330047	16.65%	5.621%
19	11.625	3280	3292	3314	rBV	190146	306945	15.49%	5.227%




Sum of corrected areas: 5872112

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024496.D
Acq On : 28 Jan 2022 19:11
Operator : SY/MD
Sample : N1328-06 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

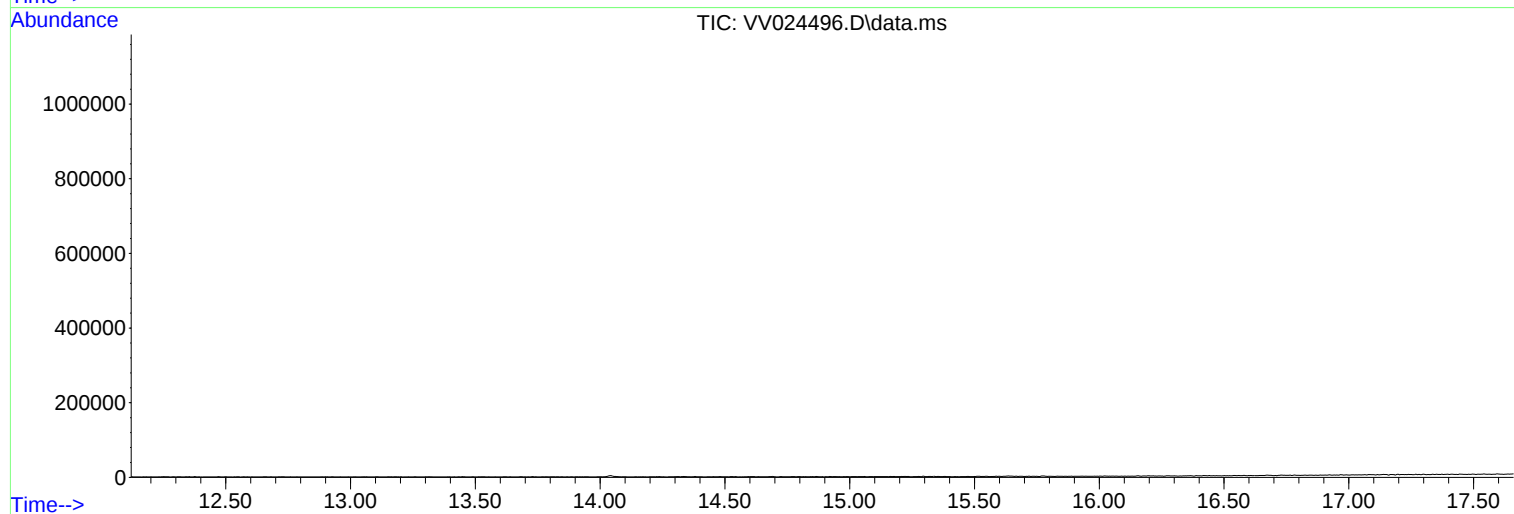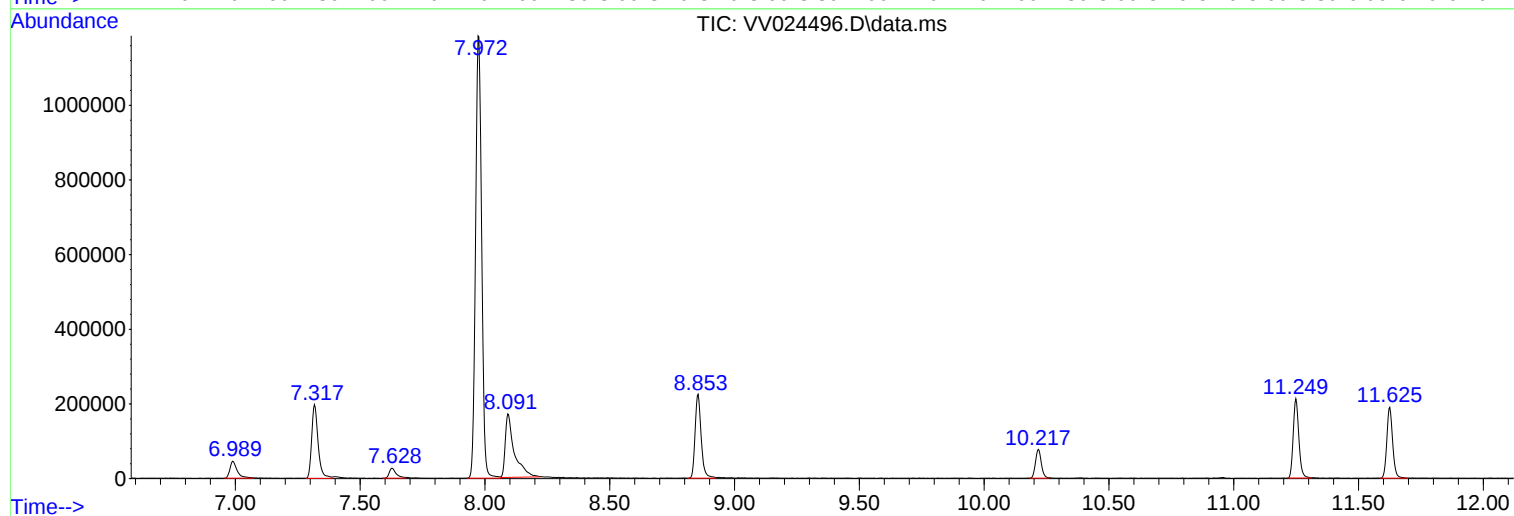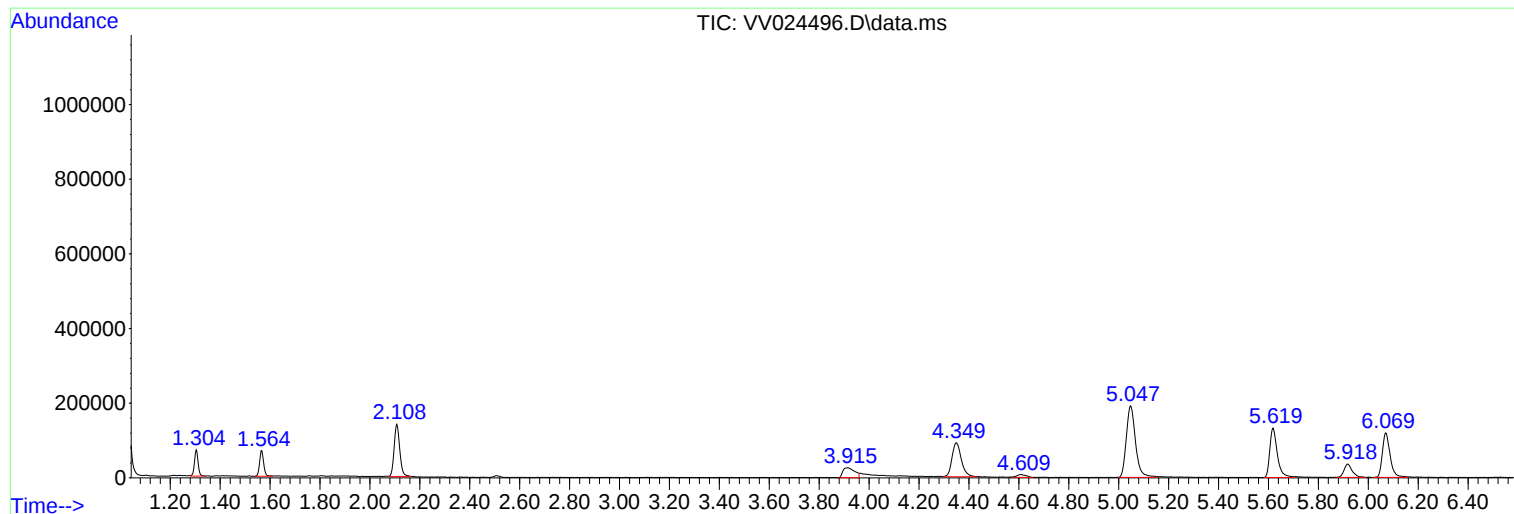

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024496.D
Acq On : 28 Jan 2022 19:11
Operator : SY/MD
Sample : N1328-06 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024496.D
Acq On : 28 Jan 2022 19:11
Operator : SY/MD
Sample : N1328-06 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
