

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024499.D
 Acq On : 28 Jan 2022 20:21
 Operator : SY/MD
 Sample : N1328-09 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0HM8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	67128	70970	15.12%	1.814%
2	1.568	156	164	176	rVB	68158	76302	16.25%	1.950%
3	2.108	322	332	352	rVB2	129157	195402	41.63%	4.994%
4	2.510	449	457	469	rBV5	3908	7151	1.52%	0.183%
5	3.918	884	895	916	rBV2	28880	108458	23.10%	2.772%
6	4.349	1014	1029	1052	rBV2	86674	223492	47.61%	5.712%
7	5.046	1228	1246	1271	rBV3	181479	469427	100.00%	11.997%
8	5.619	1412	1424	1450	rBV	129438	278952	59.42%	7.129%
9	5.918	1505	1517	1534	rBV7	15591	37798	8.05%	0.966%
10	6.069	1552	1564	1588	rBV	112977	241827	51.52%	6.180%
11	6.992	1840	1851	1870	rBV	43744	86217	18.37%	2.203%
12	7.316	1941	1952	1971	rBV	177327	327395	69.74%	8.367%
13	7.628	2039	2049	2068	rBV2	25973	53611	11.42%	1.370%
14	7.976	2146	2157	2172	rBV	108935	183528	39.10%	4.690%
15	8.091	2183	2193	2231	rBV	154865	410144	87.37%	10.482%
16	8.853	2418	2430	2453	rBV	223571	384888	81.99%	9.836%
17	10.217	2843	2854	2870	rBV	73609	119991	25.56%	3.067%
18	11.249	3161	3175	3193	rBV	214894	341252	72.70%	8.721%
19	11.625	3279	3292	3310	rBV	177550	289097	61.59%	7.388%
20	14.036	4033	4042	4051	rBV3	3586	6974	1.49%	0.178%




Sum of corrected areas: 3912876

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024499.D
Acq On : 28 Jan 2022 20:21
Operator : SY/MD
Sample : N1328-09 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

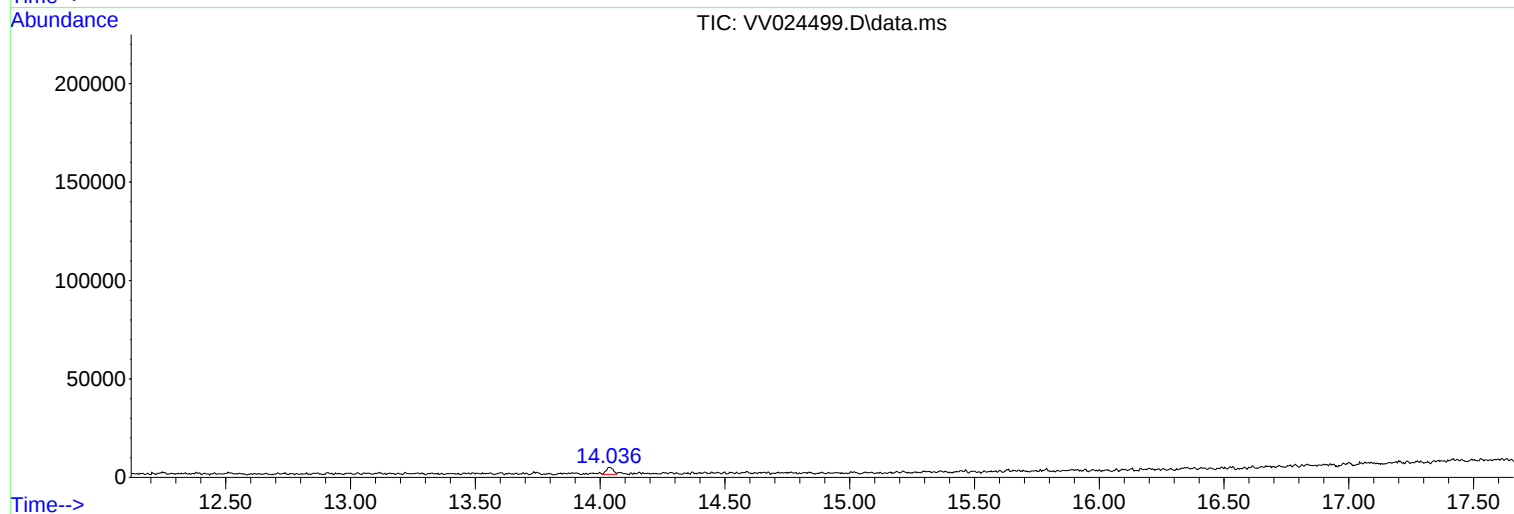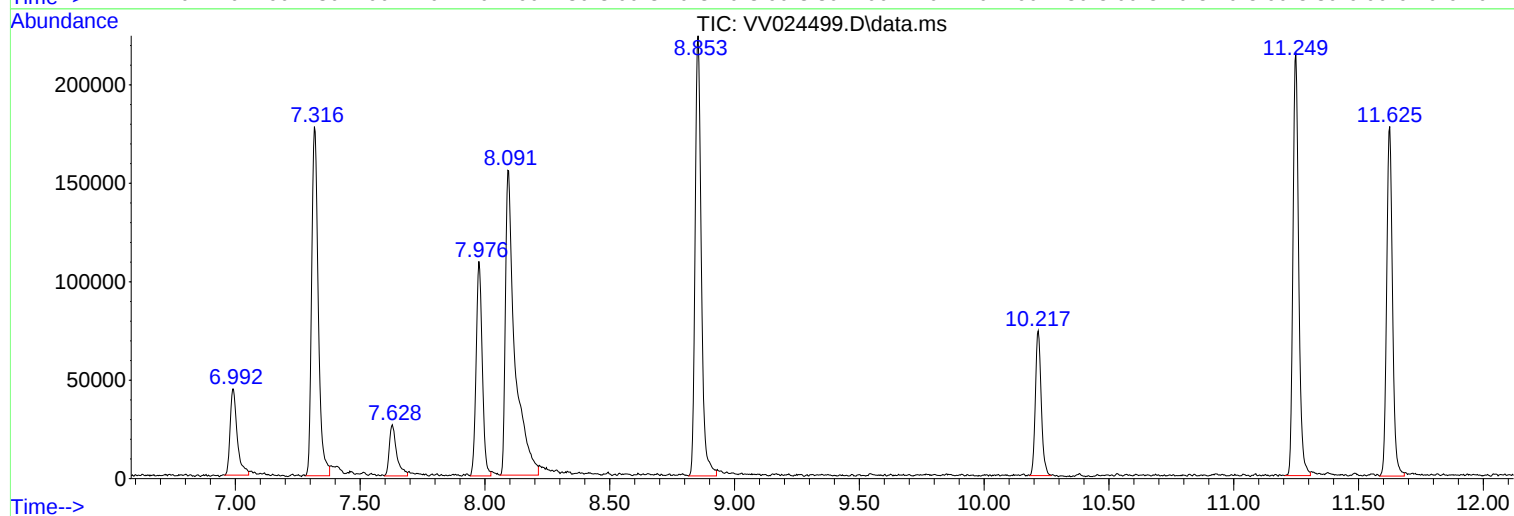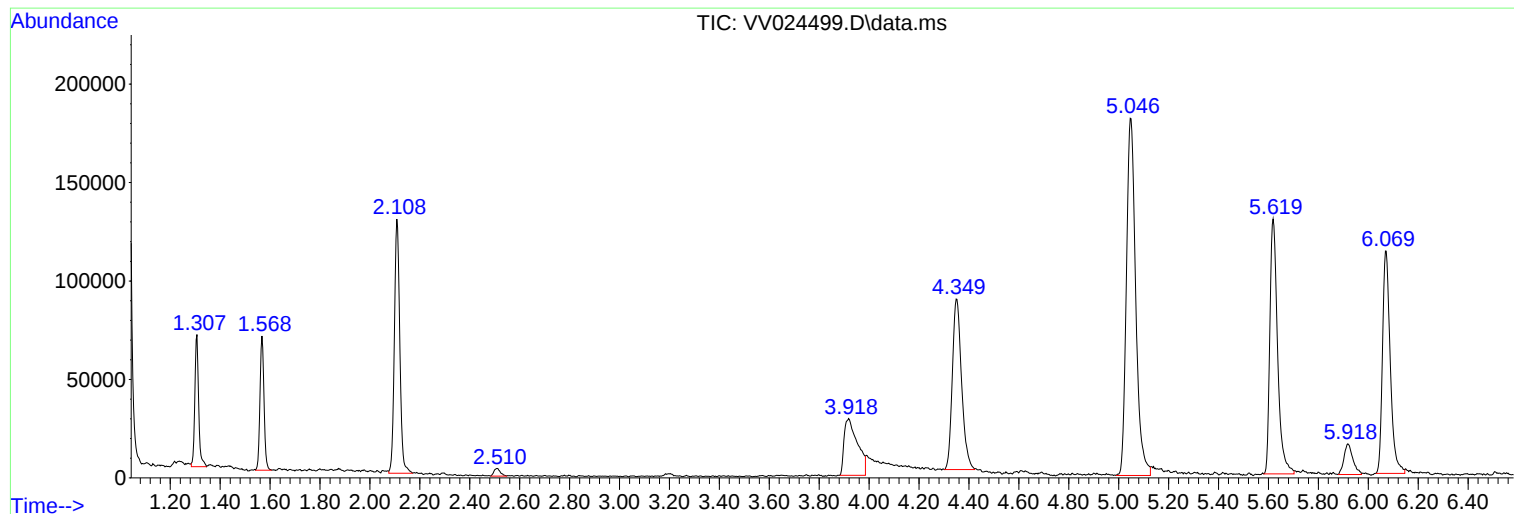

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024499.D
Acq On : 28 Jan 2022 20:21
Operator : SY/MD
Sample : N1328-09 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024499.D
Acq On : 28 Jan 2022 20:21
Operator : SY/MD
Sample : N1328-09 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc