

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024500.D
 Acq On : 28 Jan 2022 20:45
 Operator : SY/MD
 Sample : N1328-10 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0HM9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	71144	74879	15.20%	1.907%
2	1.568	155	164	174	rBV	68761	80458	16.33%	2.049%
3	2.108	321	332	346	rBV	130306	191723	38.91%	4.882%
4	2.510	448	457	469	rVB8	3611	7872	1.60%	0.200%
5	3.915	880	894	914	rBV2	34767	124748	25.32%	3.176%
6	4.352	1012	1030	1052	rBV	93136	240691	48.85%	6.129%
7	5.050	1232	1247	1270	rBV3	192076	492711	100.00%	12.546%
8	5.619	1413	1424	1448	rBV	125130	267472	54.29%	6.811%
9	5.918	1505	1517	1532	rBV5	16555	40701	8.26%	1.036%
10	6.072	1551	1565	1586	rBV	119483	254750	51.70%	6.487%
11	6.989	1840	1850	1870	rBV	43887	89437	18.15%	2.277%
12	7.317	1940	1952	1970	rBV	187937	339911	68.99%	8.655%
13	7.628	2038	2049	2068	rBV2	27307	53703	10.90%	1.367%
14	7.979	2142	2158	2177	rBV3	55778	100830	20.46%	2.567%
15	8.091	2183	2193	2230	rBV	168622	437085	88.71%	11.129%
16	8.854	2419	2430	2455	rBV	215143	366125	74.31%	9.323%
17	10.217	2843	2854	2868	rBV	77971	129552	26.29%	3.299%
18	11.249	3163	3175	3200	rBV	208122	332790	67.54%	8.474%
19	11.625	3278	3292	3310	rBV	185254	301830	61.26%	7.685%




Sum of corrected areas: 3927268

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024500.D
Acq On : 28 Jan 2022 20:45
Operator : SY/MD
Sample : N1328-10 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

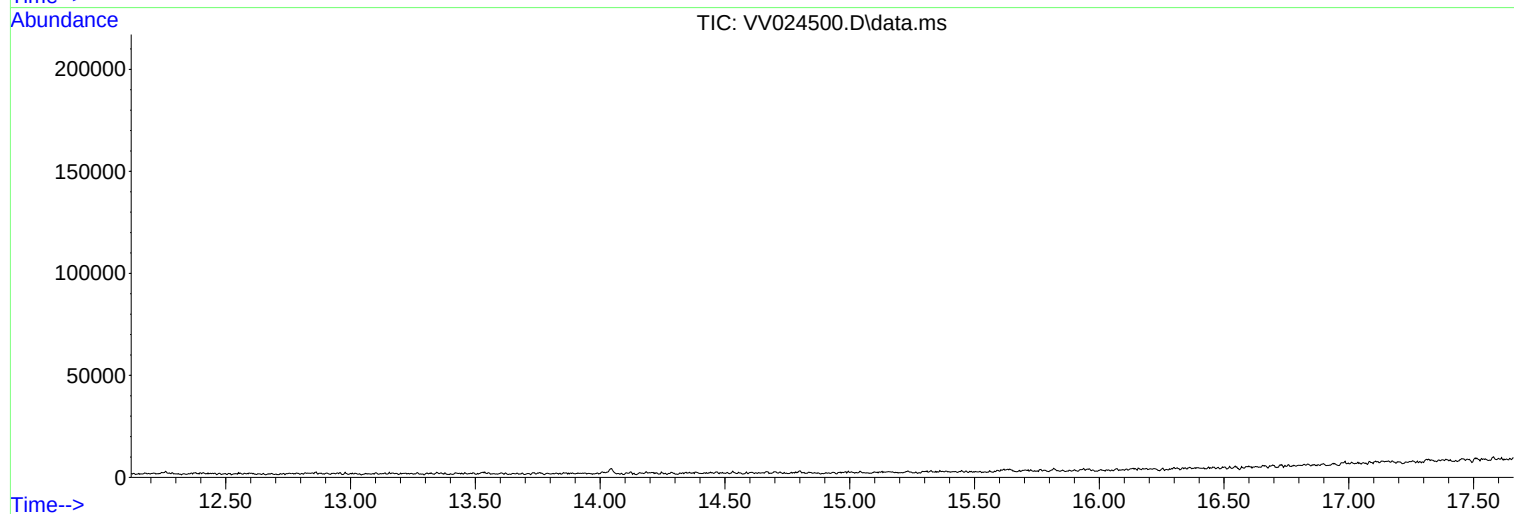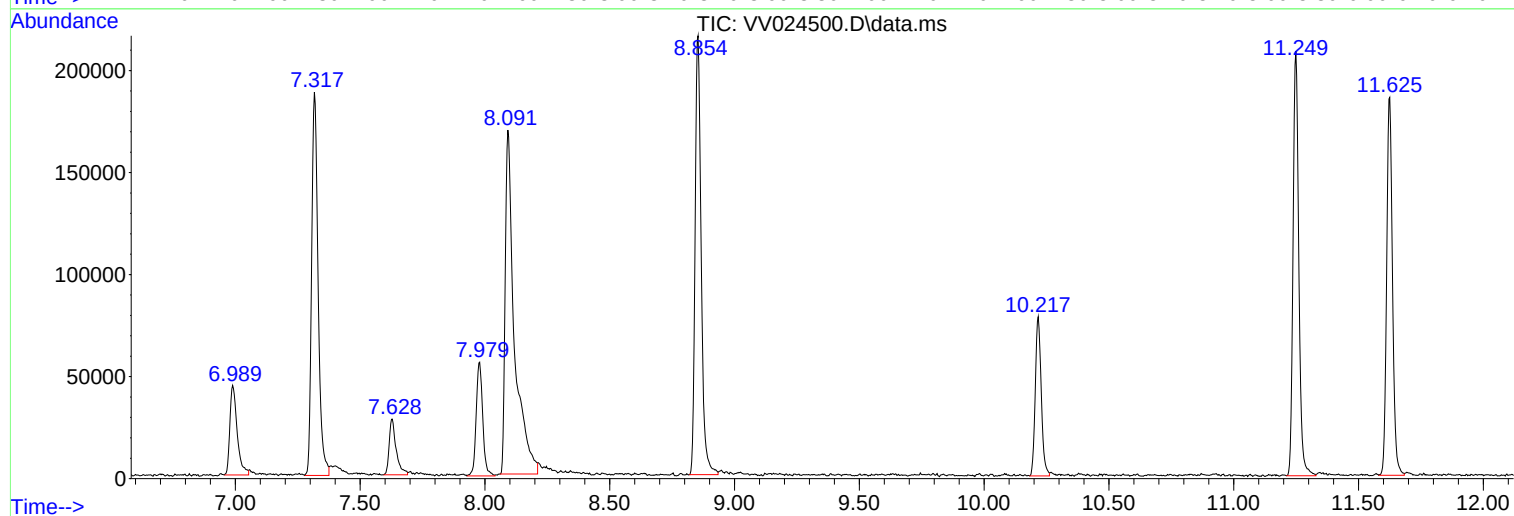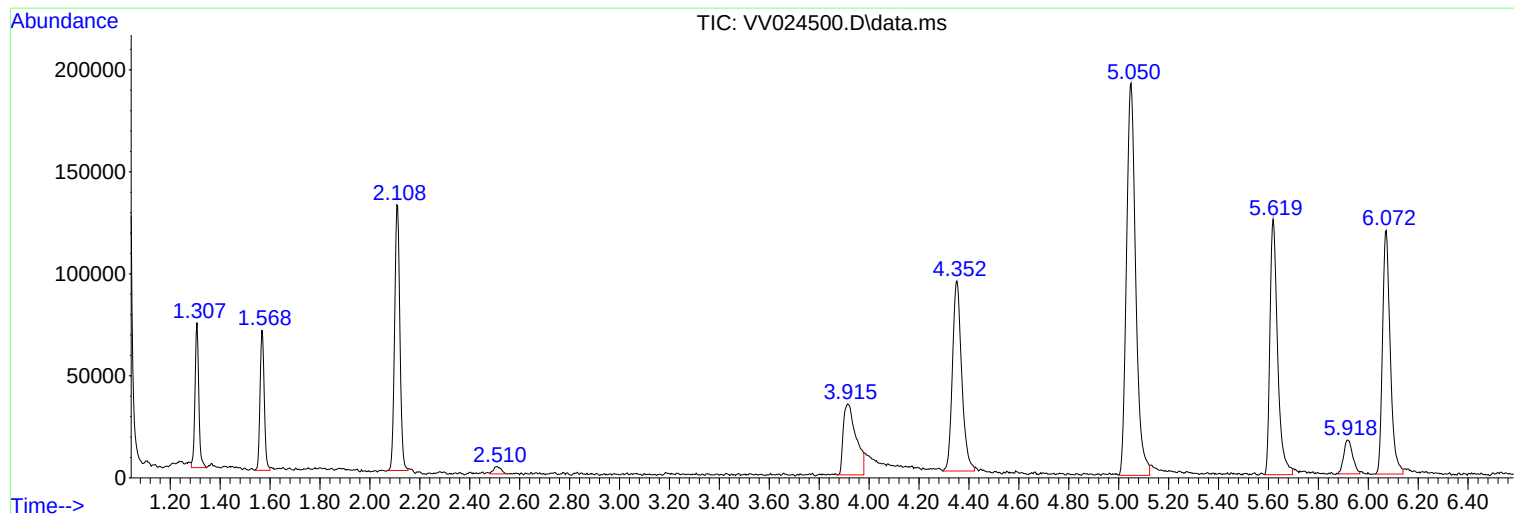

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024500.D
Acq On : 28 Jan 2022 20:45
Operator : SY/MD
Sample : N1328-10 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024500.D
Acq On : 28 Jan 2022 20:45
Operator : SY/MD
Sample : N1328-10 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HM9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc