

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024502.D
 Acq On : 28 Jan 2022 21:31
 Operator : SY/MD
 Sample : N1328-12 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COHN1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024502.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	102	rVB	69462	73549	5.09%	1.352%
2	1.571	157	165	175	rVB	68273	77666	5.38%	1.428%
3	2.111	322	333	352	rVB2	130782	198094	13.72%	3.641%
4	3.194	660	670	684	rVB2	9913	20519	1.42%	0.377%
5	3.915	880	894	924	rBV3	130458	386257	26.75%	7.100%
6	4.352	1013	1030	1052	rBV	90080	232430	16.10%	4.272%
7	5.050	1231	1247	1272	rBV2	186359	478115	33.11%	8.789%
8	5.619	1413	1424	1444	rBV	121586	253006	17.52%	4.651%
9	5.918	1507	1517	1536	rBV5	21752	50821	3.52%	0.934%
10	6.072	1551	1565	1584	rBV	116841	247870	17.17%	4.556%
11	6.992	1841	1851	1871	rBV	43838	85976	5.95%	1.580%
12	7.316	1940	1952	1969	rBV	186871	330551	22.89%	6.076%
13	7.628	2036	2049	2062	rBV	27092	52100	3.61%	0.958%
14	7.976	2143	2157	2184	rBV	858887	1443912	100.00%	26.541%
15	8.091	2184	2193	2232	rVV	175121	426156	29.51%	7.833%
16	8.853	2420	2430	2454	rBV	207601	350472	24.27%	6.442%
17	10.217	2840	2854	2872	rBV	75035	123694	8.57%	2.274%
18	11.249	3165	3175	3199	rBV	196224	316985	21.95%	5.827%
19	11.625	3279	3292	3312	rBV	179780	292061	20.23%	5.369%




Sum of corrected areas: 5440234

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024502.D
Acq On : 28 Jan 2022 21:31
Operator : SY/MD
Sample : N1328-12 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

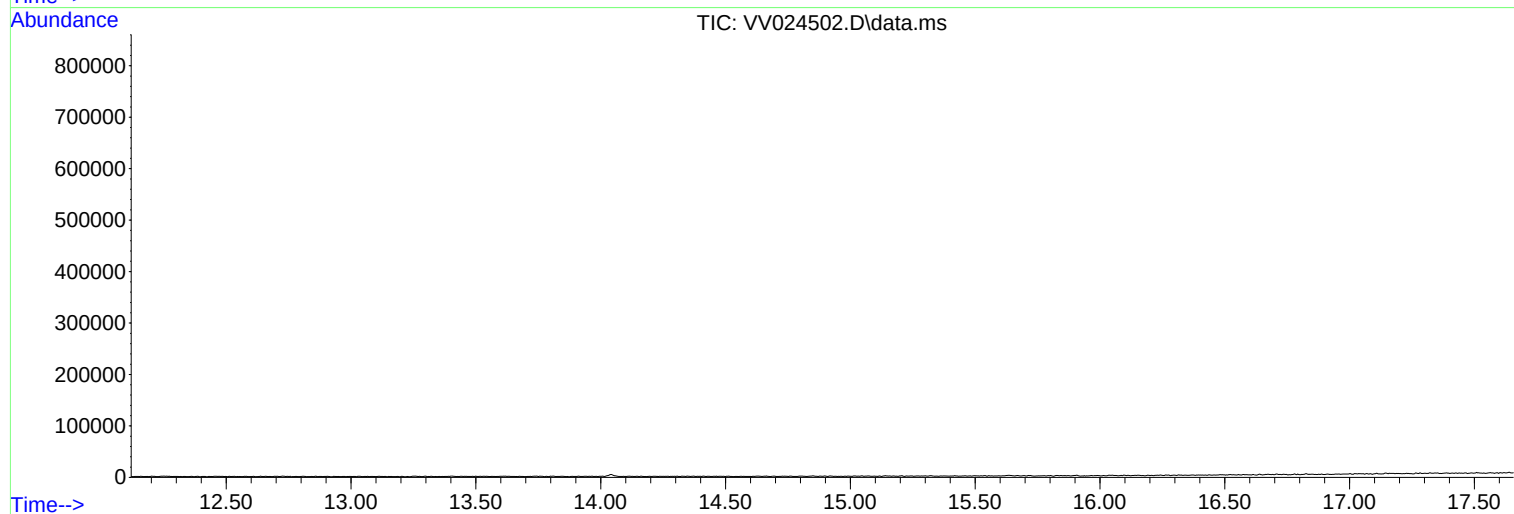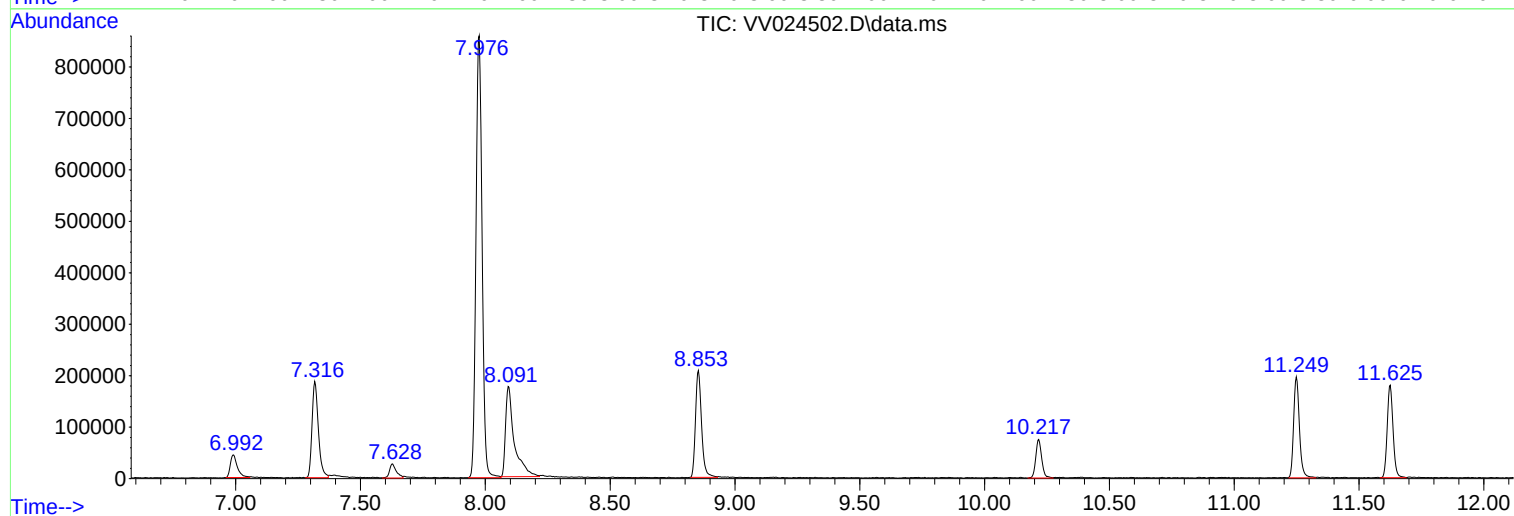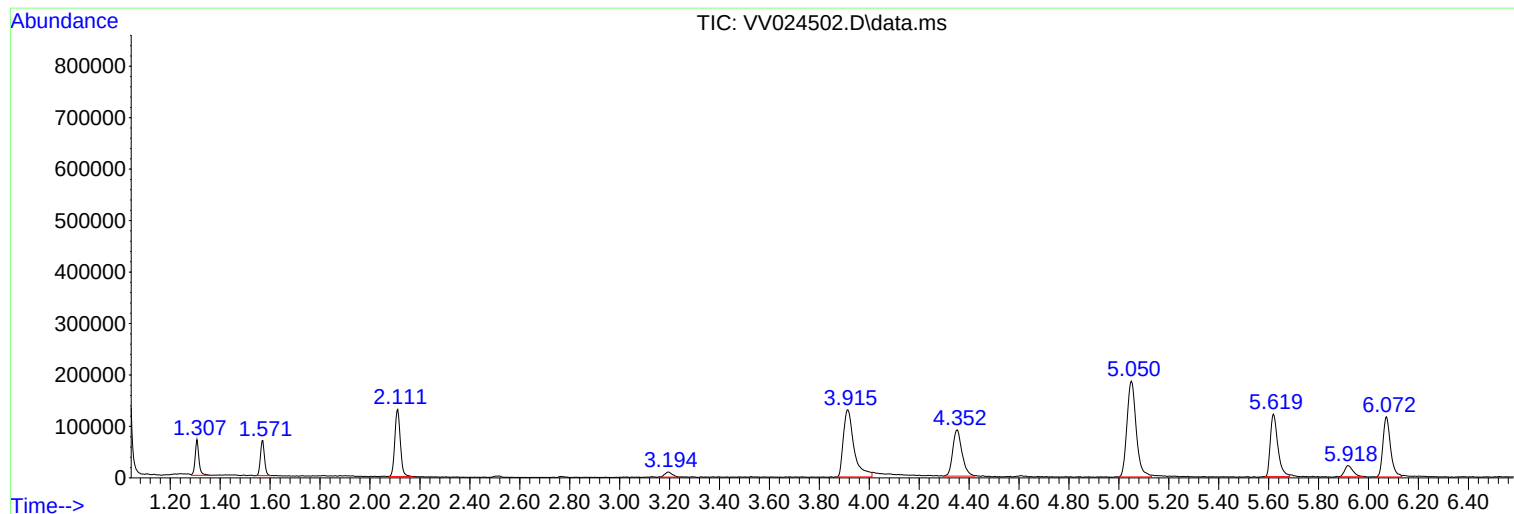

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024502.D
Acq On : 28 Jan 2022 21:31
Operator : SY/MD
Sample : N1328-12 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024502.D
Acq On : 28 Jan 2022 21:31
Operator : SY/MD
Sample : N1328-12 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc