

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024505.D
 Acq On : 28 Jan 2022 22:41
 Operator : SY/MD
 Sample : N1328-15 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0HN4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024505.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	64858	67348	12.69%	1.556%
2	1.568	156	164	176	rVB	68619	77965	14.69%	1.802%
3	2.111	321	333	345	rBV2	136271	210312	39.63%	4.860%
4	3.915	881	894	914	rBV2	54985	175857	33.13%	4.064%
5	4.349	1013	1029	1054	rBV	87777	226688	42.71%	5.238%
6	4.609	1102	1110	1124	rVB9	5441	11951	2.25%	0.276%
7	5.050	1232	1247	1267	rBV2	180172	454416	85.62%	10.500%
8	5.619	1407	1424	1454	rBV	120534	262839	49.52%	6.073%
9	5.918	1503	1517	1536	rBV3	57917	128581	24.23%	2.971%
10	6.069	1549	1564	1593	rBV	115728	246861	46.51%	5.704%
11	6.992	1840	1851	1866	rBV2	41653	82750	15.59%	1.912%
12	7.317	1940	1952	1972	rBV	174077	317969	59.91%	7.347%
13	7.629	2040	2049	2065	rBV	24918	46635	8.79%	1.078%
14	7.976	2143	2157	2177	rBV	314637	530745	100.00%	12.264%
15	8.092	2181	2193	2241	rBV	160291	420126	79.16%	9.708%
16	8.854	2419	2430	2450	rBV	205400	345583	65.11%	7.985%
17	10.217	2842	2854	2872	rBV	72408	120400	22.69%	2.782%
18	11.249	3165	3175	3194	rBV	199620	314501	59.26%	7.267%
19	11.625	3281	3292	3307	rBV	173510	280591	52.87%	6.484%
20	14.040	4036	4043	4052	rVB3	3286	5590	1.05%	0.129%




Sum of corrected areas: 4327708

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024505.D
Acq On : 28 Jan 2022 22:41
Operator : SY/MD
Sample : N1328-15 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

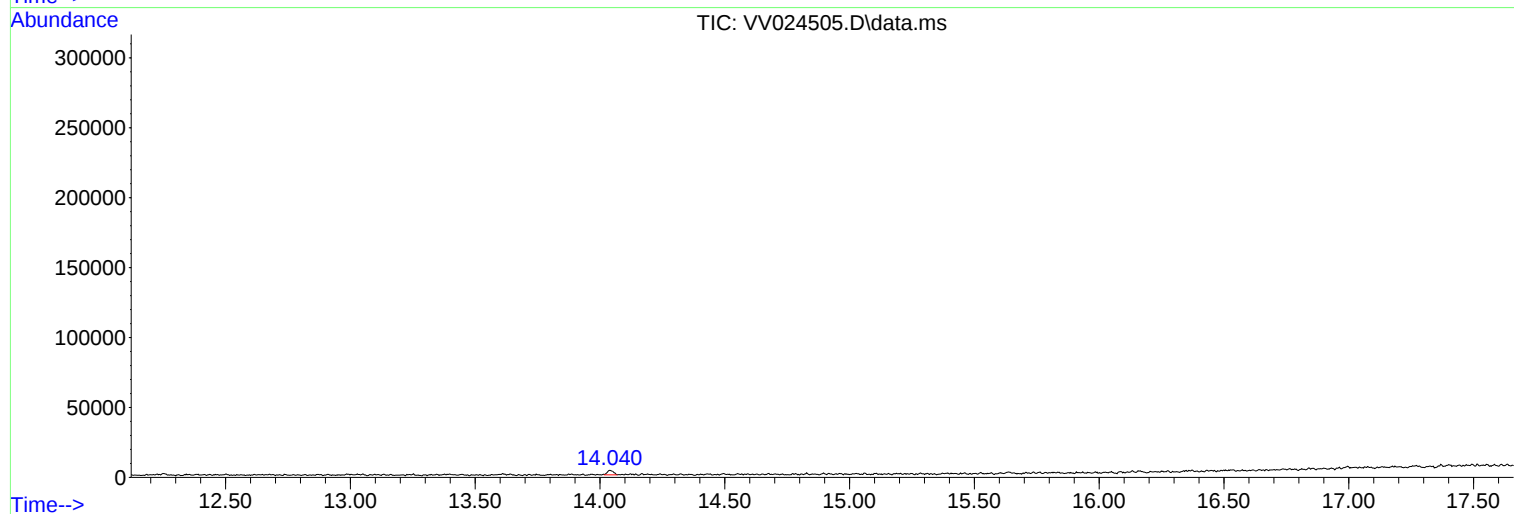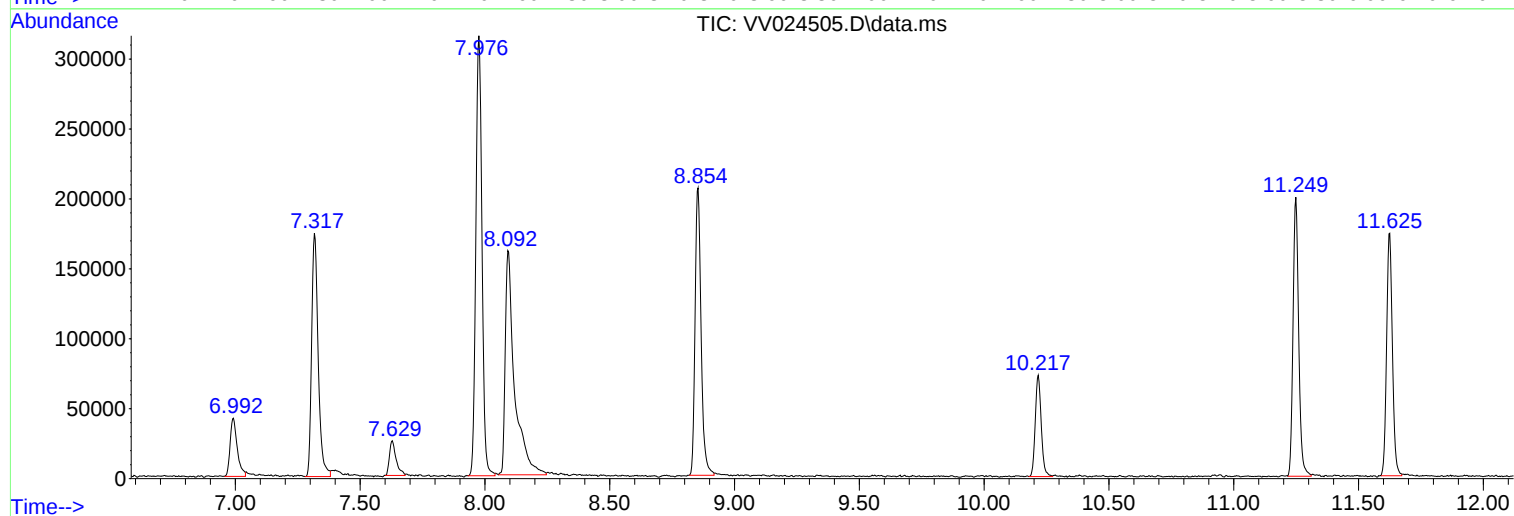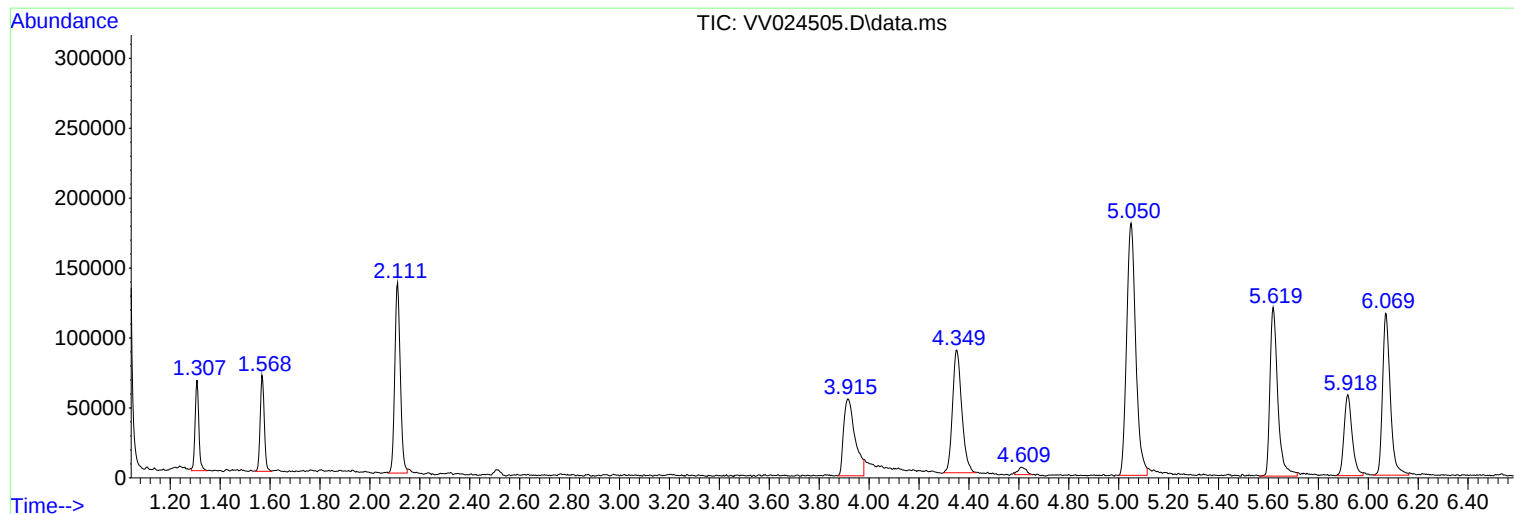

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024505.D
Acq On : 28 Jan 2022 22:41
Operator : SY/MD
Sample : N1328-15 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024505.D
Acq On : 28 Jan 2022 22:41
Operator : SY/MD
Sample : N1328-15 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc