

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024506.D
 Acq On : 28 Jan 2022 23:04
 Operator : SY/MD
 Sample : N1328-16 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0HN5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024506.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	64507	65600	14.90%	1.849%
2	1.568	156	164	176	rBV	65856	77407	17.58%	2.181%
3	2.111	321	333	348	rVB	120760	176716	40.14%	4.980%
4	2.506	449	456	467	rVB3	4588	7848	1.78%	0.221%
5	3.912	883	893	920	rBV2	30668	120120	27.28%	3.385%
6	4.349	1013	1029	1050	rBV	85500	217280	49.35%	6.123%
7	5.050	1230	1247	1269	rBV3	171144	440296	100.00%	12.407%
8	5.619	1411	1424	1448	rBV	125999	270462	61.43%	7.621%
9	5.918	1506	1517	1529	rBV	8156	19876	4.51%	0.560%
10	6.072	1552	1565	1584	rBV	109928	230102	52.26%	6.484%
11	6.992	1840	1851	1870	rBV	40610	81408	18.49%	2.294%
12	7.317	1940	1952	1971	rBV	168253	306933	69.71%	8.649%
13	7.628	2039	2049	2064	rBV2	22633	45670	10.37%	1.287%
14	7.976	2146	2157	2168	rBV9	5666	10165	2.31%	0.286%
15	8.091	2183	2193	2233	rBV	157279	394386	89.57%	11.113%
16	8.853	2419	2430	2445	rBV	213746	359258	81.59%	10.124%
17	10.217	2841	2854	2866	rBV	70961	114528	26.01%	3.227%
18	11.249	3164	3175	3194	rBV	207459	329636	74.87%	9.289%
19	11.625	3278	3292	3306	rBV	166501	273714	62.17%	7.713%
20	14.040	4033	4043	4051	rBV2	3809	7322	1.66%	0.206%


Sum of corrected areas: 3548727

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024506.D
Acq On : 28 Jan 2022 23:04
Operator : SY/MD
Sample : N1328-16 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

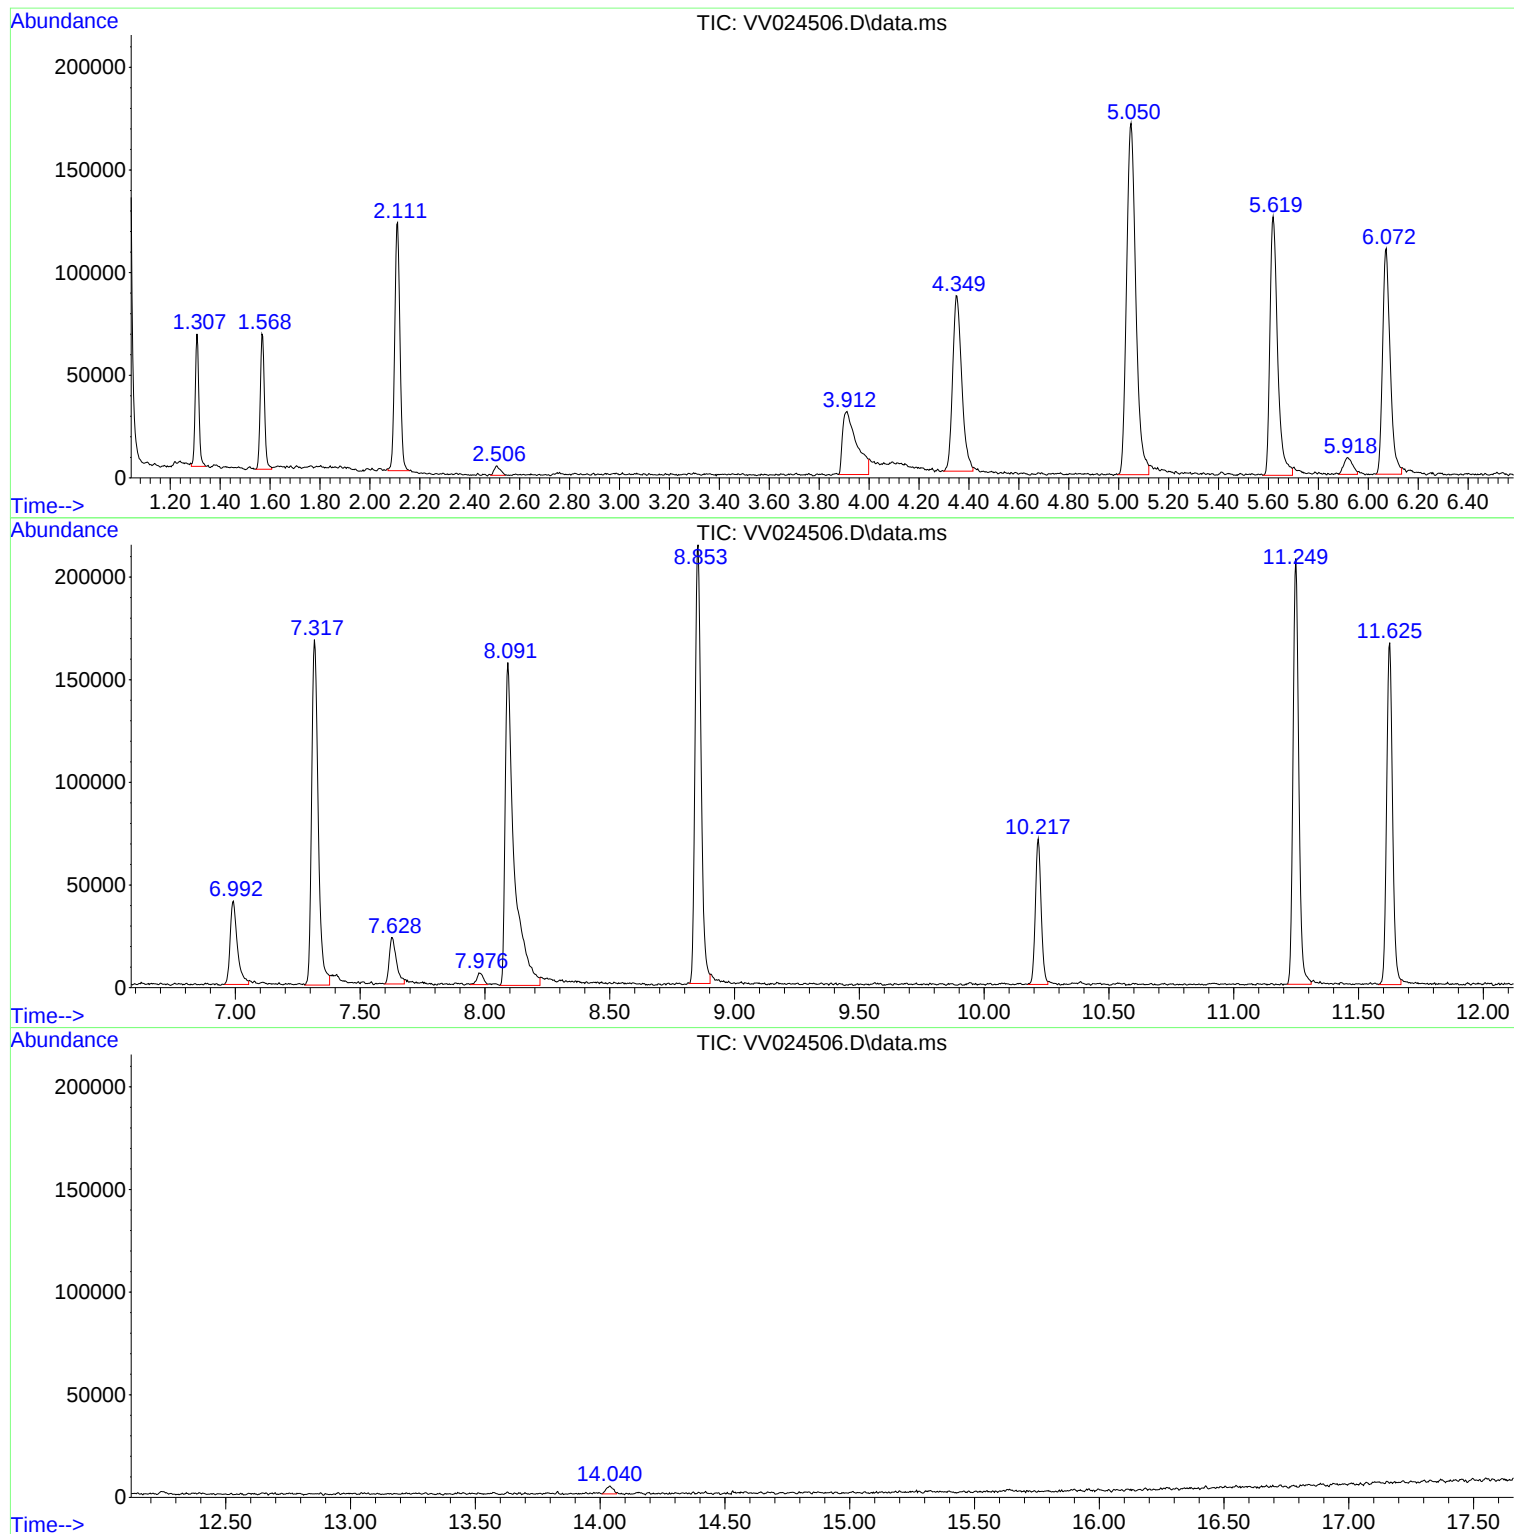

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024506.D
Acq On : 28 Jan 2022 23:04
Operator : SY/MD
Sample : N1328-16 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024506.D
Acq On : 28 Jan 2022 23:04
Operator : SY/MD
Sample : N1328-16 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc