

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024509.D
 Acq On : 29 Jan 2022 00:14
 Operator : SY/MD
 Sample : N1328-19 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COHN8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024509.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	96	rVB	68181	68478	14.57%	1.745%
2	1.568	157	164	178	rVB	67334	77837	16.56%	1.984%
3	2.111	322	333	354	rVB	124848	191141	40.66%	4.872%
4	2.510	450	457	467	rVB8	4160	6916	1.47%	0.176%
5	3.915	881	894	918	rBV3	54131	180415	38.38%	4.599%
6	4.352	1013	1030	1055	rVB	89290	234721	49.94%	5.983%
7	5.050	1230	1247	1272	rBV2	183807	470045	100.00%	11.981%
8	5.619	1413	1424	1442	rBV	122550	254338	54.11%	6.483%
9	5.921	1505	1518	1538	rBV6	25836	62561	13.31%	1.595%
10	6.069	1552	1564	1587	rBV	114473	244635	52.05%	6.236%
11	6.989	1841	1850	1870	rBV	42989	85520	18.19%	2.180%
12	7.317	1937	1952	1970	rBV	179689	322470	68.60%	8.220%
13	7.629	2038	2049	2064	rBV	26208	51689	11.00%	1.318%
14	7.976	2145	2157	2177	rBV	90905	155638	33.11%	3.967%
15	8.092	2181	2193	2227	rBV	163631	414588	88.20%	10.568%
16	8.854	2417	2430	2449	rBV	209757	363985	77.44%	9.278%
17	10.217	2842	2854	2871	rBV2	74620	123809	26.34%	3.156%
18	11.249	3162	3175	3194	rBV	201587	326030	69.36%	8.310%
19	11.625	3279	3292	3307	rBV	180680	288404	61.36%	7.351%




Sum of corrected areas: 3923220

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024509.D
Acq On : 29 Jan 2022 00:14
Operator : SY/MD
Sample : N1328-19 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COHN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

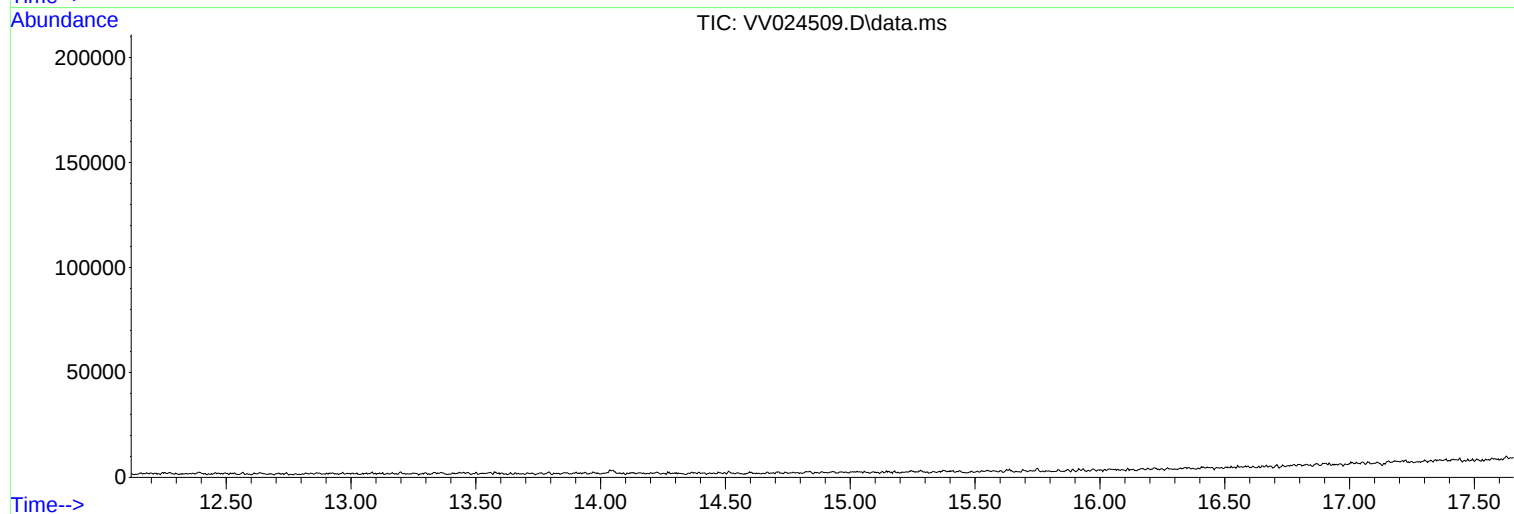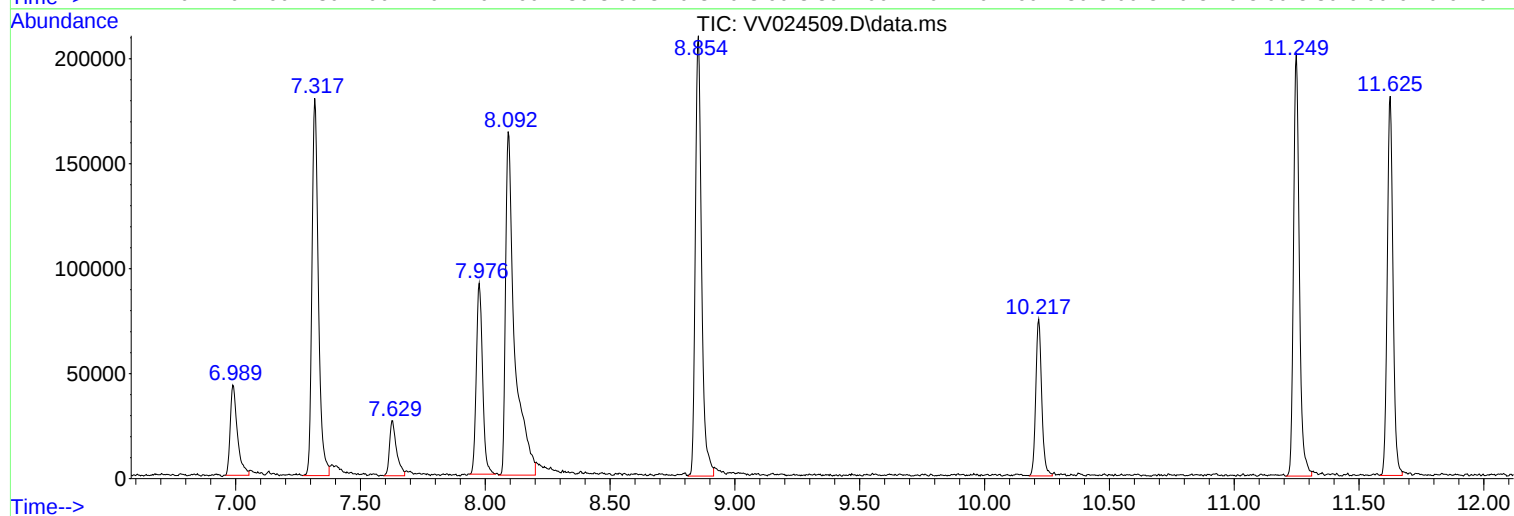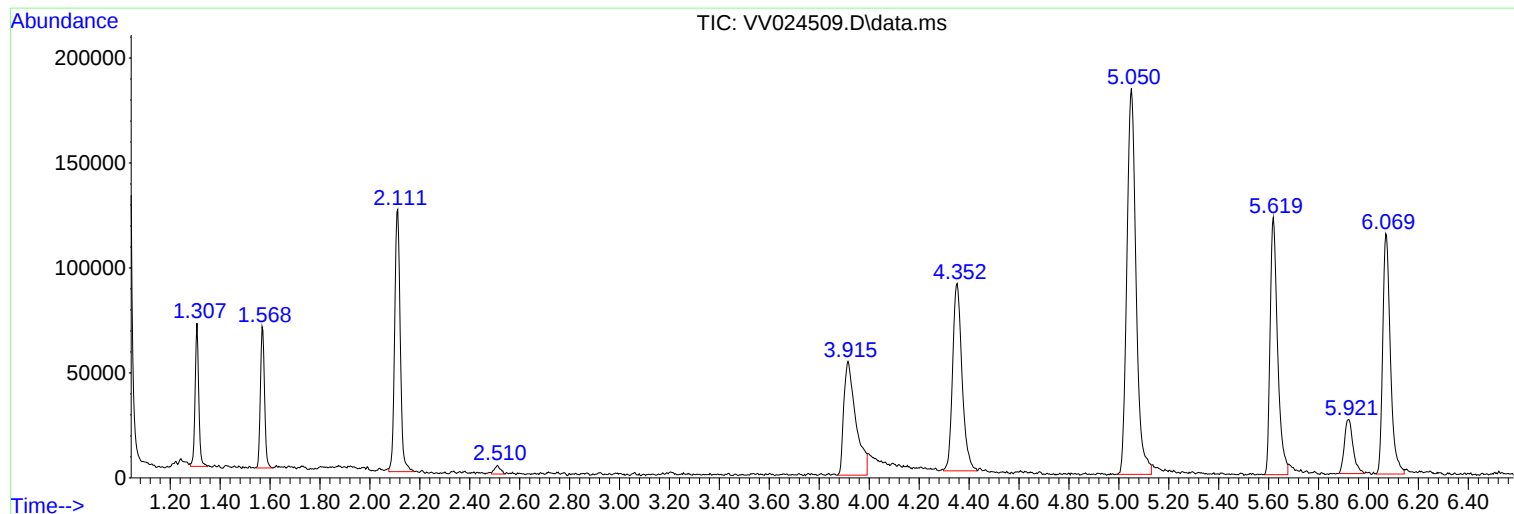

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024509.D
Acq On : 29 Jan 2022 00:14
Operator : SY/MD
Sample : N1328-19 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0HN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
Data File : VV024509.D
Acq On : 29 Jan 2022 00:14
Operator : SY/MD
Sample : N1328-19 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COHN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
