
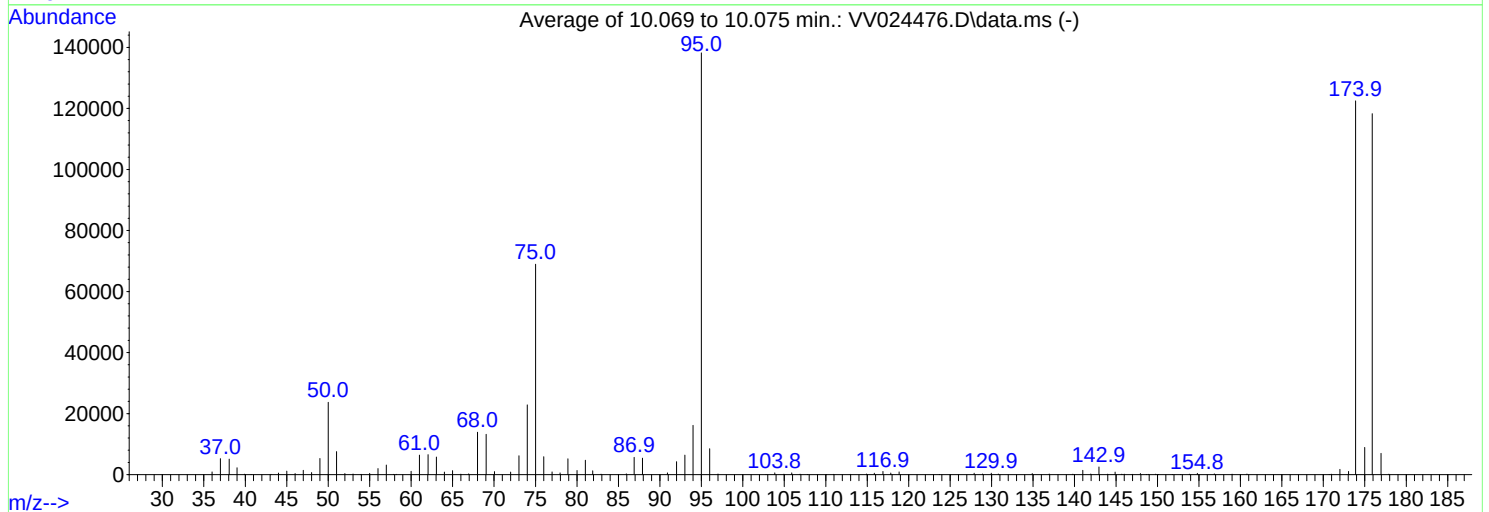


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012822\
 Data File : VV024476.D
 Acq On : 28 Jan 2022 08:55
 Operator : SY/MD
 Sample : BFB265
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB265

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Jan 29 03:50:16 2022

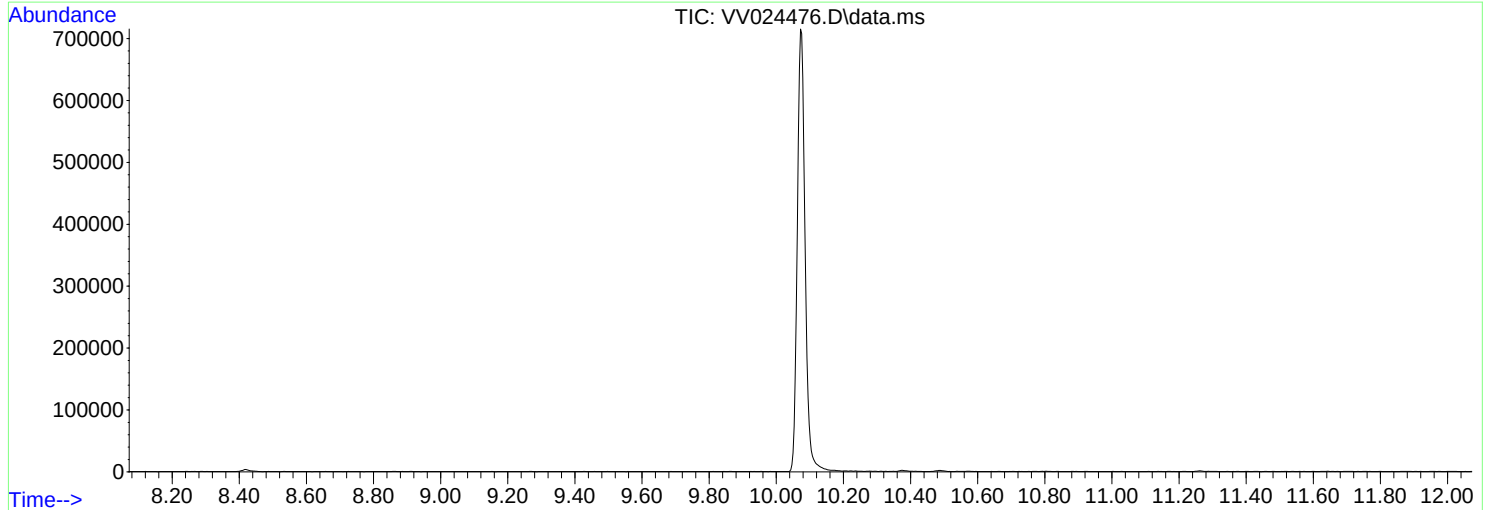

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	23707	PASS
75	95	30	80	49.9	68973	PASS
95	95	100	100	100.0	138216	PASS
96	95	5	9	6.2	8526	PASS
173	174	0.00	2	0.9	1066	PASS
174	95	50	120	88.6	122480	PASS
175	174	5	9	7.3	8917	PASS
176	174	95	105	96.6	118309	PASS
177	176	5	10	5.9	6991	PASS

m/z	Abundance
39.90	148.0
44.00	410.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
36.00	946.0
37.00	5177.0
38.10	4762.0
39.00	2130.0
39.90	312.0
43.10	152.0
44.00	934.0
45.00	1138.0
46.00	316.0
47.00	1454.0
48.00	674.0
49.00	5029.0
50.00	22616.0
51.00	7164.0
52.00	368.0
53.00	182.0
54.00	113.0
55.00	387.0
56.00	1888.0
57.00	2844.0
57.90	190.0
60.00	1075.0
61.00	6189.0
62.10	6465.0
63.00	5630.0
64.00	775.0
65.00	1127.0
66.00	183.0
67.00	301.0
68.00	13345.0
69.10	12536.0
70.00	1032.0
72.00	762.0
73.00	5904.0
74.00	21648.0
75.00	65744.0
76.00	5806.0
77.00	869.0
78.00	620.0
78.90	5037.0
80.00	1326.0
81.00	4569.0
81.90	1197.0
82.90	133.0
86.10	205.0
86.90	5314.0
87.90	5002.0
90.90	568.0
92.00	4099.0
93.00	5953.0
94.00	15271.0
95.00	130232.0
96.00	8242.0
97.00	212.0
103.80	594.0
105.00	174.0
105.90	544.0
106.90	112.0
111.00	162.0
112.90	137.0
114.90	213.0
115.90	410.0
116.90	995.0
117.80	471.0
118.80	845.0
123.70	110.0
127.90	443.0
128.90	199.0
129.90	434.0
130.80	209.0
134.90	368.0
137.00	183.0
139.80	169.0
141.00	1335.0
142.00	256.0
142.90	2483.0
144.00	188.0
144.90	820.0
146.00	256.0
146.90	113.0
147.90	352.0
148.70	141.0
149.80	118.0
150.10	113.0
151.80	117.0
153.80	113.0
154.80	342.0
156.90	290.0
159.00	186.0
160.80	189.0
171.00	296.0
172.00	1562.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

173.00	1555.0
173.90	113120.0
175.00	8019.0
175.90	110088.0
177.00	6691.0
177.90	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
36.00	928.0
37.00	5435.0
38.00	5256.0
39.00	2347.0
40.00	330.0
43.10	135.0
44.00	962.0
45.00	1222.0
46.00	386.0
47.00	1388.0
48.00	718.0
49.00	5549.0
50.00	24528.0
51.00	7856.0
52.00	384.0
53.00	202.0
53.90	108.0
55.00	443.0
56.00	2037.0
57.00	3259.0
57.90	159.0
58.20	154.0
60.00	1150.0
61.00	6705.0
62.00	6743.0
63.00	6028.0
64.00	854.0
65.00	1395.0
66.00	188.0
66.90	292.0
68.00	14374.0
69.00	13606.0
70.10	1003.0
72.00	845.0
73.00	6414.0
74.00	23512.0
75.00	71264.0
76.00	6019.0
77.00	929.0
77.90	605.0
78.90	5479.0
80.00	1406.0
81.00	4883.0
81.90	1271.0
82.90	174.0
85.90	282.0
86.90	5900.0
87.90	5539.0
90.90	643.0
92.00	4411.0
93.00	6580.0
94.00	16648.0
95.00	142976.0
96.00	8787.0
97.00	242.0
103.80	601.0
105.00	166.0
105.90	591.0
106.90	139.0
110.10	111.0
110.90	131.0
113.00	139.0
114.90	238.0
115.80	474.0
116.90	1074.0
117.80	557.0
118.90	922.0
123.70	108.0
127.90	488.0
128.90	199.0
129.90	465.0
130.80	247.0
134.90	386.0
136.90	206.0
139.80	166.0
141.00	1478.0
142.00	255.0
142.90	2680.0
144.00	196.0
144.90	875.0
145.70	230.0
146.00	245.0
147.00	127.0
147.90	368.0
148.90	132.0
149.80	164.0
151.80	112.0
153.90	142.0
154.80	411.0
156.80	279.0
159.00	189.0
160.80	253.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

170.90	247.0
172.00	1823.0
173.10	1642.0
173.90	126576.0
175.00	9240.0
175.90	122224.0
177.00	7096.0
177.90	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
36.00	866.0
37.00	5188.0
38.00	5194.0
39.00	2261.0
40.00	342.0
40.70	107.0
44.00	953.0
45.00	1171.0
46.00	366.0
47.00	1468.0
48.00	660.0
49.00	5404.0
50.00	23976.0
51.00	7601.0
52.00	384.0
53.00	204.0
53.90	133.0
55.00	446.0
56.00	1979.0
57.00	3352.0
58.20	155.0
60.00	1142.0
61.00	6354.0
62.00	6437.0
63.10	5664.0
64.00	856.0
65.00	1462.0
66.00	167.0
66.90	274.0
68.00	14009.0
69.00	13444.0
70.00	938.0
72.00	840.0
73.00	6211.0
74.00	23496.0
75.00	69912.0
76.00	5721.0
77.00	918.0
78.00	507.0
78.90	5094.0
80.00	1398.0
81.00	4790.0
81.90	1255.0
82.90	168.0
85.90	368.0
86.90	5806.0
87.90	5630.0
90.90	593.0
92.00	4201.0
93.00	6688.0
94.00	16592.0
95.00	141440.0
96.00	8549.0
97.00	260.0
102.80	131.0
103.90	566.0
104.90	172.0
105.90	617.0
106.90	174.0
107.80	109.0
110.10	118.0
111.00	101.0
113.00	115.0
114.90	227.0
115.90	525.0
116.90	1056.0
117.90	576.0
118.90	982.0
127.90	452.0
128.90	236.0
130.00	503.0
130.80	259.0
134.90	366.0
136.90	208.0
139.80	130.0
141.00	1494.0
141.90	199.0
143.00	2469.0
144.00	180.0
144.90	804.0
145.70	226.0
147.00	114.0
148.00	336.0
149.00	131.0
149.80	202.0
152.80	101.0
153.90	153.0
154.80	470.0
156.80	257.0
159.00	168.0
160.80	245.0
170.70	259.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

172.00	1834.0
173.90	127744.0
175.00	9491.0
175.90	122616.0
176.90	7185.0
177.90	191.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265