
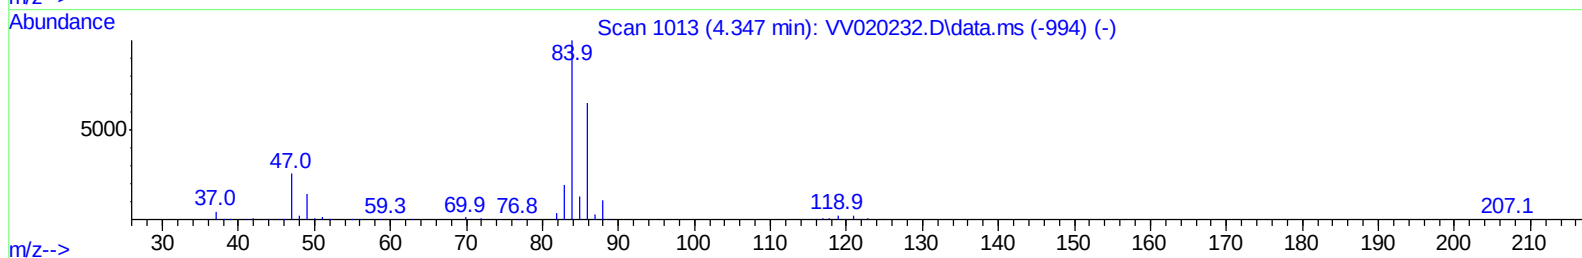
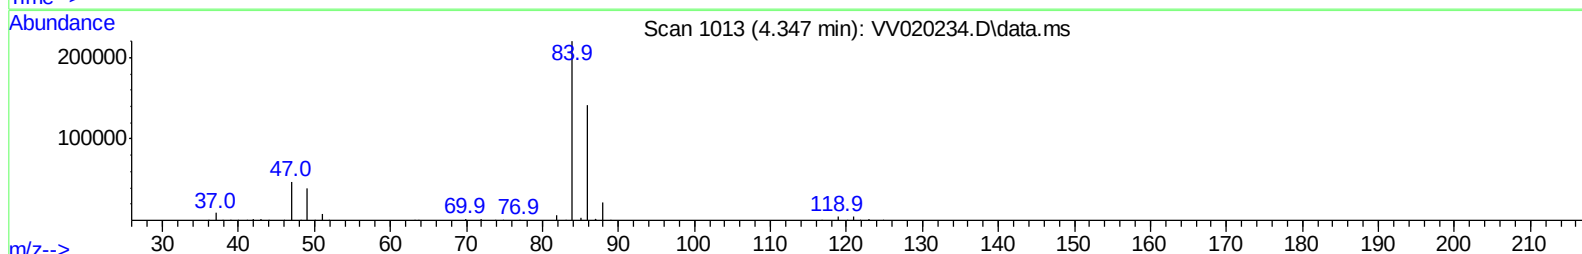


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020234.D
Acq On : 02 Feb 2021 13:43
Operator : SY/MD
Sample : M1258-19 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 02:28:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 03 02:27:31 2021
Response via : Initial Calibration

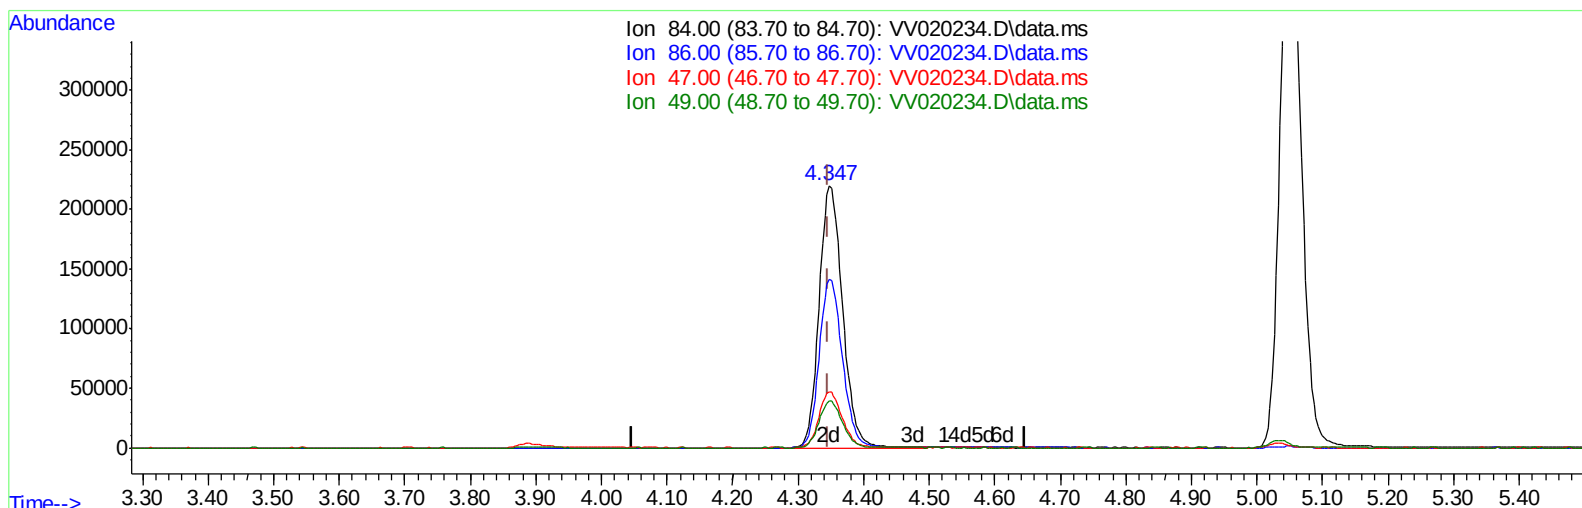

TIC: VV020234.D\data.ms

(24) Chloroform-d (S)

4.347min (+ 0.000) 48.51 ug/L m

response 544413

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.60	0.02#
47.00	46.50	0.02#
49.00	28.00	0.01#