

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020233.D
 Acq On : 02 Feb 2021 12:57
 Operator : SY/MD
 Sample : VV0202WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

Signal : TIC: VV020233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	84	rVB	510100	502439	15.22%	1.914%
2	1.569	142	149	159	rVB	402031	445887	13.51%	1.699%
3	2.110	306	317	345	rBV	729912	1100650	33.34%	4.194%
4	2.261	362	364	366	rVB3	1710	715	0.02%	0.003%
5	2.512	437	442	451	rVB7	3674	4620	0.14%	0.018%
6	2.711	500	504	506	rBV4	673	500	0.02%	0.002%
7	2.753	513	517	519	rBV3	1311	994	0.03%	0.004%
8	2.814	534	536	540	rVB3	822	536	0.02%	0.002%
9	2.878	553	556	558	rBV3	1309	705	0.02%	0.003%
10	2.897	558	562	564	rVV4	913	665	0.02%	0.003%
11	2.926	568	571	575	rVB5	768	546	0.02%	0.002%
12	2.994	589	592	593	rBV2	972	465	0.01%	0.002%
13	3.036	602	605	610	rBV4	927	1049	0.03%	0.004%
14	3.177	646	649	652	rBV4	1111	788	0.02%	0.003%
15	3.306	686	689	690	rBV4	994	582	0.02%	0.002%
16	3.367	705	708	713	rBV3	954	805	0.02%	0.003%
17	3.431	726	728	734	rBV5	1245	997	0.03%	0.004%
18	3.486	741	745	746	rBV2	827	503	0.02%	0.002%
19	3.618	779	786	789	rBV5	985	1022	0.03%	0.004%
20	3.669	798	802	805	rBV3	1042	827	0.03%	0.003%
21	3.894	860	872	912	rBV	215610	671377	20.33%	2.558%
22	4.354	997	1015	1047	rBV	536473	1329862	40.28%	5.067%
23	4.666	1110	1112	1120	rVB7	2261	2162	0.07%	0.008%
24	4.830	1161	1163	1169	rVB6	914	869	0.03%	0.003%
25	4.942	1195	1198	1200	rBV3	642	538	0.02%	0.002%
26	5.052	1213	1232	1257	rBV2	1287273	3301597	100.00%	12.580%
27	5.351	1321	1325	1329	rBV7	1146	1322	0.04%	0.005%
28	5.421	1345	1347	1353	rBV5	912	573	0.02%	0.002%
29	5.466	1358	1361	1365	rBV6	966	985	0.03%	0.004%
30	5.621	1395	1409	1440	rBV	1120584	2250931	68.18%	8.577%
31	5.910	1489	1499	1513	rVB3	27709	58918	1.78%	0.224%
32	6.007	1527	1529	1532	rBV4	987	579	0.02%	0.002%
33	6.074	1536	1550	1580	rVV	730568	1485421	44.99%	5.660%
34	6.482	1674	1677	1679	rBV	873	485	0.01%	0.002%
35	6.589	1705	1710	1712	rBV5	633	709	0.02%	0.003%
36	6.617	1715	1719	1720	rBV	1103	607	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020233.D
 Acq On : 02 Feb 2021 12:57
 Operator : SY/MD
 Sample : VV0202WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis

37	6.736	1752	1756	1760	rBV5	994	738	0.02%	0.003%
38	6.772	1764	1767	1771	rBV3	1223	1204	0.04%	0.005%
39	6.807	1776	1778	1782	rVB2	920	567	0.02%	0.002%
40	6.830	1782	1785	1788	rBV4	1048	747	0.02%	0.003%
41	6.916	1809	1812	1816	rBV4	624	573	0.02%	0.002%
42	6.990	1819	1835	1863	rBV	408094	752128	22.78%	2.866%
43	7.318	1924	1937	1963	rBV	1532617	2673566	80.98%	10.187%
44	7.624	2022	2032	2059	rBV	283478	506604	15.34%	1.930%
45	7.826	2092	2095	2097	rVB4	1644	947	0.03%	0.004%
46	8.093	2167	2178	2212	rBV	827238	1497498	45.36%	5.706%
47	8.412	2275	2277	2281	rVV3	825	509	0.02%	0.002%
48	8.434	2281	2284	2291	rVB6	1570	1775	0.05%	0.007%
49	8.617	2338	2341	2347	rVB6	1198	1291	0.04%	0.005%
50	8.650	2347	2351	2352	rBV2	588	438	0.01%	0.002%
51	8.685	2357	2362	2365	rBV4	589	547	0.02%	0.002%
52	8.714	2369	2371	2375	rVB4	828	553	0.02%	0.002%
53	8.746	2375	2381	2382	rBV2	796	730	0.02%	0.003%
54	8.768	2386	2388	2392	rVB3	848	453	0.01%	0.002%
55	8.855	2400	2415	2438	rBV	1711461	2773088	83.99%	10.566%
56	9.212	2524	2526	2528	rBV4	912	560	0.02%	0.002%
57	9.248	2534	2537	2540	rVB4	910	633	0.02%	0.002%
58	9.363	2571	2573	2577	rBV4	753	469	0.01%	0.002%
59	9.466	2602	2605	2611	rVB5	1785	1463	0.04%	0.006%
60	9.495	2611	2614	2616	rBV	608	430	0.01%	0.002%
61	9.511	2616	2619	2621	rBV4	732	417	0.01%	0.002%
62	9.550	2629	2631	2633	rBV3	985	422	0.01%	0.002%
63	9.633	2654	2657	2661	rVB4	1446	1300	0.04%	0.005%
64	9.666	2661	2667	2668	rBV4	761	644	0.02%	0.002%
65	9.740	2688	2690	2694	rVB4	627	434	0.01%	0.002%
66	9.772	2697	2700	2701	rBV2	881	460	0.01%	0.002%
67	9.810	2708	2712	2715	rBV3	469	427	0.01%	0.002%
68	9.855	2722	2726	2730	rVB4	888	725	0.02%	0.003%
69	9.894	2730	2738	2740	rBV3	755	787	0.02%	0.003%
70	10.158	2817	2820	2823	rBV4	745	574	0.02%	0.002%
71	10.222	2828	2840	2857	rBV	894490	1390133	42.10%	5.297%
72	10.347	2877	2879	2882	rVB4	1119	476	0.01%	0.002%
73	10.405	2894	2897	2899	rBV3	937	588	0.02%	0.002%
74	10.463	2913	2915	2919	rVB4	642	456	0.01%	0.002%
75	10.485	2919	2922	2924	rBV2	953	695	0.02%	0.003%
76	10.543	2938	2940	2942	rBV3	727	430	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020233.D
 Acq On : 02 Feb 2021 12:57
 Operator : SY/MD
 Sample : VV0202WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

77	10.797	3014	3019	3024	rBV6	1252	1309	0.04%	0.005%
78	10.846	3030	3034	3036	rBV4	1039	758	0.02%	0.003%
79	10.932	3057	3061	3063	rVB4	1235	893	0.03%	0.003%
80	11.003	3081	3083	3089	rBV5	884	1049	0.03%	0.004%
81	11.051	3094	3098	3102	rBV4	1117	951	0.03%	0.004%
82	11.080	3102	3107	3111	rVB8	950	970	0.03%	0.004%
83	11.164	3130	3133	3134	rBV2	1316	721	0.02%	0.003%
84	11.254	3149	3161	3193	rBV	1855829	2813782	85.22%	10.721%
85	11.508	3236	3240	3241	rBV4	933	676	0.02%	0.003%
86	11.630	3265	3278	3301	rBV	1669820	2612529	79.13%	9.954%
87	12.103	3422	3425	3428	rBV4	1094	751	0.02%	0.003%
88	12.292	3481	3484	3486	rBV3	1021	698	0.02%	0.003%
89	12.373	3506	3509	3518	rVB6	1812	2051	0.06%	0.008%
90	12.460	3531	3536	3538	rBV2	500	463	0.01%	0.002%
91	12.518	3550	3554	3560	rVB3	341	455	0.01%	0.002%
92	12.556	3560	3566	3568	rBV3	523	622	0.02%	0.002%
93	12.656	3591	3597	3603	rBV7	2484	3142	0.10%	0.012%
94	13.112	3733	3739	3745	rBV4	701	1017	0.03%	0.004%
95	13.273	3780	3789	3790	rBV5	3397	3407	0.10%	0.013%
96	13.524	3860	3867	3872	rVV6	2086	2793	0.08%	0.011%
97	13.755	3933	3939	3949	rBV9	3867	4827	0.15%	0.018%
98	13.845	3964	3967	3971	rVB5	804	614	0.02%	0.002%
99	13.945	3996	3998	4001	rVB5	1127	587	0.02%	0.002%
100	14.524	4176	4178	4185	rBV8	1177	1137	0.03%	0.004%




Sum of corrected areas: 26244911

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020233.D
Acq On : 02 Feb 2021 12:57
Operator : SY/MD
Sample : VV0202WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

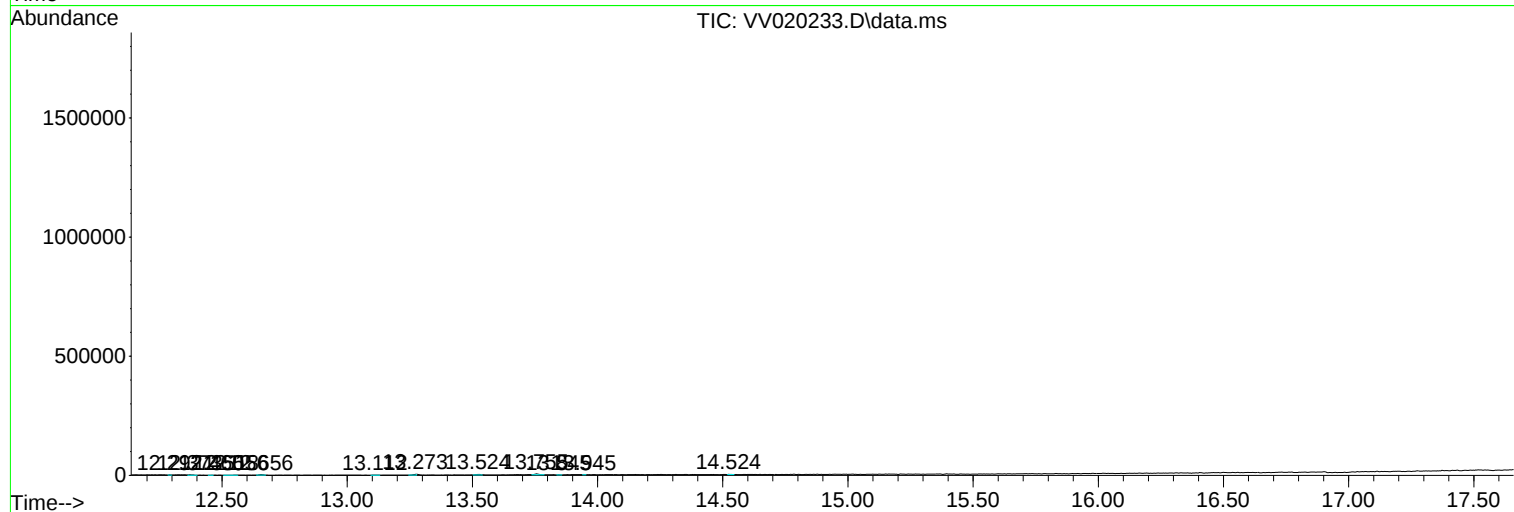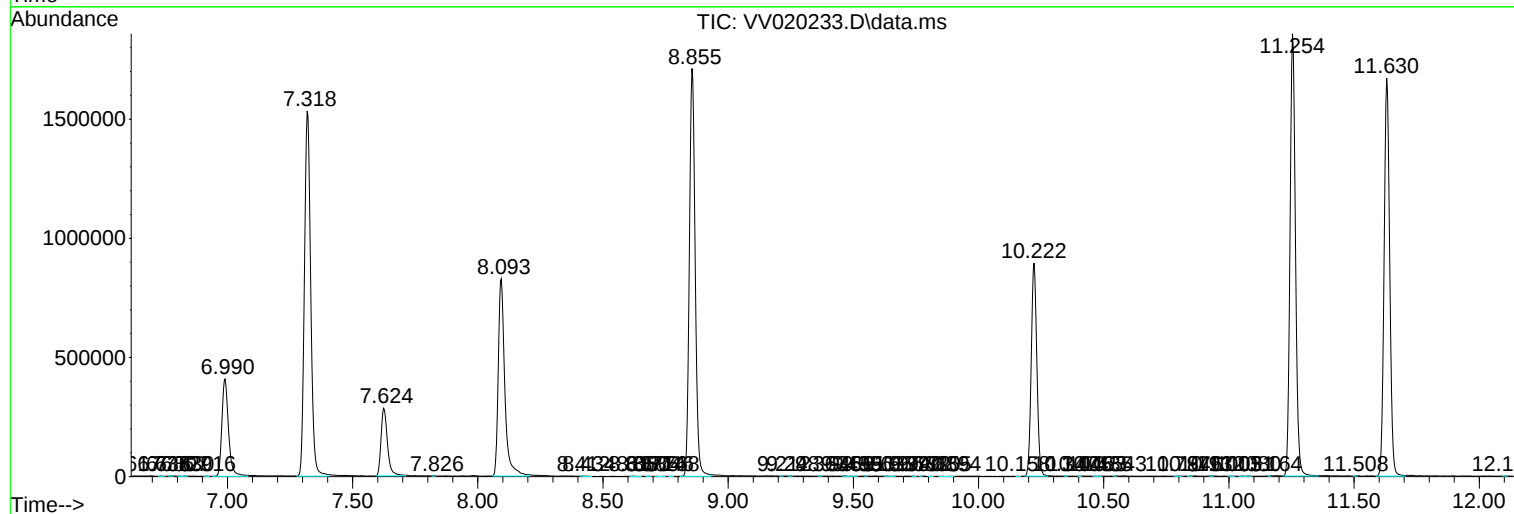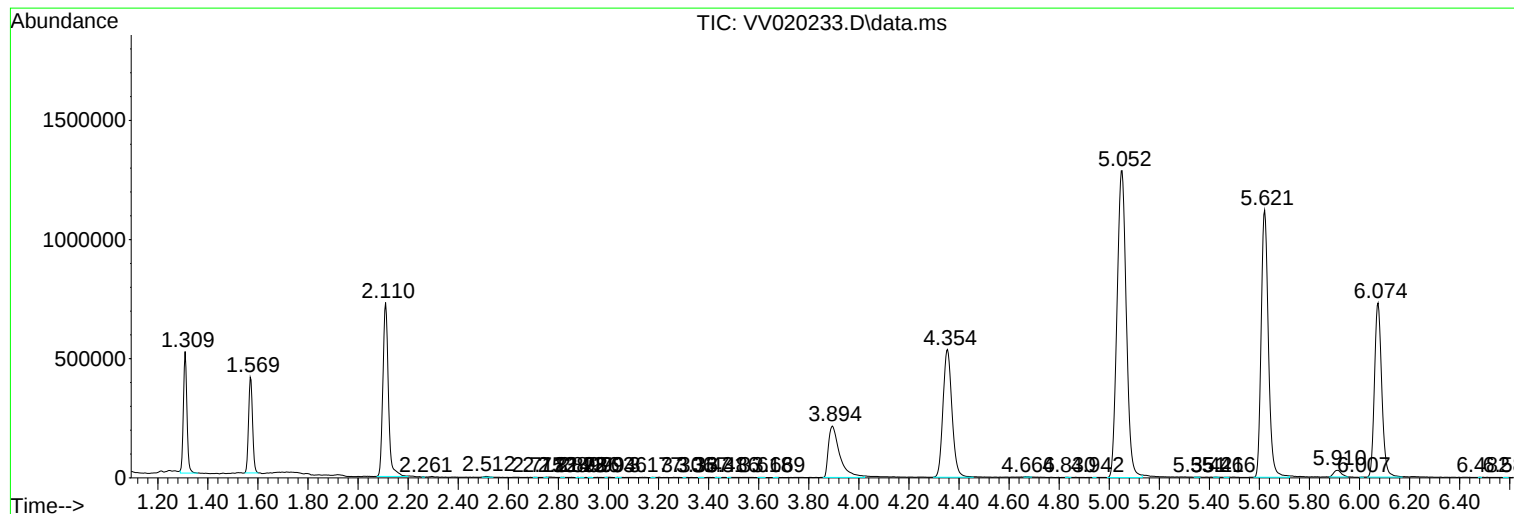

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020233.D
Acq On : 02 Feb 2021 12:57
Operator : SY/MD
Sample : VV0202WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020233.D
Acq On : 02 Feb 2021 12:57
Operator : SY/MD
Sample : VV0202WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
