

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020234.D
 Acq On : 02 Feb 2021 13:43
 Operator : SY/MD
 Sample : M1258-19 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG531

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

Signal : TIC: VV020234.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	89	rVB	432856	451798	14.04%	1.925%
2	1.569	142	149	162	rVB	366707	409963	12.74%	1.747%
3	2.110	305	317	345	rBV	673842	1024051	31.83%	4.364%
4	2.296	370	375	378	rBV2	3708	3930	0.12%	0.017%
5	2.515	436	443	446	rBV7	2755	3391	0.11%	0.014%
6	2.672	490	492	494	rBV2	745	392	0.01%	0.002%
7	2.721	504	507	508	rBV3	944	432	0.01%	0.002%
8	2.868	550	553	555	rBV3	838	639	0.02%	0.003%
9	3.023	596	601	603	rBV4	1337	1203	0.04%	0.005%
10	3.113	625	629	633	rBV5	743	702	0.02%	0.003%
11	3.155	640	642	647	rVB4	797	590	0.02%	0.003%
12	3.180	647	650	653	rBV5	754	523	0.02%	0.002%
13	3.216	658	661	662	rBV2	903	470	0.01%	0.002%
14	3.241	667	669	671	rBV2	809	354	0.01%	0.002%
15	3.296	684	686	689	rBV	586	350	0.01%	0.001%
16	3.354	700	704	706	rBV2	1174	617	0.02%	0.003%
17	3.393	712	716	718	rBV5	812	669	0.02%	0.003%
18	3.434	727	729	732	rBV2	609	394	0.01%	0.002%
19	3.470	737	740	742	rBV4	896	396	0.01%	0.002%
20	3.508	748	752	754	rBV3	892	593	0.02%	0.003%
21	3.608	780	783	786	rBV4	556	457	0.01%	0.002%
22	3.640	789	793	794	rBV3	699	458	0.01%	0.002%
23	3.708	812	814	822	rVB6	1257	1098	0.03%	0.005%
24	3.759	827	830	832	rBV	619	361	0.01%	0.002%
25	3.888	859	870	903	rBV	208276	642396	19.97%	2.738%
26	4.347	995	1013	1039	rBV	518737	1284709	39.93%	5.475%
27	4.724	1128	1130	1135	rBV4	637	495	0.02%	0.002%
28	4.817	1157	1159	1163	rVB5	1170	783	0.02%	0.003%
29	4.852	1168	1170	1176	rVB4	935	818	0.03%	0.003%
30	4.878	1176	1178	1181	rBV3	735	396	0.01%	0.002%
31	4.907	1185	1187	1191	rVB4	1181	617	0.02%	0.003%
32	4.968	1205	1206	1211	rVB2	670	425	0.01%	0.002%
33	5.048	1211	1231	1272	rBV2	1242046	3217479	100.00%	13.711%
34	5.518	1373	1377	1380	rVB5	963	771	0.02%	0.003%
35	5.540	1380	1384	1385	rBV3	1143	795	0.02%	0.003%
36	5.618	1394	1408	1435	rBV	1042093	2100397	65.28%	8.951%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020234.D
 Acq On : 02 Feb 2021 13:43
 Operator : SY/MD
 Sample : M1258-19 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG531

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis

37	5.910	1490	1499	1514	rVB3	19943	41573	1.29%	0.177%
38	6.000	1526	1527	1532	rVB5	1149	725	0.02%	0.003%
39	6.071	1533	1549	1572	rBV	708573	1444984	44.91%	6.158%
40	6.338	1628	1632	1634	rBV4	1396	1233	0.04%	0.005%
41	6.370	1638	1642	1645	rBV3	1286	1051	0.03%	0.004%
42	6.405	1650	1653	1655	rVV4	1041	631	0.02%	0.003%
43	6.418	1655	1657	1660	rVB2	1289	667	0.02%	0.003%
44	6.437	1660	1663	1665	rBV4	940	639	0.02%	0.003%
45	6.479	1674	1676	1679	rBV3	971	414	0.01%	0.002%
46	6.495	1679	1681	1686	rVB5	1147	741	0.02%	0.003%
47	6.563	1700	1702	1705	rVB3	815	378	0.01%	0.002%
48	6.582	1705	1708	1709	rBV2	1086	601	0.02%	0.003%
49	6.608	1713	1716	1719	rBV3	893	876	0.03%	0.004%
50	6.778	1767	1769	1772	rVB3	930	446	0.01%	0.002%
51	6.801	1774	1776	1779	rVB6	1013	478	0.01%	0.002%
52	6.987	1819	1834	1856	rBV	302548	544962	16.94%	2.322%
53	7.315	1924	1936	1969	rBV	1466959	2511159	78.05%	10.701%
54	7.537	2002	2005	2015	rVB4	3196	3710	0.12%	0.016%
55	7.624	2019	2032	2053	rBV	281225	493023	15.32%	2.101%
56	8.023	2153	2156	2157	rBV2	752	461	0.01%	0.002%
57	8.090	2166	2177	2216	rBV	765965	1444433	44.89%	6.155%
58	8.560	2319	2323	2324	rBV3	1232	752	0.02%	0.003%
59	8.598	2333	2335	2339	rVB4	729	369	0.01%	0.002%
60	8.675	2357	2359	2364	rVB4	1426	838	0.03%	0.004%
61	8.723	2371	2374	2380	rVV4	1481	1339	0.04%	0.006%
62	8.855	2401	2415	2446	rBV	1401116	2243368	69.72%	9.560%
63	9.119	2495	2497	2504	rVB4	570	443	0.01%	0.002%
64	9.170	2512	2513	2518	rVB3	677	406	0.01%	0.002%
65	9.225	2527	2530	2532	rBV2	664	335	0.01%	0.001%
66	9.305	2552	2555	2558	rVB2	632	395	0.01%	0.002%
67	9.932	2744	2750	2754	rBV2	517	410	0.01%	0.002%
68	9.981	2761	2765	2769	rBV2	531	493	0.02%	0.002%
69	10.222	2826	2840	2865	rVV	754404	1185201	36.84%	5.051%
70	10.338	2874	2876	2882	rVB4	446	400	0.01%	0.002%
71	10.392	2887	2893	2896	rBV5	406	439	0.01%	0.002%
72	10.482	2918	2921	2928	rVB	368	371	0.01%	0.002%
73	10.514	2928	2931	2935	rBV2	418	380	0.01%	0.002%
74	10.547	2935	2941	2945	rVB2	418	406	0.01%	0.002%
75	10.749	2998	3004	3008	rVB3	542	647	0.02%	0.003%
76	10.775	3008	3012	3017	rBV2	693	643	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020234.D
 Acq On : 02 Feb 2021 13:43
 Operator : SY/MD
 Sample : M1258-19 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG531

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

77	10.858	3034	3038	3042	rBV4	1067	865	0.03%	0.004%
78	10.929	3056	3060	3064	rBV	505	392	0.01%	0.002%
79	11.071	3099	3104	3108	rBB2	544	524	0.02%	0.002%
80	11.186	3138	3140	3142	rBV	666	364	0.01%	0.002%
81	11.254	3149	3161	3188	rBV	1409750	2172134	67.51%	9.256%
82	11.453	3221	3223	3228	rVB3	445	341	0.01%	0.001%
83	11.505	3237	3239	3246	rVB2	444	374	0.01%	0.002%
84	11.630	3264	3278	3301	rBV	1401099	2189072	68.04%	9.329%
85	11.894	3358	3360	3365	rBV3	474	403	0.01%	0.002%
86	12.019	3396	3399	3401	rBV2	644	438	0.01%	0.002%
87	12.067	3411	3414	3418	rBV3	590	529	0.02%	0.002%
88	12.151	3437	3440	3442	rBV	747	505	0.02%	0.002%
89	12.225	3459	3463	3464	rBV2	571	458	0.01%	0.002%
90	12.260	3472	3474	3477	rBV2	995	512	0.02%	0.002%
91	12.357	3500	3504	3505	rBV3	1113	809	0.03%	0.003%
92	12.460	3534	3536	3543	rVB6	815	666	0.02%	0.003%
93	12.653	3593	3596	3599	rBV4	1971	1788	0.06%	0.008%
94	12.881	3664	3667	3671	rBV5	942	871	0.03%	0.004%
95	12.987	3698	3700	3703	rBV3	975	527	0.02%	0.002%
96	13.273	3783	3789	3799	rVB10	3704	5747	0.18%	0.024%
97	13.318	3801	3803	3805	rBV3	928	511	0.02%	0.002%
98	13.759	3936	3940	3944	rVB6	1889	1673	0.05%	0.007%
99	14.254	4090	4094	4098	rBV5	1175	1096	0.03%	0.005%
100	14.688	4226	4229	4232	rBV4	1277	1076	0.03%	0.005%




Sum of corrected areas: 23466407

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020234.D
Acq On : 02 Feb 2021 13:43
Operator : SY/MD
Sample : M1258-19 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

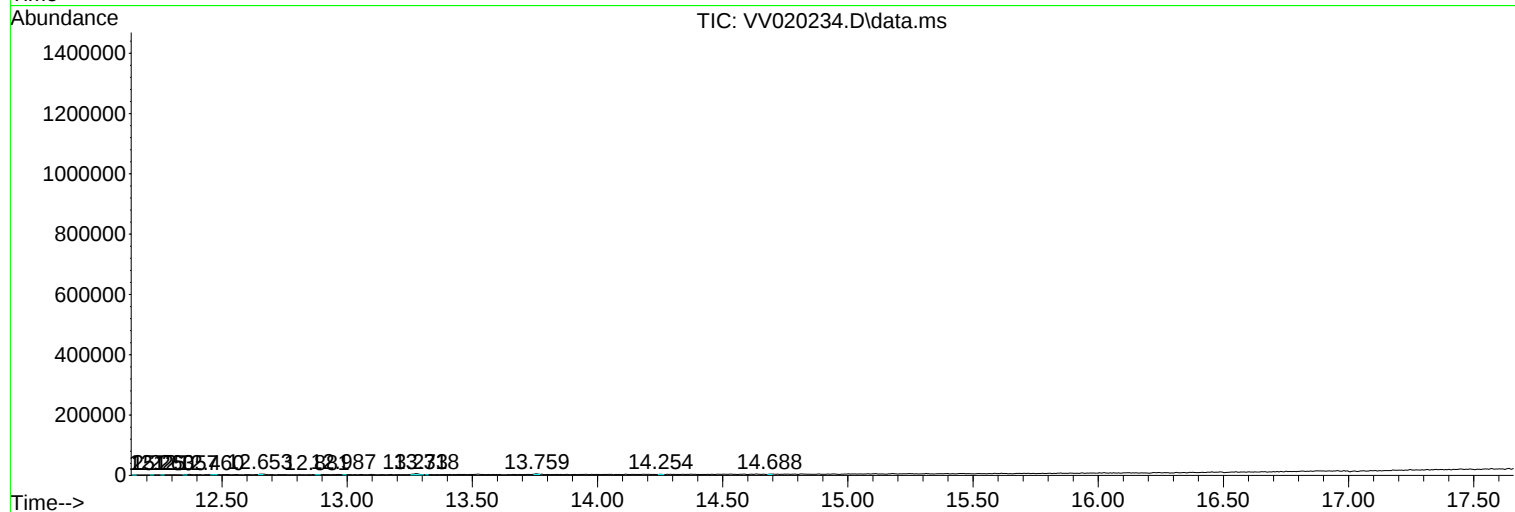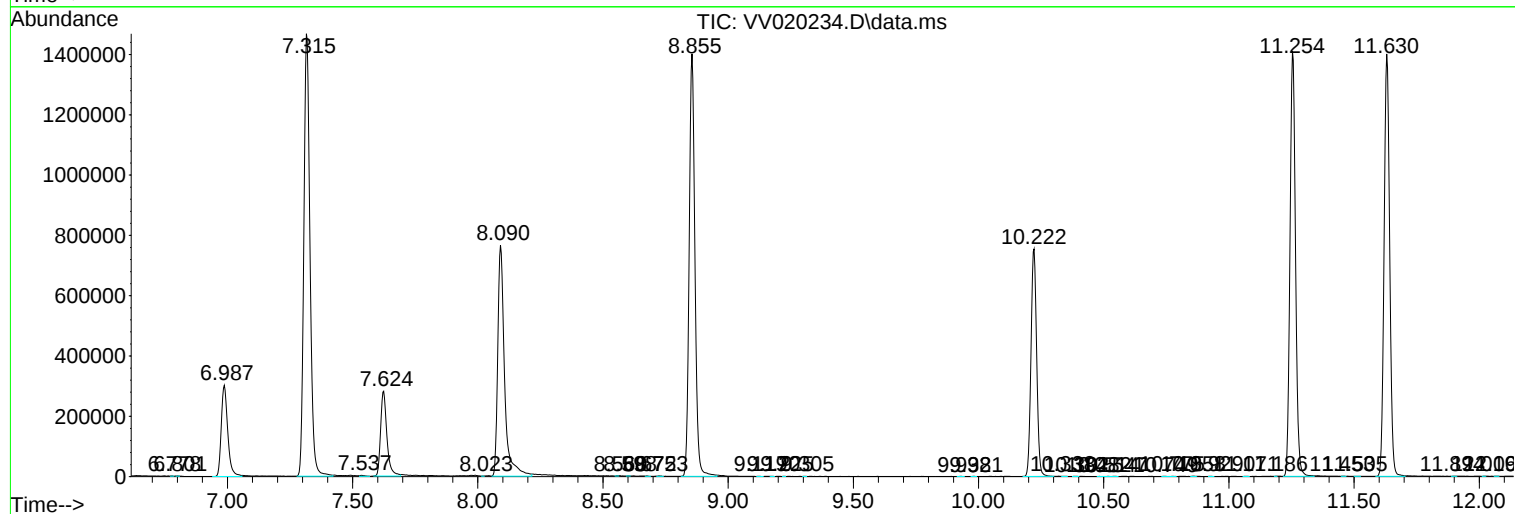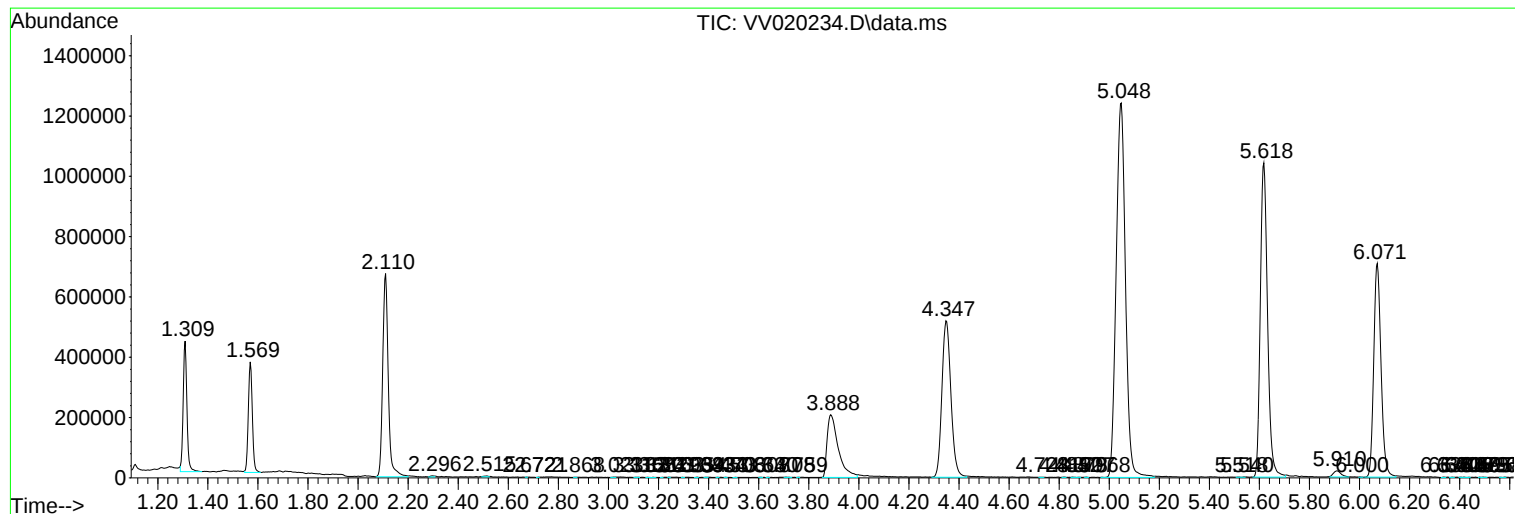

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020234.D
Acq On : 02 Feb 2021 13:43
Operator : SY/MD
Sample : M1258-19 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020234.D
Acq On : 02 Feb 2021 13:43
Operator : SY/MD
Sample : M1258-19 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
