

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020235.D
 Acq On : 02 Feb 2021 14:06
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

Signal : TIC: VV020235.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	80	rVB	410987	416540	13.06%	1.668%
2	1.570	142	149	162	rVB	365137	399125	12.51%	1.598%
3	2.110	306	317	342	rVB	608955	924149	28.97%	3.700%
4	2.518	434	444	452	rVB	4090	8437	0.26%	0.034%
5	2.582	462	464	467	rBV3	853	498	0.02%	0.002%
6	2.688	493	497	499	rBV5	912	650	0.02%	0.003%
7	2.778	520	525	530	rVB7	1685	1478	0.05%	0.006%
8	2.817	534	537	540	rVV5	1252	994	0.03%	0.004%
9	2.846	542	546	550	rVV3	1337	1318	0.04%	0.005%
10	2.952	577	579	583	rVB3	954	523	0.02%	0.002%
11	3.055	609	611	615	rVB2	856	473	0.01%	0.002%
12	3.106	624	627	629	rBV3	837	473	0.01%	0.002%
13	3.377	708	711	714	rBV3	1324	841	0.03%	0.003%
14	3.560	765	768	771	rVV4	1428	992	0.03%	0.004%
15	3.605	778	782	784	rBV2	621	507	0.02%	0.002%
16	3.634	790	791	797	rVB5	990	624	0.02%	0.002%
17	3.772	831	834	835	rBV2	1026	560	0.02%	0.002%
18	3.891	860	871	900	rBV	217158	637836	19.99%	2.554%
19	4.354	999	1015	1043	rBV	513767	1261069	39.53%	5.049%
20	4.553	1075	1077	1080	rBV4	854	676	0.02%	0.003%
21	4.717	1126	1128	1131	rBV4	948	536	0.02%	0.002%
22	4.823	1159	1161	1164	rBV4	892	689	0.02%	0.003%
23	4.968	1204	1206	1211	rVB5	1031	762	0.02%	0.003%
24	5.048	1211	1231	1267	rBV2	1237208	3190289	100.00%	12.773%
25	5.418	1344	1346	1351	rVB5	1573	1070	0.03%	0.004%
26	5.544	1381	1385	1388	rVB6	1089	833	0.03%	0.003%
27	5.621	1395	1409	1439	rBV	1043642	2094538	65.65%	8.386%
28	5.913	1488	1500	1514	rBV5	22099	51282	1.61%	0.205%
29	6.074	1536	1550	1578	rBV	702131	1428251	44.77%	5.718%
30	6.267	1606	1610	1616	rBV6	1327	1214	0.04%	0.005%
31	6.331	1628	1630	1633	rVB3	1279	540	0.02%	0.002%
32	6.357	1633	1638	1641	rBV6	1505	1249	0.04%	0.005%
33	6.418	1655	1657	1662	rVB6	1053	623	0.02%	0.002%
34	6.486	1676	1678	1683	rVB4	1116	832	0.03%	0.003%
35	6.531	1690	1692	1698	rVB4	901	572	0.02%	0.002%
36	6.582	1703	1708	1712	rBV6	1340	1382	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020235.D
 Acq On : 02 Feb 2021 14:06
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis

37	6.601	1712	1714	1718	rVB3	873	542	0.02%	0.002%
38	6.627	1718	1722	1725	rBV5	800	715	0.02%	0.003%
39	6.682	1737	1739	1741	rVB2	1273	539	0.02%	0.002%
40	6.711	1746	1748	1754	rVB6	1498	1052	0.03%	0.004%
41	6.778	1765	1769	1770	rBV3	1429	795	0.02%	0.003%
42	6.846	1784	1790	1793	rBV5	896	1042	0.03%	0.004%
43	6.929	1812	1816	1819	rVB5	1420	1059	0.03%	0.004%
44	6.990	1819	1835	1865	rBV	387424	724674	22.71%	2.901%
45	7.318	1924	1937	1959	rBV	1501513	2574718	80.70%	10.309%
46	7.624	2022	2032	2058	rBV	280798	491760	15.41%	1.969%
47	7.778	2079	2080	2085	rVB5	812	474	0.01%	0.002%
48	7.801	2085	2087	2092	rBV6	1121	1006	0.03%	0.004%
49	7.958	2132	2136	2139	rBV5	637	631	0.02%	0.003%
50	8.090	2167	2177	2218	rVV	803725	1457619	45.69%	5.836%
51	8.367	2261	2263	2270	rVB6	1065	966	0.03%	0.004%
52	8.437	2282	2285	2290	rVB6	1345	1170	0.04%	0.005%
53	8.486	2296	2300	2301	rBV	908	540	0.02%	0.002%
54	8.498	2301	2304	2307	rVV5	973	681	0.02%	0.003%
55	8.569	2322	2326	2334	rVB5	1958	2362	0.07%	0.009%
56	8.621	2334	2342	2354	rVB7	2122	2891	0.09%	0.012%
57	8.679	2354	2360	2361	rBV3	1251	1116	0.03%	0.004%
58	8.807	2397	2400	2403	rBV	1035	790	0.02%	0.003%
59	8.855	2403	2415	2437	rBV	1582191	2529382	79.28%	10.127%
60	9.061	2475	2479	2481	rBV4	959	862	0.03%	0.003%
61	9.093	2487	2489	2493	rBV5	797	534	0.02%	0.002%
62	9.161	2507	2510	2514	rVB4	1273	927	0.03%	0.004%
63	9.241	2533	2535	2540	rVB4	864	631	0.02%	0.003%
64	9.360	2567	2572	2575	rBV3	1129	1072	0.03%	0.004%
65	9.405	2583	2586	2589	rBV4	1095	898	0.03%	0.004%
66	9.588	2640	2643	2648	rVB7	779	563	0.02%	0.002%
67	9.730	2684	2687	2689	rBV4	782	467	0.01%	0.002%
68	9.801	2707	2709	2713	rVB2	1125	590	0.02%	0.002%
69	9.910	2738	2743	2745	rBV4	1293	1010	0.03%	0.004%
70	10.019	2775	2777	2780	rVB3	1078	518	0.02%	0.002%
71	10.096	2796	2801	2807	rBV5	1015	1372	0.04%	0.005%
72	10.222	2827	2840	2866	rVV	954746	1504619	47.16%	6.024%
73	10.415	2896	2900	2903	rBV4	984	773	0.02%	0.003%
74	10.540	2936	2939	2941	rBV4	847	609	0.02%	0.002%
75	10.630	2963	2967	2971	rVB2	677	614	0.02%	0.002%
76	10.656	2971	2975	2978	rBV3	1265	948	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020235.D
 Acq On : 02 Feb 2021 14:06
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

77	10.852	3032	3036	3037	rVV3	1178	823	0.03%	0.003%
78	10.862	3037	3039	3044	rVB5	1617	1303	0.04%	0.005%
79	10.971	3070	3073	3076	rBV4	754	686	0.02%	0.003%
80	11.039	3091	3094	3097	rBV3	827	508	0.02%	0.002%
81	11.077	3102	3106	3109	rBV4	1444	1198	0.04%	0.005%
82	11.119	3117	3119	3123	rBV3	945	736	0.02%	0.003%
83	11.170	3130	3135	3137	rBV4	1706	1506	0.05%	0.006%
84	11.254	3149	3161	3184	rBV	1696591	2620376	82.14%	10.491%
85	11.630	3265	3278	3305	rBV	1663894	2587864	81.12%	10.361%
86	12.209	3456	3458	3463	rVB3	942	647	0.02%	0.003%
87	12.653	3592	3596	3600	rBV5	1540	1667	0.05%	0.007%
88	12.723	3614	3618	3623	rBV4	684	689	0.02%	0.003%
89	12.817	3645	3647	3652	rVB3	693	596	0.02%	0.002%
90	12.839	3652	3654	3658	rBV3	869	556	0.02%	0.002%
91	13.138	3744	3747	3751	rBV4	681	674	0.02%	0.003%
92	13.164	3753	3755	3759	rVB4	778	473	0.01%	0.002%
93	13.276	3784	3790	3794	rBV8	1595	1974	0.06%	0.008%
94	13.350	3809	3813	3816	rBV3	1154	935	0.03%	0.004%
95	13.482	3852	3854	3861	rVB5	807	789	0.02%	0.003%
96	13.675	3909	3914	3917	rBV4	1535	1458	0.05%	0.006%
97	13.981	4004	4009	4011	rBV3	1436	1449	0.05%	0.006%
98	14.055	4029	4032	4035	rBV3	1383	862	0.03%	0.003%
99	14.643	4213	4215	4219	rBV4	1031	547	0.02%	0.002%
100	15.051	4337	4342	4345	rBV5	1626	1913	0.06%	0.008%




Sum of corrected areas: 24976185

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020235.D
Acq On : 02 Feb 2021 14:06
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

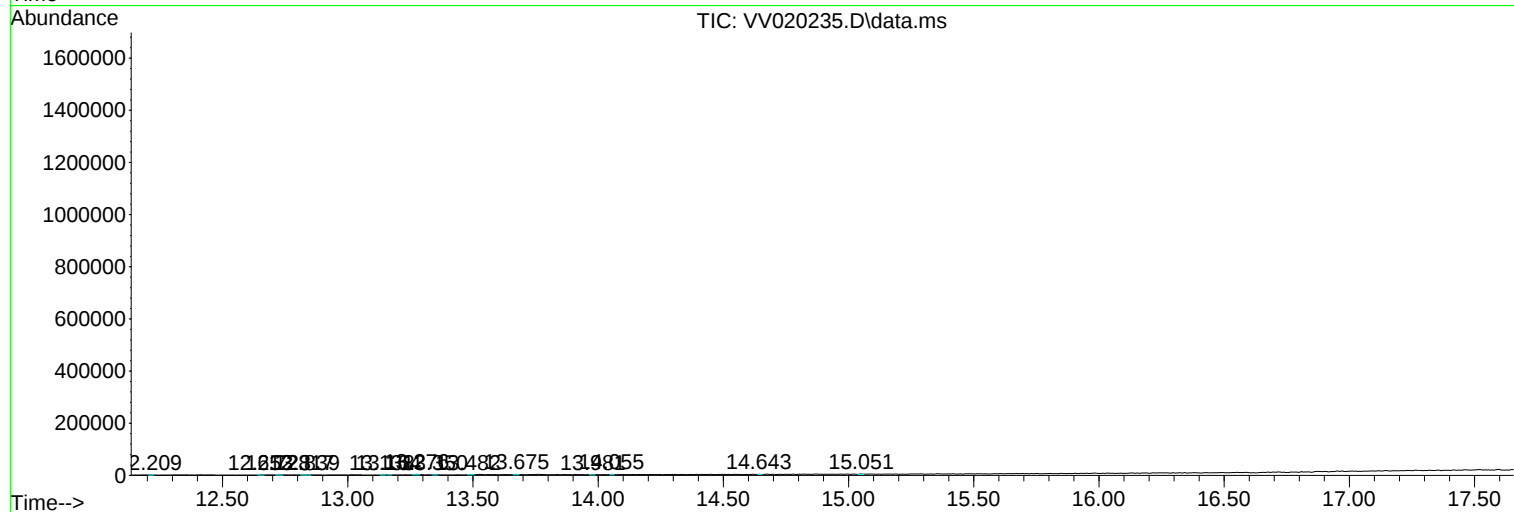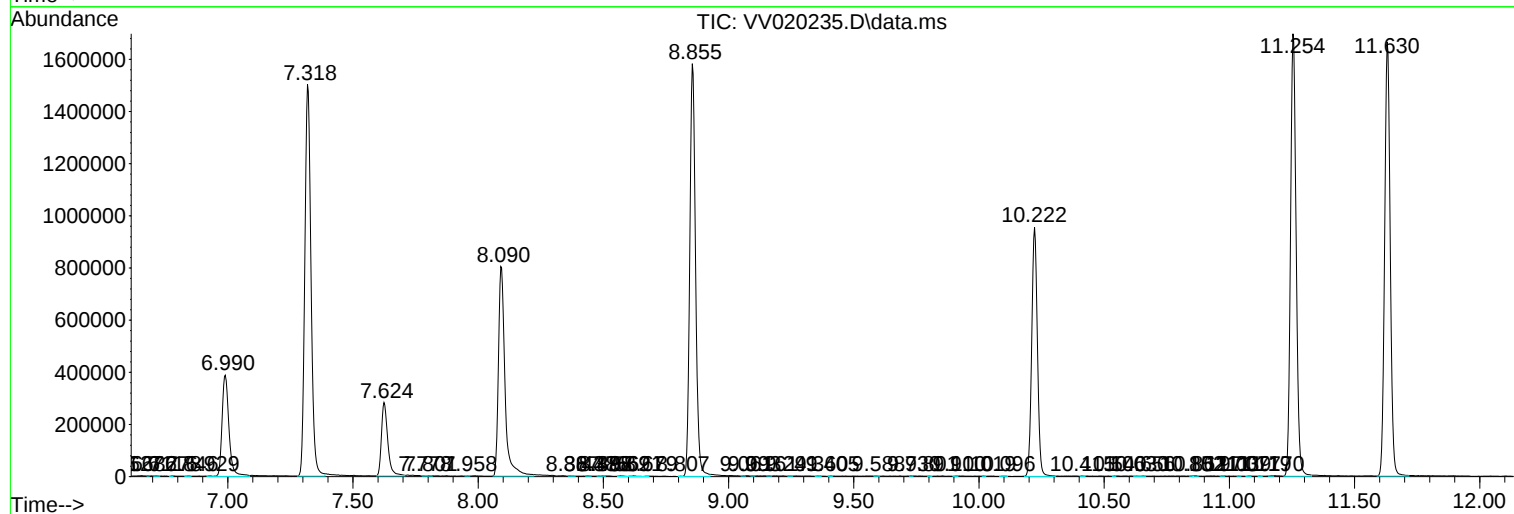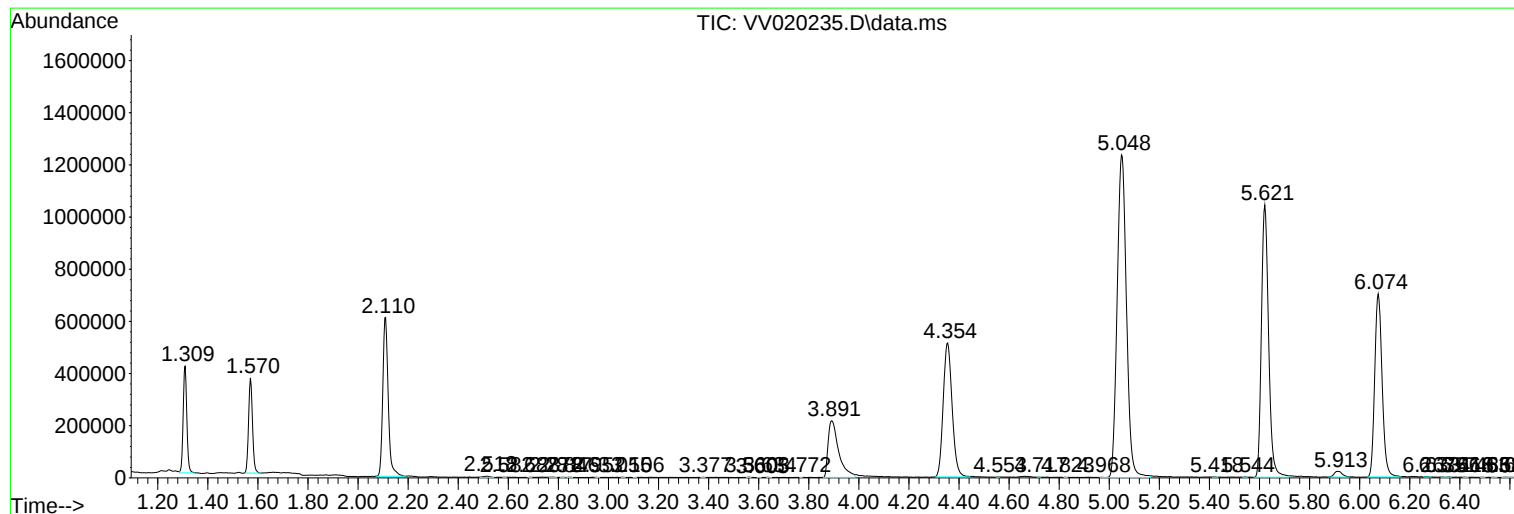

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020235.D
Acq On : 02 Feb 2021 14:06
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020235.D
Acq On : 02 Feb 2021 14:06
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
