

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020236.D
 Acq On : 02 Feb 2021 14:34
 Operator : SY/MD
 Sample : M1258-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Z0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

Signal : TIC: VV020236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	80	rVB	390025	395235	13.85%	1.936%
2	1.569	142	149	160	rVB	323582	358481	12.57%	1.756%
3	2.110	306	317	335	rBV	594804	882940	30.95%	4.324%
4	2.357	392	394	397	rBV4	1007	638	0.02%	0.003%
5	2.573	458	461	465	rBV4	1129	918	0.03%	0.004%
6	2.714	503	505	510	rVB5	815	577	0.02%	0.003%
7	2.750	514	516	518	rBV3	984	570	0.02%	0.003%
8	3.013	594	598	601	rBV3	979	794	0.03%	0.004%
9	3.203	653	657	658	rBV3	854	586	0.02%	0.003%
10	3.335	697	698	701	rVB2	621	293	0.01%	0.001%
11	3.418	722	724	728	rBV3	540	400	0.01%	0.002%
12	3.470	737	740	743	rVV5	749	445	0.02%	0.002%
13	3.505	748	751	753	rBV3	711	494	0.02%	0.002%
14	3.598	777	780	783	rBV3	1421	899	0.03%	0.004%
15	3.647	793	795	800	rVB4	1191	702	0.02%	0.003%
16	3.695	808	810	812	rVB3	802	352	0.01%	0.002%
17	3.785	832	838	839	rBV5	1118	1160	0.04%	0.006%
18	3.827	849	851	854	rBV4	616	303	0.01%	0.001%
19	3.888	859	870	903	rBV	186584	570252	19.99%	2.793%
20	4.351	998	1014	1045	rBV	466640	1142240	40.04%	5.594%
21	4.582	1084	1086	1088	rBV2	918	452	0.02%	0.002%
22	4.978	1203	1209	1212	rBV6	1117	1199	0.04%	0.006%
23	5.048	1212	1231	1262	rBV2	1110878	2852919	100.00%	13.971%
24	5.338	1319	1321	1322	rBV2	719	302	0.01%	0.001%
25	5.434	1349	1351	1357	rVB7	1339	862	0.03%	0.004%
26	5.553	1386	1388	1395	rVB5	1174	889	0.03%	0.004%
27	5.618	1395	1408	1446	rBV	897412	1816271	63.66%	8.894%
28	5.910	1487	1499	1519	rVB2	21559	47346	1.66%	0.232%
29	6.019	1528	1533	1535	rBV5	1090	897	0.03%	0.004%
30	6.074	1535	1550	1575	rBV	584511	1177578	41.28%	5.767%
31	6.505	1678	1684	1689	rBV3	322	410	0.01%	0.002%
32	6.569	1702	1704	1709	rVV2	372	306	0.01%	0.001%
33	6.653	1726	1730	1735	rVV4	622	705	0.02%	0.003%
34	6.701	1738	1745	1748	rVV4	541	491	0.02%	0.002%
35	6.990	1819	1835	1867	rBV	241921	448243	15.71%	2.195%
36	7.199	1898	1900	1905	rVB5	818	512	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020236.D
 Acq On : 02 Feb 2021 14:34
 Operator : SY/MD
 Sample : M1258-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Z0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis

37	7.318	1925	1937	1966	rBV	1015699	1757862	61.62%	8.608%
38	7.624	2022	2032	2063	rBV	173935	307568	10.78%	1.506%
39	7.781	2079	2081	2085	rBV3	546	356	0.01%	0.002%
40	7.814	2089	2091	2094	rBV2	630	337	0.01%	0.002%
41	7.942	2119	2131	2149	rVB	29164	53907	1.89%	0.264%
42	8.093	2166	2178	2212	rBV	460146	885780	31.05%	4.338%
43	8.363	2259	2262	2266	rVB2	684	420	0.01%	0.002%
44	8.405	2271	2275	2281	rVV7	681	657	0.02%	0.003%
45	8.434	2282	2284	2288	rVB3	604	296	0.01%	0.001%
46	8.576	2323	2328	2330	rBV2	460	360	0.01%	0.002%
47	8.624	2342	2343	2347	rVB2	684	349	0.01%	0.002%
48	8.669	2355	2357	2361	rVB	533	333	0.01%	0.002%
49	8.720	2369	2373	2376	rBV3	592	455	0.02%	0.002%
50	8.781	2390	2392	2396	rBV2	608	446	0.02%	0.002%
51	8.855	2402	2415	2447	rBV	1113217	1817068	63.69%	8.898%
52	9.026	2465	2468	2472	rVB3	1278	1034	0.04%	0.005%
53	9.261	2539	2541	2548	rVB4	521	386	0.01%	0.002%
54	9.412	2586	2588	2591	rVB3	675	309	0.01%	0.002%
55	9.428	2591	2593	2599	rBV4	477	325	0.01%	0.002%
56	9.498	2611	2615	2618	rVB4	528	320	0.01%	0.002%
57	9.518	2618	2621	2625	rVB2	529	339	0.01%	0.002%
58	9.588	2639	2643	2645	rVB	553	318	0.01%	0.002%
59	9.637	2653	2658	2662	rVB2	532	563	0.02%	0.003%
60	9.733	2683	2688	2691	rBV2	551	494	0.02%	0.002%
61	9.778	2694	2702	2705	rVV2	419	528	0.02%	0.003%
62	9.884	2733	2735	2743	rBV2	458	380	0.01%	0.002%
63	10.174	2822	2825	2828	rBV3	615	606	0.02%	0.003%
64	10.222	2828	2840	2859	rVV	751903	1171858	41.08%	5.739%
65	10.389	2880	2892	2909	rVB	52086	86497	3.03%	0.424%
66	10.682	2979	2983	2987	rBV2	820	874	0.03%	0.004%
67	10.733	2996	2999	3002	rBV2	538	415	0.01%	0.002%
68	10.791	3014	3017	3020	rVV5	1054	692	0.02%	0.003%
69	10.810	3020	3023	3025	rVV2	867	569	0.02%	0.003%
70	10.859	3034	3038	3042	rBV4	1794	2223	0.08%	0.011%
71	10.894	3046	3049	3052	rVV3	828	604	0.02%	0.003%
72	10.961	3068	3070	3076	rBV6	751	610	0.02%	0.003%
73	11.032	3087	3092	3093	rBV5	1054	925	0.03%	0.005%
74	11.084	3105	3108	3110	rBV3	1085	629	0.02%	0.003%
75	11.170	3129	3135	3137	rBV5	2202	2276	0.08%	0.011%
76	11.254	3149	3161	3185	rBV	1474456	2279878	79.91%	11.165%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020236.D
 Acq On : 02 Feb 2021 14:34
 Operator : SY/MD
 Sample : M1258-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Z0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

77	11.457	3221	3224	3227	rBV4	1582	1068	0.04%	0.005%
78	11.505	3237	3239	3243	rBV4	1042	637	0.02%	0.003%
79	11.630	3266	3278	3298	rBV	1476997	2301178	80.66%	11.269%
80	11.830	3338	3340	3341	rBV2	1057	397	0.01%	0.002%
81	11.878	3350	3355	3364	rVB8	1456	2094	0.07%	0.010%
82	11.958	3378	3380	3381	rBV	751	307	0.01%	0.002%
83	12.016	3396	3398	3399	rBV2	761	367	0.01%	0.002%
84	12.190	3450	3452	3456	rBV4	737	585	0.02%	0.003%
85	12.260	3464	3474	3483	rBV3	8088	13540	0.47%	0.066%
86	12.328	3493	3495	3498	rBV3	958	595	0.02%	0.003%
87	12.360	3499	3505	3510	rVV7	2905	3454	0.12%	0.017%
88	12.511	3550	3552	3554	rBV3	949	455	0.02%	0.002%
89	12.707	3610	3613	3615	rBV3	830	552	0.02%	0.003%
90	13.019	3708	3710	3712	rBV3	789	365	0.01%	0.002%
91	13.074	3725	3727	3729	rBV3	671	294	0.01%	0.001%
92	13.341	3806	3810	3812	rBV2	1122	911	0.03%	0.004%
93	13.469	3848	3850	3852	rBV3	805	326	0.01%	0.002%
94	13.627	3897	3899	3901	rBV3	962	396	0.01%	0.002%
95	13.672	3911	3913	3917	rBV4	901	471	0.02%	0.002%
96	13.714	3924	3926	3928	rBV2	866	493	0.02%	0.002%
97	13.727	3928	3930	3935	rVV3	1522	1147	0.04%	0.006%
98	13.759	3935	3940	3944	rVV6	1801	1819	0.06%	0.009%
99	14.318	4112	4114	4115	rBV	1076	583	0.02%	0.003%
100	14.563	4188	4190	4193	rBV3	1053	720	0.03%	0.004%




Sum of corrected areas: 20420261

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020236.D
Acq On : 02 Feb 2021 14:34
Operator : SY/MD
Sample : M1258-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

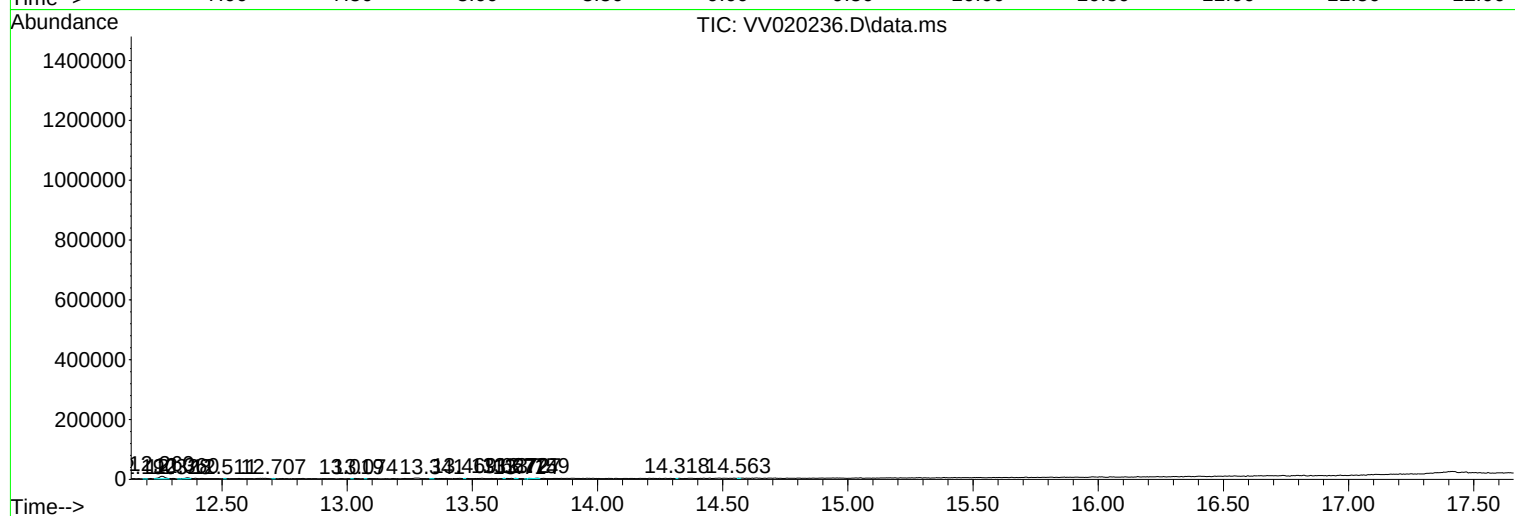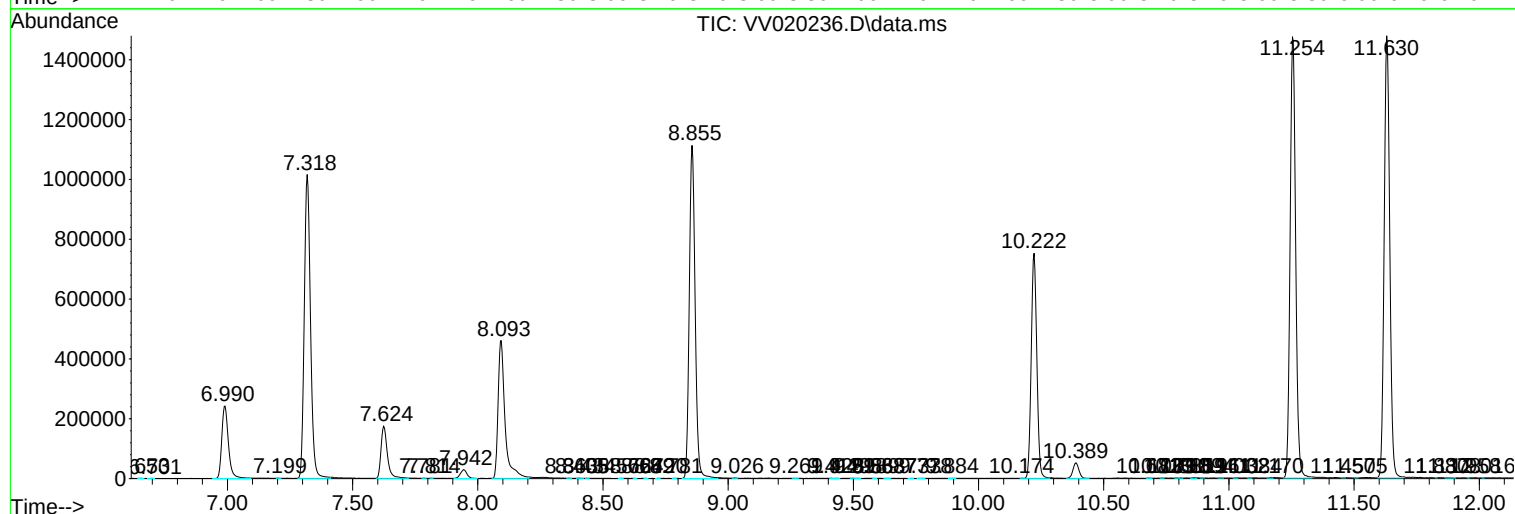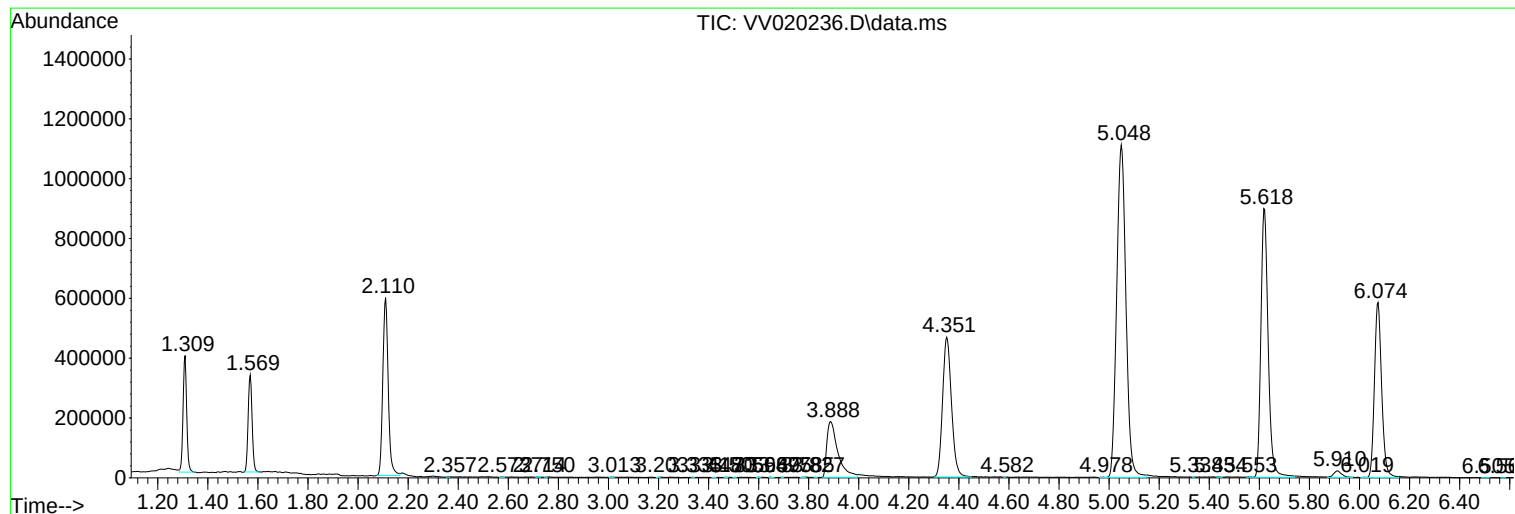

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020236.D
Acq On : 02 Feb 2021 14:34
Operator : SY/MD
Sample : M1258-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020236.D
Acq On : 02 Feb 2021 14:34
Operator : SY/MD
Sample : M1258-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
