

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020237.D
 Acq On : 02 Feb 2021 14:57
 Operator : SY/MD
 Sample : M1258-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Z4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

Signal : TIC: VV020237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	85	rVB	374494	390306	13.70%	1.774%
2	1.570	142	149	161	rVB	322806	354559	12.45%	1.612%
3	2.107	305	316	334	rBV	536254	822030	28.86%	3.736%
4	2.377	397	400	402	rBV3	1234	924	0.03%	0.004%
5	2.508	434	441	445	rBV4	2360	3276	0.12%	0.015%
6	2.563	456	458	463	rVB5	1176	846	0.03%	0.004%
7	2.714	502	505	508	rBV5	1112	672	0.02%	0.003%
8	2.807	532	534	538	rVB5	1218	748	0.03%	0.003%
9	2.907	562	565	567	rBV3	1029	637	0.02%	0.003%
10	2.943	573	576	579	rBV3	753	576	0.02%	0.003%
11	2.962	580	582	585	rVB2	1225	589	0.02%	0.003%
12	3.013	594	598	599	rBV3	1135	645	0.02%	0.003%
13	3.042	600	607	618	rVV7	6350	12852	0.45%	0.058%
14	3.277	677	680	683	rBV4	786	475	0.02%	0.002%
15	3.322	691	694	695	rBV2	885	425	0.01%	0.002%
16	3.457	733	736	741	rBV4	665	654	0.02%	0.003%
17	3.492	745	747	751	rVB4	746	428	0.02%	0.002%
18	3.653	792	797	800	rVB4	1120	1011	0.04%	0.005%
19	3.669	800	802	807	rBV3	923	778	0.03%	0.004%
20	3.698	808	811	813	rVB4	936	498	0.02%	0.002%
21	3.766	820	832	851	rBV4	4882	13197	0.46%	0.060%
22	3.894	858	872	908	rBV	185683	581445	20.41%	2.643%
23	4.261	984	986	988	rBV2	699	427	0.01%	0.002%
24	4.351	997	1014	1038	rBV	458487	1133464	39.79%	5.152%
25	4.528	1067	1069	1072	rVB3	1112	563	0.02%	0.003%
26	4.544	1072	1074	1079	rVB5	1390	1036	0.04%	0.005%
27	4.566	1079	1081	1084	rBV3	1250	937	0.03%	0.004%
28	4.878	1177	1178	1183	rVB3	1190	727	0.03%	0.003%
29	4.901	1183	1185	1188	rBV3	966	496	0.02%	0.002%
30	4.965	1203	1205	1208	rVB	1079	613	0.02%	0.003%
31	5.049	1211	1231	1264	rBV2	1103353	2848447	100.00%	12.947%
32	5.396	1335	1339	1341	rBV4	1206	926	0.03%	0.004%
33	5.460	1356	1359	1360	rBV2	1180	612	0.02%	0.003%
34	5.492	1366	1369	1374	rBV6	1193	1135	0.04%	0.005%
35	5.566	1390	1392	1395	rBV3	1238	872	0.03%	0.004%
36	5.621	1395	1409	1442	rBV	891006	1782798	62.59%	8.103%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020237.D
 Acq On : 02 Feb 2021 14:57
 Operator : SY/MD
 Sample : M1258-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Z4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis

37	5.913	1488	1500	1514	rBV3	27742	59286	2.08%	0.269%
38	6.007	1526	1529	1532	rBV3	774	556	0.02%	0.003%
39	6.074	1532	1550	1576	rBV	632795	1291454	45.34%	5.870%
40	6.412	1653	1655	1658	rVB3	1064	571	0.02%	0.003%
41	6.499	1680	1682	1686	rVB4	961	624	0.02%	0.003%
42	6.528	1687	1691	1694	rBV5	903	907	0.03%	0.004%
43	6.643	1720	1727	1730	rBV5	1475	1929	0.07%	0.009%
44	6.711	1743	1748	1751	rBV6	1085	920	0.03%	0.004%
45	6.772	1764	1767	1769	rBV3	627	468	0.02%	0.002%
46	6.788	1769	1772	1773	rBV2	949	570	0.02%	0.003%
47	6.987	1823	1834	1857	rBV	341698	626283	21.99%	2.847%
48	7.319	1924	1937	1960	rBV	1331834	2302235	80.82%	10.464%
49	7.624	2021	2032	2056	rBV	203079	365272	12.82%	1.660%
50	7.897	2113	2117	2119	rVB5	805	492	0.02%	0.002%
51	7.946	2123	2132	2145	rVV2	8181	16412	0.58%	0.075%
52	8.093	2167	2178	2218	rBV	685676	1247757	43.80%	5.672%
53	8.421	2278	2280	2284	rVB4	1572	871	0.03%	0.004%
54	8.499	2300	2304	2307	rBV5	1799	1469	0.05%	0.007%
55	8.589	2329	2332	2334	rBV3	925	523	0.02%	0.002%
56	8.759	2381	2385	2388	rBV4	1462	1228	0.04%	0.006%
57	8.788	2392	2394	2396	rBV3	917	464	0.02%	0.002%
58	8.855	2403	2415	2441	rBV	1381420	2224873	78.11%	10.113%
59	9.068	2479	2481	2487	rVB4	1704	1300	0.05%	0.006%
60	9.100	2489	2491	2493	rVB3	1097	476	0.02%	0.002%
61	9.119	2493	2497	2499	rBV3	1144	867	0.03%	0.004%
62	9.257	2538	2540	2543	rBV3	1383	796	0.03%	0.004%
63	9.306	2553	2555	2557	rBV2	758	455	0.02%	0.002%
64	9.482	2607	2610	2618	rVB4	896	854	0.03%	0.004%
65	9.556	2628	2633	2637	rVB4	1001	1041	0.04%	0.005%
66	9.589	2638	2643	2645	rVV4	858	753	0.03%	0.003%
67	9.601	2645	2647	2651	rVB3	1353	735	0.03%	0.003%
68	9.630	2651	2656	2661	rBV2	1149	984	0.03%	0.004%
69	9.672	2666	2669	2674	rVB4	1152	946	0.03%	0.004%
70	9.807	2708	2711	2715	rVB3	662	466	0.02%	0.002%
71	9.907	2738	2742	2746	rBV4	638	511	0.02%	0.002%
72	10.119	2804	2808	2811	rVV3	584	434	0.02%	0.002%
73	10.154	2814	2819	2823	rBV2	809	745	0.03%	0.003%
74	10.222	2826	2840	2862	rVV	836480	1307014	45.89%	5.941%
75	10.389	2880	2892	2906	rVB3	17248	29637	1.04%	0.135%
76	10.489	2920	2923	2925	rBV	864	454	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020237.D
 Acq On : 02 Feb 2021 14:57
 Operator : SY/MD
 Sample : M1258-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Z4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis

77	10.544	2937	2940	2945	rVV5	938	625	0.02%	0.003%
78	10.727	2995	2997	3003	rBV5	827	834	0.03%	0.004%
79	10.888	3045	3047	3051	rBV3	984	647	0.02%	0.003%
80	10.936	3058	3062	3065	rBV4	759	561	0.02%	0.003%
81	10.952	3065	3067	3070	rBV2	818	505	0.02%	0.002%
82	11.158	3129	3131	3136	rBV5	938	870	0.03%	0.004%
83	11.254	3149	3161	3185	rBV	1492163	2242250	78.72%	10.192%
84	11.415	3209	3211	3214	rVB4	1555	608	0.02%	0.003%
85	11.524	3242	3245	3246	rBV2	1236	670	0.02%	0.003%
86	11.630	3265	3278	3300	rBV	1502449	2290790	80.42%	10.412%
87	11.888	3355	3358	3360	rBV2	1013	576	0.02%	0.003%
88	12.055	3408	3410	3413	rBV3	823	430	0.02%	0.002%
89	12.527	3553	3557	3560	rBV3	1012	973	0.03%	0.004%
90	12.653	3592	3596	3597	rBV2	1163	773	0.03%	0.004%
91	12.788	3635	3638	3642	rBV2	546	456	0.02%	0.002%
92	13.000	3701	3704	3709	rVB2	578	521	0.02%	0.002%
93	13.077	3726	3728	3732	rBV4	645	485	0.02%	0.002%
94	13.174	3756	3758	3762	rBV4	767	520	0.02%	0.002%
95	13.354	3810	3814	3820	rBV2	501	455	0.02%	0.002%
96	13.386	3820	3824	3830	rBV3	444	469	0.02%	0.002%
97	14.286	4101	4104	4107	rBV2	573	433	0.02%	0.002%
98	14.334	4117	4119	4125	rBV3	626	520	0.02%	0.002%
99	14.450	4153	4155	4158	rBV3	710	475	0.02%	0.002%
100	14.508	4170	4173	4175	rBV4	1169	753	0.03%	0.003%




Sum of corrected areas: 22000455

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020237.D
Acq On : 02 Feb 2021 14:57
Operator : SY/MD
Sample : M1258-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

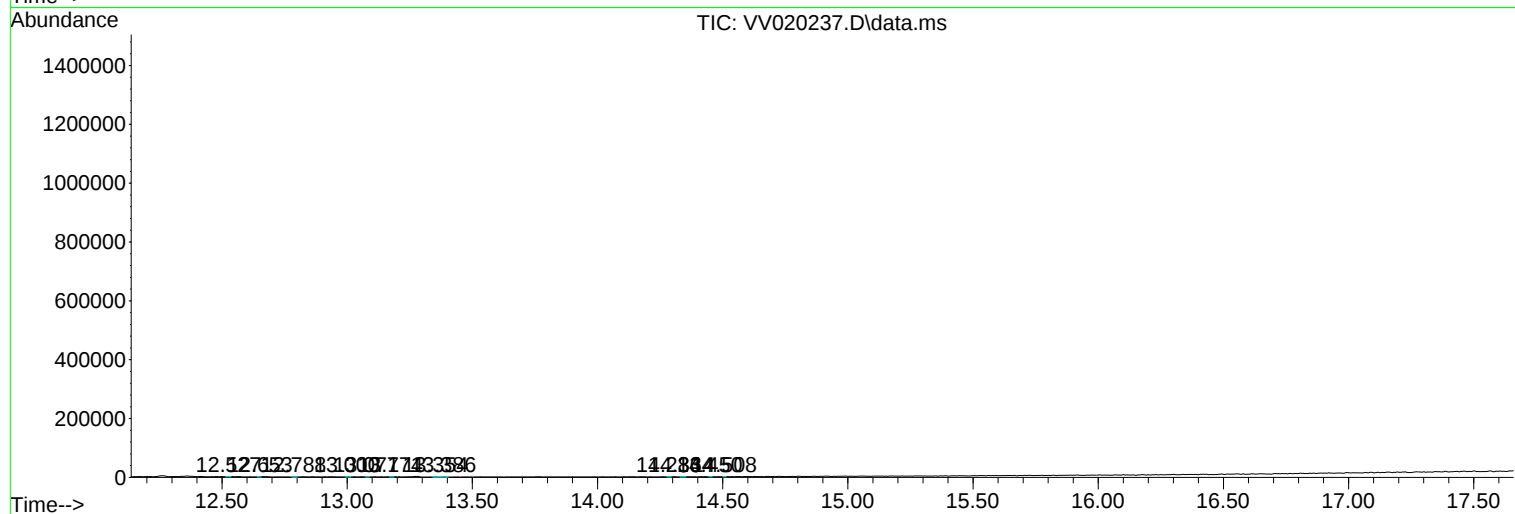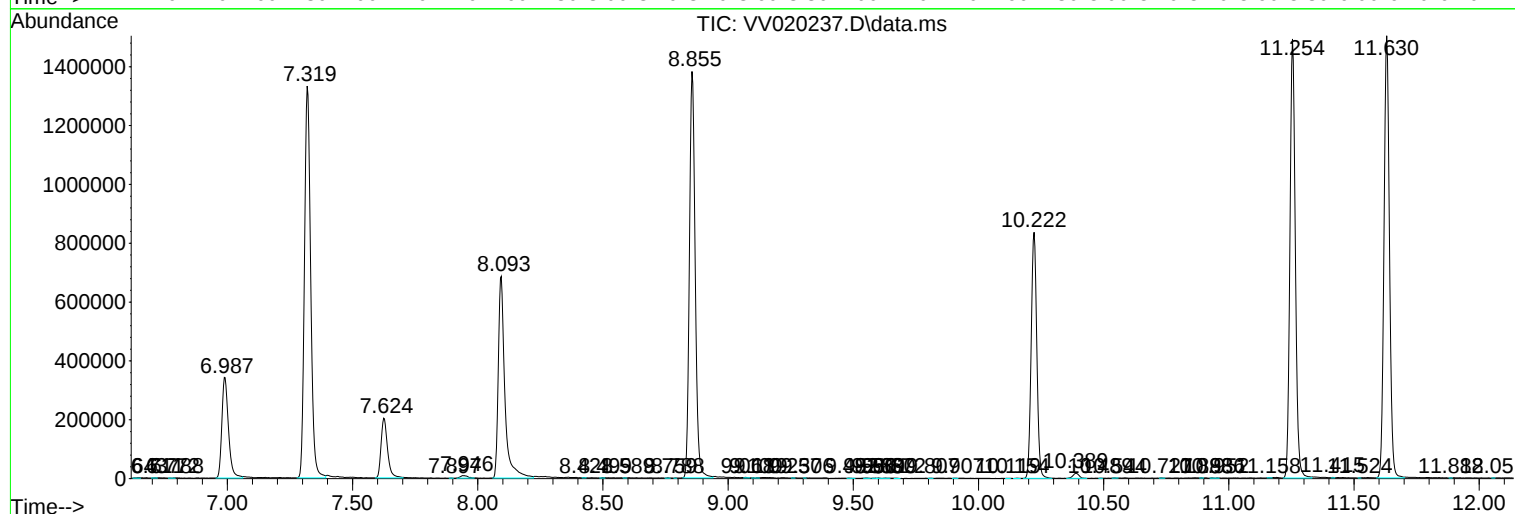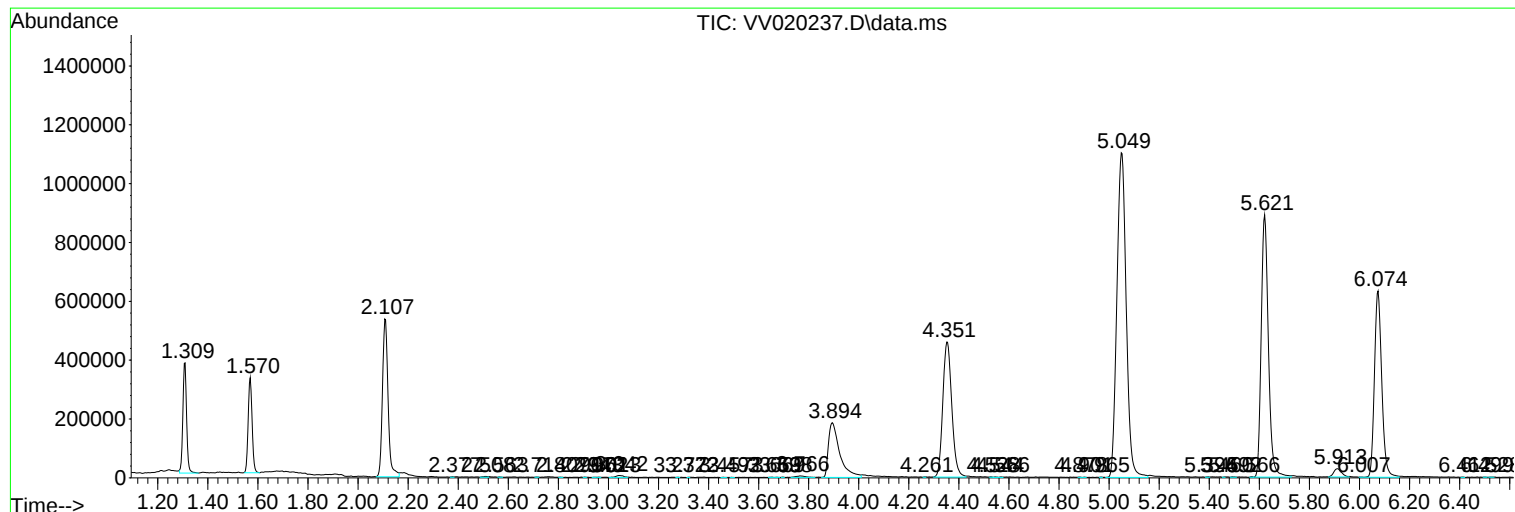

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020237.D
Acq On : 02 Feb 2021 14:57
Operator : SY/MD
Sample : M1258-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020237.D
Acq On : 02 Feb 2021 14:57
Operator : SY/MD
Sample : M1258-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
