

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020239.D
 Acq On : 02 Feb 2021 15:44
 Operator : SY/MD
 Sample : M1258-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Z5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

Signal : TIC: VV020239.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	86	rVB	430967	430283	13.64%	1.794%
2	1.570	142	149	162	rBV	369435	404429	12.82%	1.687%
3	2.110	306	317	335	rBV	657484	991933	31.44%	4.137%
4	2.296	370	375	376	rBV5	1535	1359	0.04%	0.006%
5	2.534	436	449	458	rBV5	5427	10627	0.34%	0.044%
6	2.643	480	483	484	rBV3	625	318	0.01%	0.001%
7	2.766	511	521	534	rVV5	8784	17723	0.56%	0.074%
8	2.814	534	536	541	rVB4	931	637	0.02%	0.003%
9	2.959	576	581	584	rBV3	1160	1199	0.04%	0.005%
10	3.045	595	608	623	rBV2	49147	102130	3.24%	0.426%
11	3.219	658	662	663	rBV2	904	758	0.02%	0.003%
12	3.258	671	674	679	rVB5	1583	1080	0.03%	0.005%
13	3.280	679	681	684	rBV3	646	414	0.01%	0.002%
14	3.309	687	690	695	rBV5	938	732	0.02%	0.003%
15	3.373	707	710	711	rBV2	647	313	0.01%	0.001%
16	3.701	808	812	816	rBV5	898	885	0.03%	0.004%
17	3.769	816	833	852	rBV4	38059	101891	3.23%	0.425%
18	3.888	859	870	906	rBV	219680	634269	20.10%	2.645%
19	4.354	998	1015	1042	rBV2	508906	1265290	40.10%	5.276%
20	4.634	1100	1102	1104	rBV2	787	453	0.01%	0.002%
21	4.836	1162	1165	1167	rBV3	848	563	0.02%	0.002%
22	4.868	1173	1175	1177	rVB3	1061	488	0.02%	0.002%
23	4.881	1177	1179	1181	rBV2	908	559	0.02%	0.002%
24	5.052	1214	1232	1258	rBV2	1235033	3154947	100.00%	13.157%
25	5.386	1334	1336	1339	rVB3	1132	504	0.02%	0.002%
26	5.524	1376	1379	1381	rBV6	803	523	0.02%	0.002%
27	5.621	1396	1409	1442	rBV	1016727	2046011	64.85%	8.532%
28	5.910	1488	1499	1514	rBV2	31878	65413	2.07%	0.273%
29	6.074	1536	1550	1576	rBV	706786	1425768	45.19%	5.946%
30	6.267	1608	1610	1614	rBV3	767	407	0.01%	0.002%
31	6.338	1628	1632	1635	rBV5	816	811	0.03%	0.003%
32	6.524	1684	1690	1692	rBV3	319	358	0.01%	0.001%
33	6.804	1773	1777	1780	rBV2	439	346	0.01%	0.001%
34	6.843	1784	1789	1791	rBV2	417	321	0.01%	0.001%
35	6.946	1813	1821	1822	rBV2	520	499	0.02%	0.002%
36	6.991	1822	1835	1863	rBV	294786	531363	16.84%	2.216%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020239.D
 Acq On : 02 Feb 2021 15:44
 Operator : SY/MD
 Sample : M1258-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Z5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis

37	7.119	1873	1875	1878	rBV3	545	323	0.01%	0.001%
38	7.245	1911	1914	1915	rBV2	486	286	0.01%	0.001%
39	7.318	1925	1937	1962	rBV	1232721	2126668	67.41%	8.869%
40	7.486	1986	1989	1992	rBV4	1098	924	0.03%	0.004%
41	7.544	2003	2007	2010	rVB5	877	753	0.02%	0.003%
42	7.560	2010	2012	2018	rVB3	1296	1025	0.03%	0.004%
43	7.624	2020	2032	2058	rBV	252874	454055	14.39%	1.893%
44	7.817	2089	2092	2093	rBV2	1284	789	0.03%	0.003%
45	7.945	2126	2132	2139	rVV2	4151	6673	0.21%	0.028%
46	7.984	2142	2144	2152	rVB7	2040	2561	0.08%	0.011%
47	8.090	2167	2177	2213	rBV	789853	1440778	45.67%	6.008%
48	8.794	2394	2396	2399	rBV3	1376	900	0.03%	0.004%
49	8.855	2403	2415	2447	rBV	1559422	2550900	80.85%	10.638%
50	9.071	2480	2482	2488	rVB6	1451	1121	0.04%	0.005%
51	9.125	2497	2499	2501	rBV3	677	272	0.01%	0.001%
52	9.148	2502	2506	2515	rVB9	1751	2146	0.07%	0.009%
53	9.206	2521	2524	2529	rVB4	1479	1281	0.04%	0.005%
54	9.232	2529	2532	2533	rBV3	522	380	0.01%	0.002%
55	9.241	2533	2535	2539	rBV3	932	768	0.02%	0.003%
56	9.373	2569	2576	2577	rBV6	835	1041	0.03%	0.004%
57	9.550	2628	2631	2632	rBV2	1013	528	0.02%	0.002%
58	9.588	2640	2643	2647	rVB3	1098	836	0.03%	0.003%
59	9.611	2647	2650	2651	rBV2	883	465	0.01%	0.002%
60	9.659	2661	2665	2667	rBV2	1111	895	0.03%	0.004%
61	9.688	2670	2674	2677	rVV5	928	772	0.02%	0.003%
62	9.765	2696	2698	2700	rBV2	1006	488	0.02%	0.002%
63	9.797	2705	2708	2712	rVB5	988	703	0.02%	0.003%
64	9.826	2712	2717	2721	rBV5	1336	1747	0.06%	0.007%
65	9.878	2731	2733	2735	rVB3	848	291	0.01%	0.001%
66	9.933	2744	2750	2754	rBV5	964	1144	0.04%	0.005%
67	10.006	2770	2773	2775	rBV5	931	490	0.02%	0.002%
68	10.068	2790	2792	2794	rBV	603	318	0.01%	0.001%
69	10.084	2795	2797	2799	rVV4	555	289	0.01%	0.001%
70	10.135	2806	2813	2814	rBV3	1030	930	0.03%	0.004%
71	10.222	2827	2840	2863	rVB	955040	1503186	47.65%	6.269%
72	10.389	2882	2892	2901	rVB2	9466	15999	0.51%	0.067%
73	10.550	2938	2942	2946	rVB2	487	404	0.01%	0.002%
74	10.727	2995	2997	3002	rVB3	500	302	0.01%	0.001%
75	10.891	3046	3048	3053	rVB	447	376	0.01%	0.002%
76	10.932	3056	3061	3068	rVB4	690	695	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020239.D
 Acq On : 02 Feb 2021 15:44
 Operator : SY/MD
 Sample : M1258-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Z5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

77	11.090	3107	3110	3111	rBV	521	312	0.01%	0.001%
78	11.100	3111	3113	3118	rVB	545	369	0.01%	0.002%
79	11.161	3131	3132	3135	rBV3	568	396	0.01%	0.002%
80	11.254	3149	3161	3190	rBV	1394958	2137299	67.74%	8.913%
81	11.434	3215	3217	3220	rBV	779	443	0.01%	0.002%
82	11.469	3226	3228	3231	rVB2	735	385	0.01%	0.002%
83	11.511	3237	3241	3245	rBV4	633	662	0.02%	0.003%
84	11.540	3245	3250	3252	rBV5	623	699	0.02%	0.003%
85	11.559	3253	3256	3257	rBV3	733	375	0.01%	0.002%
86	11.630	3265	3278	3298	rBV	1630317	2506369	79.44%	10.452%
87	11.904	3359	3363	3365	rBV3	1089	880	0.03%	0.004%
88	11.965	3380	3382	3386	rVB5	1269	781	0.02%	0.003%
89	11.990	3387	3390	3391	rBV2	1041	539	0.02%	0.002%
90	12.145	3435	3438	3440	rBV4	1045	772	0.02%	0.003%
91	12.360	3501	3505	3513	rVB9	3380	3843	0.12%	0.016%
92	12.518	3552	3554	3557	rVB4	753	400	0.01%	0.002%
93	12.537	3557	3560	3566	rBV4	763	765	0.02%	0.003%
94	12.563	3566	3568	3572	rVB3	745	351	0.01%	0.001%
95	12.948	3685	3688	3689	rBV	1027	575	0.02%	0.002%
96	12.981	3696	3698	3701	rBV3	901	563	0.02%	0.002%
97	13.122	3740	3742	3747	rBV2	973	828	0.03%	0.003%
98	13.926	3990	3992	3994	rBV3	967	494	0.02%	0.002%
99	14.235	4085	4088	4096	rBV6	1085	1341	0.04%	0.006%
100	14.325	4114	4116	4119	rBV	807	409	0.01%	0.002%




Sum of corrected areas: 23979956

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020239.D
Acq On : 02 Feb 2021 15:44
Operator : SY/MD
Sample : M1258-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

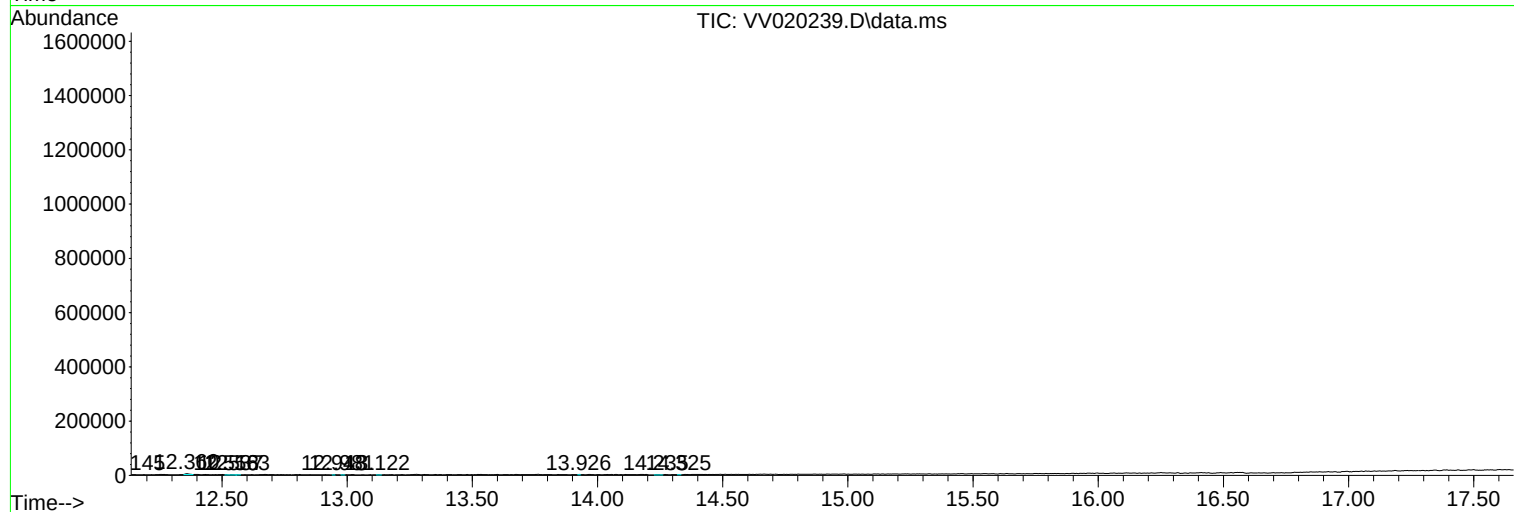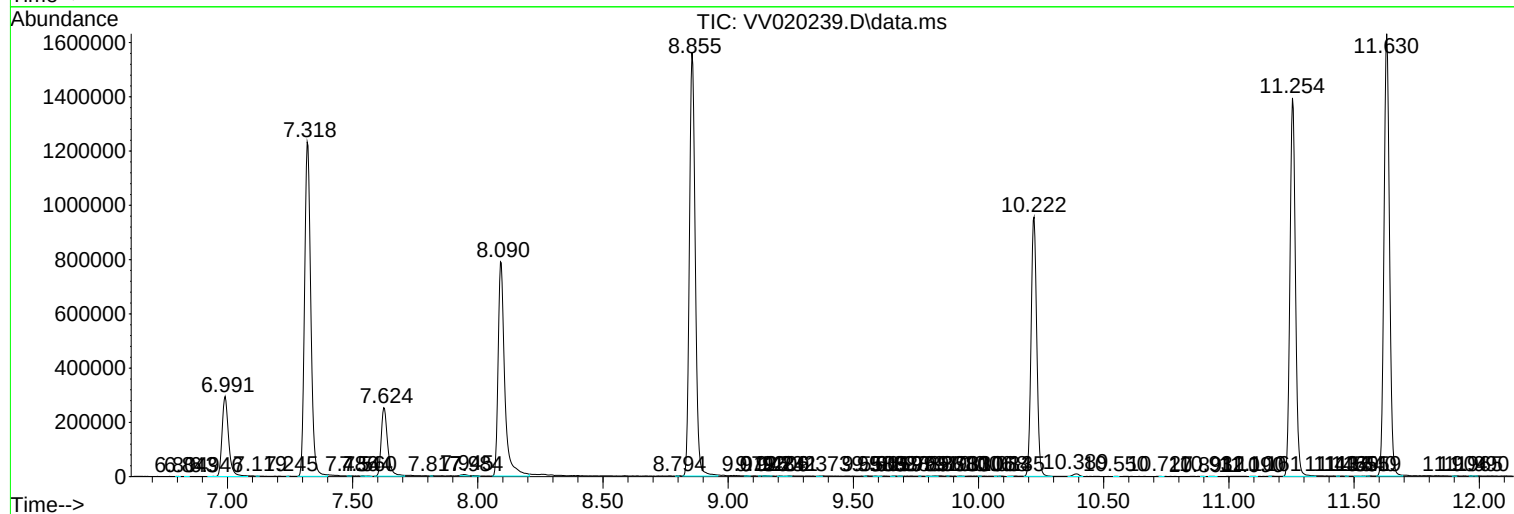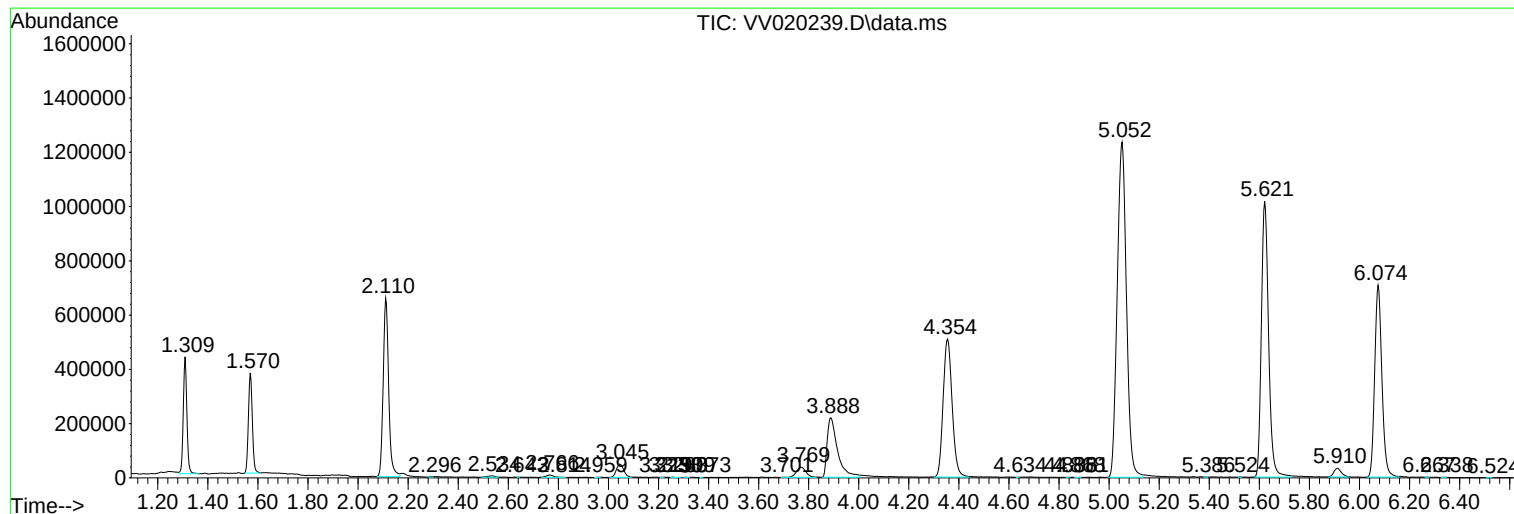

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020239.D
Acq On : 02 Feb 2021 15:44
Operator : SY/MD
Sample : M1258-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020239.D
Acq On : 02 Feb 2021 15:44
Operator : SY/MD
Sample : M1258-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
