

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020240.D
 Acq On : 02 Feb 2021 16:08
 Operator : SY/MD
 Sample : M1258-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG503

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

Signal : TIC: VV020240.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	86	rVB	420105	431790	13.66%	1.779%
2	1.570	142	149	163	rVB	363197	399763	12.65%	1.647%
3	2.110	307	317	335	rBV	628711	949501	30.05%	3.911%
4	2.502	435	439	440	rBV4	1368	944	0.03%	0.004%
5	2.595	464	468	472	rBV6	780	676	0.02%	0.003%
6	2.750	513	516	517	rBV3	954	477	0.02%	0.002%
7	2.856	546	549	554	rBV5	898	643	0.02%	0.003%
8	2.878	554	556	559	rBV4	724	549	0.02%	0.002%
9	3.042	602	607	609	rBV5	1905	1701	0.05%	0.007%
10	3.084	617	620	625	rBV5	786	621	0.02%	0.003%
11	3.148	638	640	644	rVB3	1019	525	0.02%	0.002%
12	3.177	647	649	650	rBV	922	393	0.01%	0.002%
13	3.248	668	671	673	rVB2	898	475	0.02%	0.002%
14	3.338	696	699	701	rBV3	703	468	0.01%	0.002%
15	3.415	718	723	725	rBV7	678	598	0.02%	0.002%
16	3.450	731	734	736	rBV4	903	489	0.02%	0.002%
17	3.537	759	761	765	rVB3	1066	728	0.02%	0.003%
18	3.560	765	768	771	rBV4	640	506	0.02%	0.002%
19	3.614	782	785	788	rBV3	1026	733	0.02%	0.003%
20	3.688	805	808	811	rBV3	679	460	0.01%	0.002%
21	3.714	811	816	819	rBV5	1132	1235	0.04%	0.005%
22	3.759	827	830	831	rBV2	807	439	0.01%	0.002%
23	3.891	860	871	905	rBV	211789	624009	19.75%	2.571%
24	4.354	999	1015	1043	rVV	508484	1249579	39.54%	5.148%
25	4.775	1143	1146	1150	rBV5	1268	781	0.02%	0.003%
26	4.917	1187	1190	1193	rVV5	1139	617	0.02%	0.003%
27	4.936	1193	1196	1198	rVB2	717	439	0.01%	0.002%
28	5.052	1213	1232	1267	rBV2	1226107	3160010	100.00%	13.017%
29	5.396	1337	1339	1341	rBV3	1183	717	0.02%	0.003%
30	5.418	1344	1346	1350	rBV5	1079	583	0.02%	0.002%
31	5.460	1355	1359	1361	rBV5	803	506	0.02%	0.002%
32	5.550	1385	1387	1389	rBV2	837	483	0.02%	0.002%
33	5.621	1396	1409	1441	rBV	1031265	2069581	65.49%	8.525%
34	5.910	1489	1499	1514	rBV3	30542	64147	2.03%	0.264%
35	6.074	1535	1550	1582	rBV	695674	1421819	44.99%	5.857%
36	6.409	1652	1654	1657	rVB3	1082	573	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020240.D
 Acq On : 02 Feb 2021 16:08
 Operator : SY/MD
 Sample : M1258-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG503

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis

37	6.537	1691	1694	1701	rVB4	1171	931	0.03%	0.004%
38	6.589	1708	1710	1716	rVB5	769	563	0.02%	0.002%
39	6.618	1716	1719	1723	rVB4	799	449	0.01%	0.002%
40	6.675	1732	1737	1739	rBV4	979	946	0.03%	0.004%
41	6.711	1745	1748	1749	rBV2	896	489	0.02%	0.002%
42	6.785	1769	1771	1775	rVB3	899	647	0.02%	0.003%
43	6.823	1779	1783	1789	rVB5	1447	1586	0.05%	0.007%
44	6.859	1789	1794	1797	rBV3	794	743	0.02%	0.003%
45	6.894	1802	1805	1811	rVB2	1041	928	0.03%	0.004%
46	6.990	1821	1835	1858	rBV	287841	529904	16.77%	2.183%
47	7.241	1909	1913	1914	rBV	624	414	0.01%	0.002%
48	7.318	1925	1937	1961	rBV	1444228	2474516	78.31%	10.194%
49	7.624	2020	2032	2057	rBV	272354	472514	14.95%	1.946%
50	7.830	2093	2096	2101	rBV4	1323	1134	0.04%	0.005%
51	7.945	2125	2132	2139	rBV5	3392	5454	0.17%	0.022%
52	8.048	2161	2164	2166	rVB2	1306	670	0.02%	0.003%
53	8.093	2166	2178	2215	rBV	776193	1439961	45.57%	5.932%
54	8.428	2280	2282	2285	rVB4	1242	552	0.02%	0.002%
55	8.460	2289	2292	2299	rBV7	1000	1460	0.05%	0.006%
56	8.515	2306	2309	2314	rBV5	979	1039	0.03%	0.004%
57	8.550	2318	2320	2322	rBV4	877	453	0.01%	0.002%
58	8.669	2352	2357	2361	rBV5	951	1097	0.03%	0.005%
59	8.775	2388	2390	2391	rBV	901	416	0.01%	0.002%
60	8.801	2396	2398	2402	rBV3	563	443	0.01%	0.002%
61	8.855	2403	2415	2445	rBV	1604196	2574809	81.48%	10.607%
62	9.273	2541	2545	2549	rBV4	872	816	0.03%	0.003%
63	9.351	2565	2569	2572	rVV2	547	532	0.02%	0.002%
64	9.386	2578	2580	2584	rVB2	799	498	0.02%	0.002%
65	9.791	2703	2706	2710	rBV	423	405	0.01%	0.002%
66	10.222	2827	2840	2865	rVV	888197	1374238	43.49%	5.661%
67	10.392	2883	2893	2902	rVB3	7636	12701	0.40%	0.052%
68	10.543	2938	2940	2942	rBV3	882	475	0.02%	0.002%
69	10.611	2958	2961	2967	rBV5	1268	1607	0.05%	0.007%
70	10.643	2967	2971	2973	rBV2	508	408	0.01%	0.002%
71	10.974	3072	3074	3077	rBV4	683	434	0.01%	0.002%
72	11.010	3083	3085	3087	rBV3	692	422	0.01%	0.002%
73	11.087	3106	3109	3114	rBV5	1142	701	0.02%	0.003%
74	11.145	3124	3127	3128	rBV2	830	436	0.01%	0.002%
75	11.254	3149	3161	3184	rBV	1681380	2579971	81.64%	10.628%
76	11.518	3241	3243	3250	rVB5	971	1048	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020240.D
 Acq On : 02 Feb 2021 16:08
 Operator : SY/MD
 Sample : M1258-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG503

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

77	11.630	3265	3278	3300	rBV	1526912	2383739	75.43%	9.820%
78	11.862	3346	3350	3354	rBV7	1051	963	0.03%	0.004%
79	11.907	3361	3364	3369	rBV3	737	561	0.02%	0.002%
80	12.013	3395	3397	3400	rVB5	716	413	0.01%	0.002%
81	12.193	3451	3453	3457	rVB2	898	630	0.02%	0.003%
82	12.225	3461	3463	3466	rBV2	591	394	0.01%	0.002%
83	12.254	3470	3472	3476	rBV3	1254	848	0.03%	0.003%
84	12.537	3556	3560	3566	rVV5	905	939	0.03%	0.004%
85	12.659	3594	3598	3606	rVB8	2028	1985	0.06%	0.008%
86	12.743	3622	3624	3626	rBV2	853	412	0.01%	0.002%
87	12.913	3673	3677	3678	rBV3	814	563	0.02%	0.002%
88	12.939	3683	3685	3689	rVB4	1374	830	0.03%	0.003%
89	13.016	3707	3709	3712	rBV3	681	405	0.01%	0.002%
90	13.164	3751	3755	3756	rBV2	842	584	0.02%	0.002%
91	13.174	3756	3758	3760	rVV3	986	402	0.01%	0.002%
92	13.453	3841	3845	3846	rBV3	1241	937	0.03%	0.004%
93	13.833	3961	3963	3967	rBV3	919	651	0.02%	0.003%
94	14.035	4024	4026	4031	rBV4	913	719	0.02%	0.003%
95	14.061	4031	4034	4041	rVB7	1217	1319	0.04%	0.005%
96	14.128	4052	4055	4060	rVB5	992	886	0.03%	0.004%
97	14.456	4154	4157	4159	rBV2	1576	902	0.03%	0.004%
98	14.556	4185	4188	4193	rBV5	1237	1023	0.03%	0.004%
99	14.707	4232	4235	4236	rBV2	923	489	0.02%	0.002%
100	14.878	4286	4288	4289	rBV2	1193	456	0.01%	0.002%




Sum of corrected areas: 24275418

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020240.D
Acq On : 02 Feb 2021 16:08
Operator : SY/MD
Sample : M1258-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG503

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

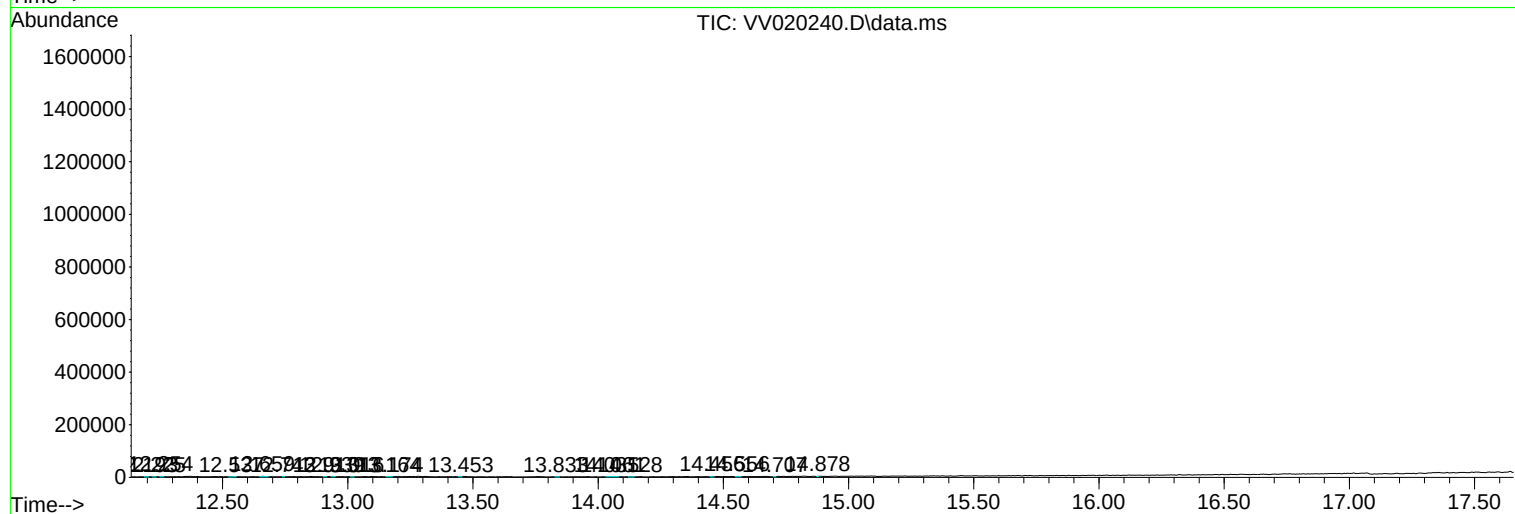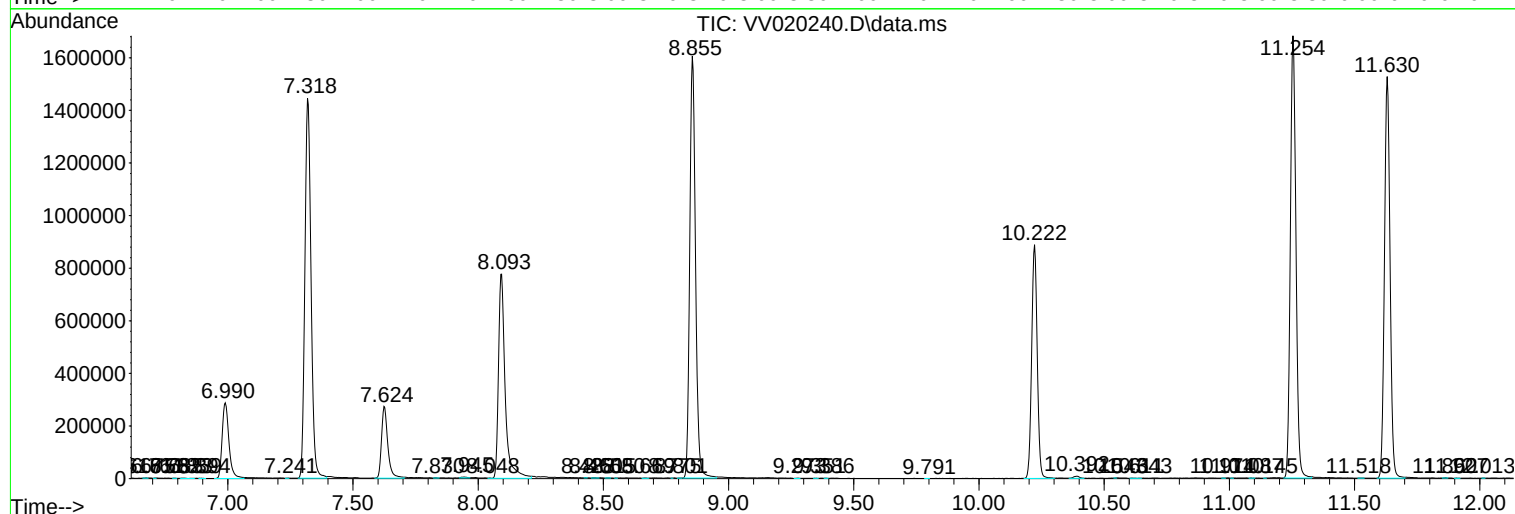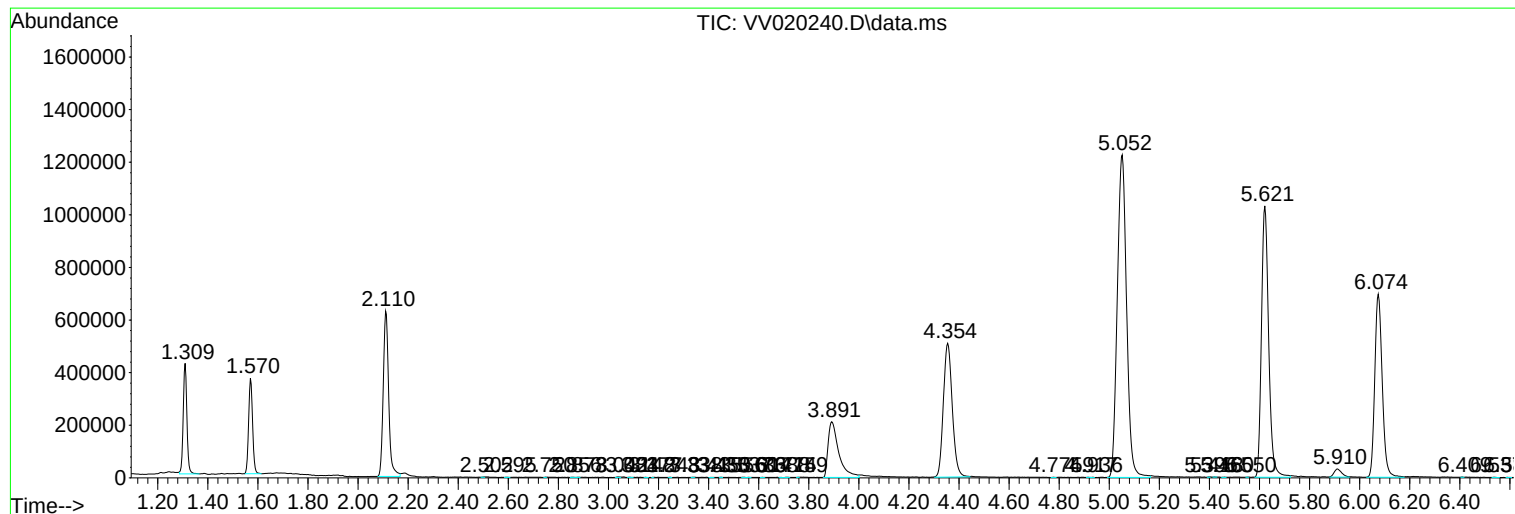

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020240.D
Acq On : 02 Feb 2021 16:08
Operator : SY/MD
Sample : M1258-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG503

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020240.D
Acq On : 02 Feb 2021 16:08
Operator : SY/MD
Sample : M1258-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG503

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
