

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020248.D
 Acq On : 02 Feb 2021 19:15
 Operator : SY/MD
 Sample : M1258-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG530

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

Signal : TIC: VV020248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	79	rVB	270740	269868	12.16%	1.505%
2	1.569	142	149	162	rVB	209014	226656	10.21%	1.264%
3	2.110	306	317	336	rBV	469641	707285	31.88%	3.943%
4	2.296	368	375	390	rVB	5934	8958	0.40%	0.050%
5	2.383	400	402	404	rBV2	301	156	0.01%	0.001%
6	2.463	425	427	430	rVB2	506	278	0.01%	0.002%
7	2.479	430	432	434	rBV	293	163	0.01%	0.001%
8	2.502	434	439	441	rBV3	1191	1040	0.05%	0.006%
9	2.624	473	477	478	rBV2	295	215	0.01%	0.001%
10	2.669	487	491	495	rBV2	545	606	0.03%	0.003%
11	2.946	575	577	582	rVB3	451	308	0.01%	0.002%
12	3.045	594	608	627	rBV2	18443	36459	1.64%	0.203%
13	3.158	640	643	644	rBV	430	207	0.01%	0.001%
14	3.200	653	656	660	rBV3	365	258	0.01%	0.001%
15	3.232	664	666	668	rBV2	154	37	0.00%	0.000%
16	3.248	668	671	672	rBV2	178	101	0.00%	0.001%
17	3.286	678	683	687	rBV4	699	875	0.04%	0.005%
18	3.466	738	739	740	rBV4	93	34	0.00%	0.000%
19	3.486	740	745	747	rVV2	170	140	0.01%	0.001%
20	3.502	747	750	751	rBV2	257	161	0.01%	0.001%
21	3.624	787	788	789	rVB2	117	23	0.00%	0.000%
22	3.637	789	792	794	rBV	140	73	0.00%	0.000%
23	3.653	794	797	802	rBV2	150	112	0.01%	0.001%
24	3.675	802	804	806	rBV	115	60	0.00%	0.000%
25	3.692	807	809	811	rVB2	184	58	0.00%	0.000%
26	3.711	811	815	819	rBV2	362	246	0.01%	0.001%
27	3.772	819	834	850	rVB4	7276	17293	0.78%	0.096%
28	3.846	853	857	858	rBV2	134	91	0.00%	0.001%
29	3.888	859	870	902	rBV	142803	401625	18.10%	2.239%
30	4.354	999	1015	1041	rBV	356531	870316	39.22%	4.852%
31	4.637	1101	1103	1105	rBV2	474	205	0.01%	0.001%
32	4.650	1105	1107	1110	rBV2	537	292	0.01%	0.002%
33	4.736	1131	1134	1137	rBV	284	218	0.01%	0.001%
34	4.749	1137	1138	1139	rBV	255	87	0.00%	0.000%
35	4.852	1168	1170	1172	rVB	187	82	0.00%	0.000%
36	4.868	1172	1175	1176	rBV	301	114	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020248.D
 Acq On : 02 Feb 2021 19:15
 Operator : SY/MD
 Sample : M1258-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG530

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis

37	4.878	1176	1178	1181	rVV2	235	117	0.01%	0.001%
38	4.952	1199	1201	1203	rBV	268	130	0.01%	0.001%
39	5.052	1214	1232	1267	rBV2	862901	2218906	100.00%	12.370%
40	5.466	1358	1361	1363	rBV	474	297	0.01%	0.002%
41	5.492	1366	1369	1371	rVV2	635	296	0.01%	0.002%
42	5.518	1375	1377	1380	rVB2	580	306	0.01%	0.002%
43	5.540	1380	1384	1386	rBV2	549	350	0.02%	0.002%
44	5.621	1396	1409	1437	rBV	765076	1537346	69.28%	8.571%
45	5.913	1490	1500	1515	rBV4	9673	20816	0.94%	0.116%
46	6.074	1537	1550	1584	rVB	480482	970384	43.73%	5.410%
47	6.344	1631	1634	1637	rVB	752	378	0.02%	0.002%
48	6.363	1637	1640	1641	rBV	324	139	0.01%	0.001%
49	6.479	1674	1676	1678	rBV	216	105	0.00%	0.001%
50	6.630	1722	1723	1725	rBV	239	121	0.01%	0.001%
51	6.675	1735	1737	1742	rVB3	681	551	0.02%	0.003%
52	6.830	1782	1785	1786	rBV	263	137	0.01%	0.001%
53	6.926	1811	1815	1816	rBV	369	228	0.01%	0.001%
54	6.990	1823	1835	1867	rBV	264537	488026	21.99%	2.721%
55	7.318	1925	1937	1972	rBV	1102161	1901236	85.68%	10.599%
56	7.624	2021	2032	2052	rBV	188661	327511	14.76%	1.826%
57	7.920	2120	2124	2126	rBV3	802	636	0.03%	0.004%
58	8.051	2162	2165	2167	rBV3	438	323	0.01%	0.002%
59	8.090	2167	2177	2221	rVV	522190	951298	42.87%	5.304%
60	8.579	2325	2329	2333	rBV3	604	532	0.02%	0.003%
61	8.614	2338	2340	2344	rVV3	717	457	0.02%	0.003%
62	8.643	2348	2349	2353	rVB3	604	282	0.01%	0.002%
63	8.662	2353	2355	2356	rBV	227	86	0.00%	0.000%
64	8.727	2373	2375	2377	rBV	170	64	0.00%	0.000%
65	8.762	2383	2386	2388	rBV2	452	326	0.01%	0.002%
66	8.855	2403	2415	2444	rBV	1188328	1900988	85.67%	10.598%
67	9.183	2515	2517	2518	rBV	285	101	0.00%	0.001%
68	9.225	2525	2530	2532	rBV	741	614	0.03%	0.003%
69	9.540	2626	2628	2631	rBV	305	138	0.01%	0.001%
70	10.039	2779	2783	2784	rBV2	383	254	0.01%	0.001%
71	10.112	2802	2806	2810	rBV	464	400	0.02%	0.002%
72	10.222	2827	2840	2865	rBV	721385	1131533	51.00%	6.308%
73	10.675	2979	2981	2985	rBV2	316	194	0.01%	0.001%
74	10.858	3034	3038	3043	rBV5	1091	944	0.04%	0.005%
75	11.254	3149	3161	3181	rBV	1297350	1973895	88.96%	11.005%
76	11.630	3265	3278	3308	rBV	1280132	1961982	88.42%	10.938%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020248.D
Acq On : 02 Feb 2021 19:15
Operator : SY/MD
Sample : M1258-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG530

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Title : VOC Analysis




Sum of corrected areas: 17937127

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020248.D
Acq On : 02 Feb 2021 19:15
Operator : SY/MD
Sample : M1258-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG530

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

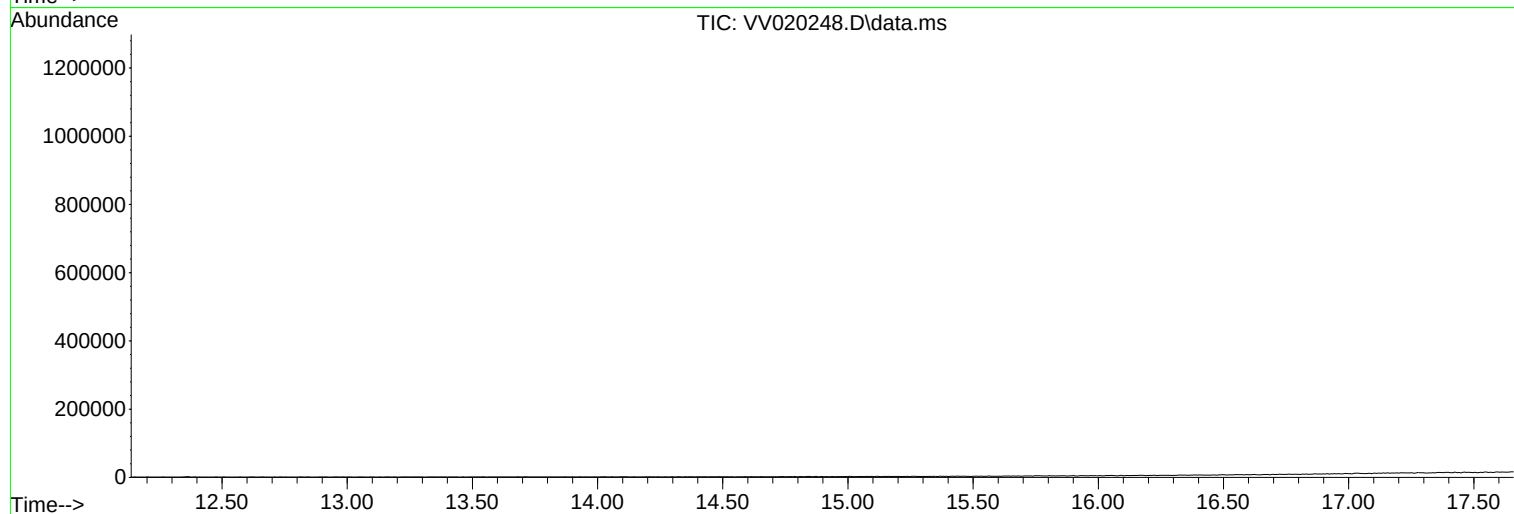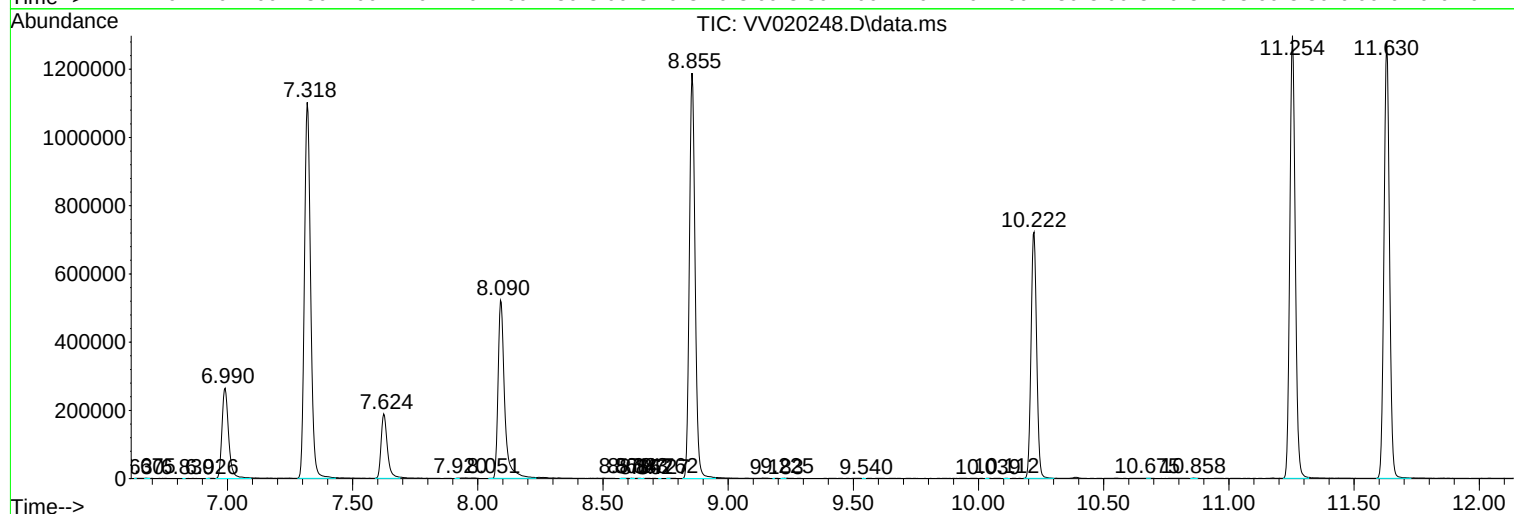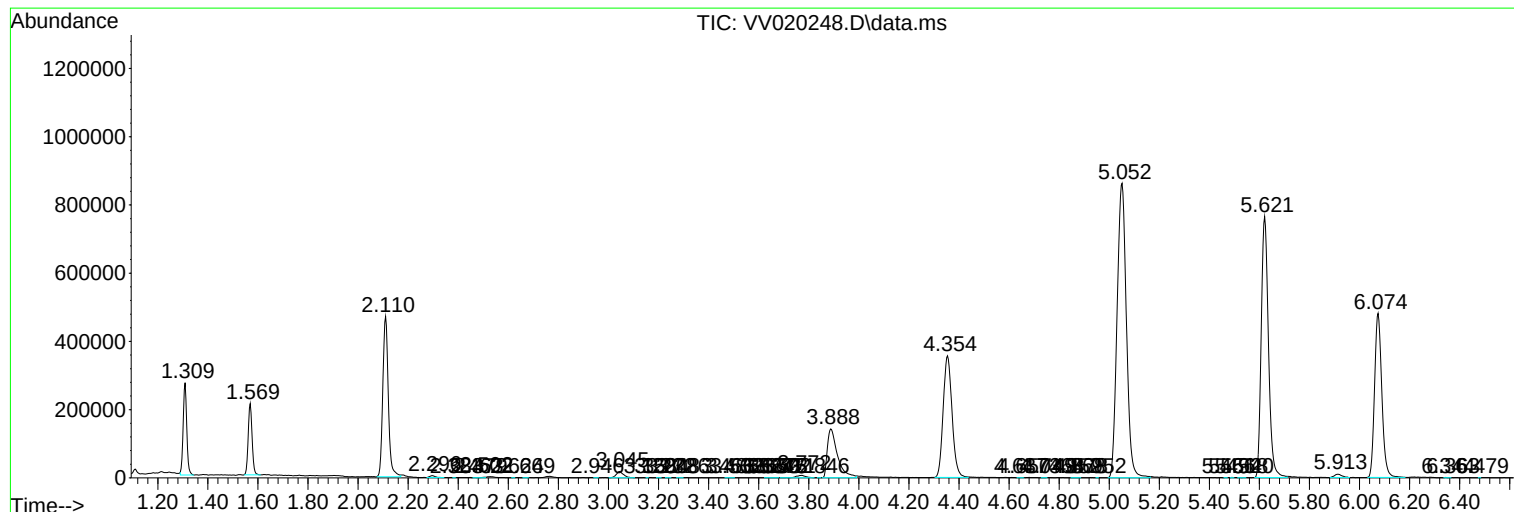

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020248.D
Acq On : 02 Feb 2021 19:15
Operator : SY/MD
Sample : M1258-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG530

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020248.D
Acq On : 02 Feb 2021 19:15
Operator : SY/MD
Sample : M1258-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG530

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
