

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020251.D
 Acq On : 02 Feb 2021 20:26
 Operator : SY/MD
 Sample : VIBLK82
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

Signal : TIC: VV020251.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	89	rVB	270425	282772	13.09%	1.544%
2	1.569	143	149	161	rVB	215827	240251	11.12%	1.311%
3	2.110	307	317	349	rVB	442226	670360	31.04%	3.659%
4	2.351	390	392	395	rBV3	537	237	0.01%	0.001%
5	2.389	402	404	406	rBV	340	193	0.01%	0.001%
6	2.463	425	427	432	rBV3	410	305	0.01%	0.002%
7	2.508	434	441	452	rVB9	2774	4774	0.22%	0.026%
8	2.868	550	553	558	rVB2	483	363	0.02%	0.002%
9	2.888	558	559	561	rBV	75	24	0.00%	0.000%
10	2.897	561	562	563	rBV	121	29	0.00%	0.000%
11	2.930	569	572	574	rVB	479	247	0.01%	0.001%
12	2.946	574	577	581	rBV2	412	284	0.01%	0.002%
13	2.978	581	587	590	rVB3	416	355	0.02%	0.002%
14	2.994	590	592	594	rBV	388	201	0.01%	0.001%
15	3.039	599	606	607	rBV4	1091	1011	0.05%	0.006%
16	3.106	624	627	631	rBV2	283	183	0.01%	0.001%
17	3.122	631	632	635	rVB2	308	145	0.01%	0.001%
18	3.139	635	637	638	rBV	156	49	0.00%	0.000%
19	3.235	664	667	671	rBV2	354	211	0.01%	0.001%
20	3.267	676	677	678	rVB2	110	21	0.00%	0.000%
21	3.277	678	680	684	rBV2	194	118	0.01%	0.001%
22	3.296	684	686	687	rBV	317	76	0.00%	0.000%
23	3.338	695	699	702	rVB	295	218	0.01%	0.001%
24	3.354	702	704	707	rBV	158	99	0.00%	0.001%
25	3.367	707	708	709	rBV	230	56	0.00%	0.000%
26	3.376	709	711	713	rBV2	273	126	0.01%	0.001%
27	3.412	721	722	726	rBB	124	63	0.00%	0.000%
28	3.438	726	730	734	rBV	342	270	0.01%	0.001%
29	3.534	756	760	768	rBV2	257	312	0.01%	0.002%
30	3.579	770	774	776	rBV2	233	218	0.01%	0.001%
31	3.663	798	800	801	rBV	170	74	0.00%	0.000%
32	3.717	814	817	819	rBV	229	168	0.01%	0.001%
33	3.785	835	838	843	rVB2	309	250	0.01%	0.001%
34	3.817	845	848	851	rBV	233	132	0.01%	0.001%
35	3.830	851	852	853	rBV	136	47	0.00%	0.000%
36	3.894	861	872	911	rBV2	141900	426016	19.72%	2.326%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020251.D
 Acq On : 02 Feb 2021 20:26
 Operator : SY/MD
 Sample : VIBLK82
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis

37	4.354	999	1015	1046	rBV	358893	853948	39.54%	4.662%
38	4.647	1104	1106	1112	rVB2	608	410	0.02%	0.002%
39	4.672	1112	1114	1117	rBV3	485	375	0.02%	0.002%
40	4.717	1126	1128	1129	rVB3	209	54	0.00%	0.000%
41	4.727	1129	1131	1134	rBV3	368	222	0.01%	0.001%
42	4.843	1165	1167	1171	rVB2	424	196	0.01%	0.001%
43	4.868	1172	1175	1179	rVB3	345	195	0.01%	0.001%
44	5.052	1214	1232	1258	rBV2	846211	2159931	100.00%	11.791%
45	5.383	1333	1335	1338	rVB3	441	223	0.01%	0.001%
46	5.402	1340	1341	1342	rBV	431	95	0.00%	0.001%
47	5.486	1363	1367	1369	rBV2	451	255	0.01%	0.001%
48	5.621	1396	1409	1444	rBV	811349	1629170	75.43%	8.893%
49	5.910	1492	1499	1515	rVB5	8519	17901	0.83%	0.098%
50	6.074	1536	1550	1581	rBV	468011	954953	44.21%	5.213%
51	6.309	1621	1623	1625	rBV2	411	200	0.01%	0.001%
52	6.344	1630	1634	1638	rBV3	488	386	0.02%	0.002%
53	6.360	1638	1639	1640	rBV	304	72	0.00%	0.000%
54	6.415	1653	1656	1658	rBV	370	211	0.01%	0.001%
55	6.553	1697	1699	1702	rVB	360	186	0.01%	0.001%
56	6.572	1702	1705	1707	rBV2	437	265	0.01%	0.001%
57	6.701	1744	1745	1746	rBV2	344	81	0.00%	0.000%
58	6.794	1772	1774	1777	rVB2	496	234	0.01%	0.001%
59	6.810	1777	1779	1781	rBV	201	93	0.00%	0.001%
60	6.855	1791	1793	1796	rBV	236	132	0.01%	0.001%
61	6.891	1799	1804	1808	rBV2	336	312	0.01%	0.002%
62	6.990	1823	1835	1854	rBV	260324	472486	21.88%	2.579%
63	7.251	1914	1916	1917	rBV2	564	191	0.01%	0.001%
64	7.318	1924	1937	1963	rBV	1094134	1865462	86.37%	10.183%
65	7.624	2022	2032	2054	rBV	187005	327428	15.16%	1.787%
66	7.923	2123	2125	2126	rBV	354	163	0.01%	0.001%
67	8.090	2166	2177	2214	rBV	567978	1024457	47.43%	5.592%
68	8.396	2269	2272	2274	rBV2	1273	547	0.03%	0.003%
69	8.605	2332	2337	2339	rBV2	561	444	0.02%	0.002%
70	8.772	2388	2389	2393	rVB	420	157	0.01%	0.001%
71	8.855	2403	2415	2440	rBV	1267162	2049477	94.89%	11.188%
72	9.158	2503	2509	2510	rBV	689	574	0.03%	0.003%
73	9.257	2538	2540	2542	rBV2	381	132	0.01%	0.001%
74	9.286	2547	2549	2551	rVB	395	144	0.01%	0.001%
75	9.299	2551	2553	2555	rBV	178	67	0.00%	0.000%
76	9.563	2632	2635	2638	rVB2	448	275	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020251.D
 Acq On : 02 Feb 2021 20:26
 Operator : SY/MD
 Sample : VIBLK82
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M

Title : VOC Analysis

77	9.624	2652	2654	2656	rVB	357	152	0.01%	0.001%
78	9.801	2706	2709	2712	rBV2	432	327	0.02%	0.002%
79	9.894	2736	2738	2741	rBV2	260	160	0.01%	0.001%
80	9.994	2768	2769	2772	rBV	278	156	0.01%	0.001%
81	10.222	2826	2840	2859	rBV	759500	1184100	54.82%	6.464%
82	10.389	2890	2892	2896	rVB3	657	350	0.02%	0.002%
83	10.431	2903	2905	2907	rBV	399	185	0.01%	0.001%
84	10.678	2980	2982	2983	rBV	250	77	0.00%	0.000%
85	10.704	2988	2990	2994	rVB	548	319	0.01%	0.002%
86	10.775	3008	3012	3016	rBV3	383	322	0.01%	0.002%
87	10.971	3070	3073	3076	rBV2	520	331	0.02%	0.002%
88	11.035	3091	3093	3097	rVB	566	315	0.01%	0.002%
89	11.061	3097	3101	3106	rBV3	455	534	0.02%	0.003%
90	11.254	3149	3161	3186	rBV	1411796	2151145	99.59%	11.743%
91	11.569	3257	3259	3263	rVB2	762	467	0.02%	0.003%
92	11.630	3264	3278	3297	rBV	1291729	1987654	92.02%	10.850%




Sum of corrected areas: 18318956

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020251.D
Acq On : 02 Feb 2021 20:26
Operator : SY/MD
Sample : VIBLK82
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

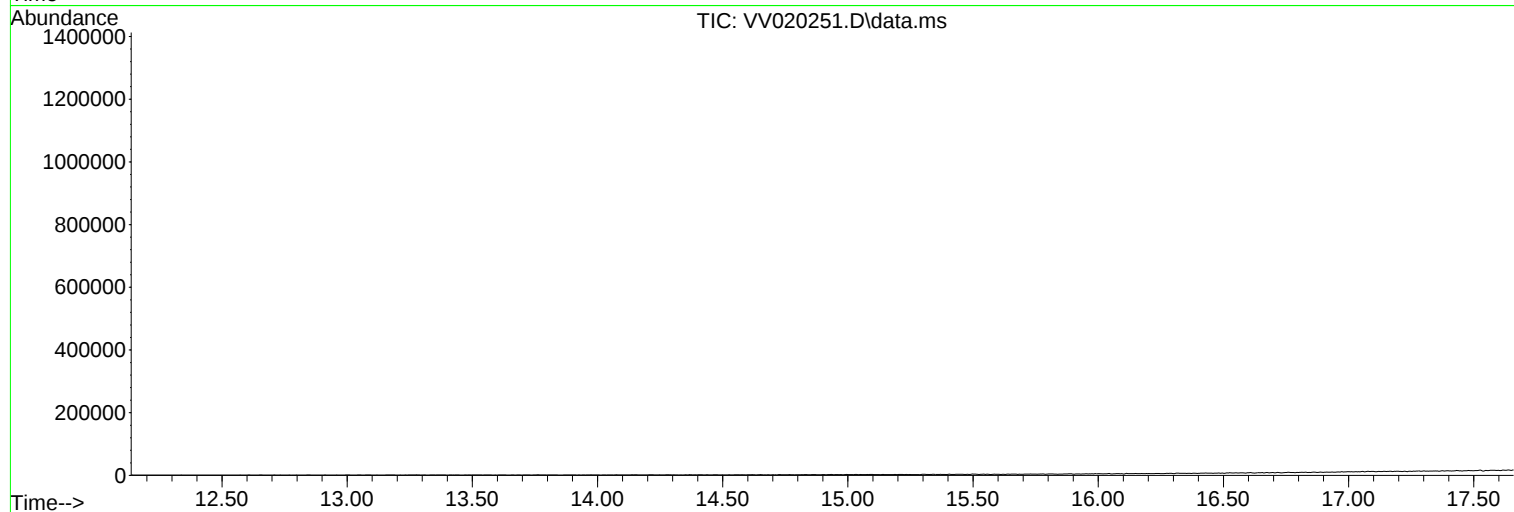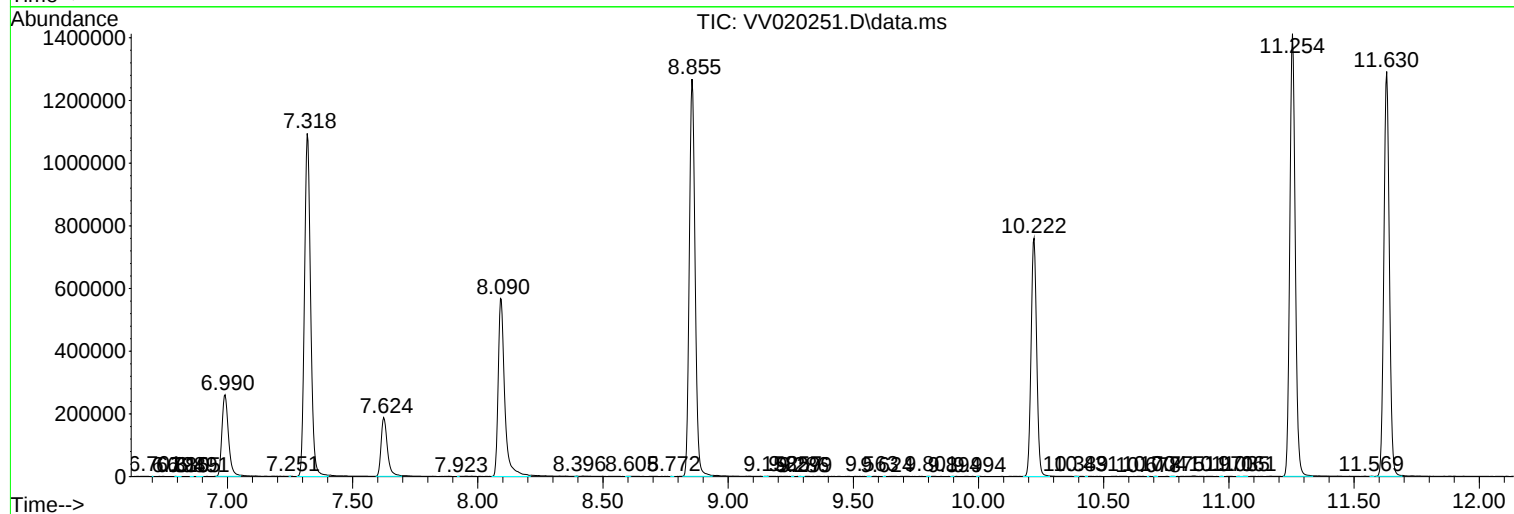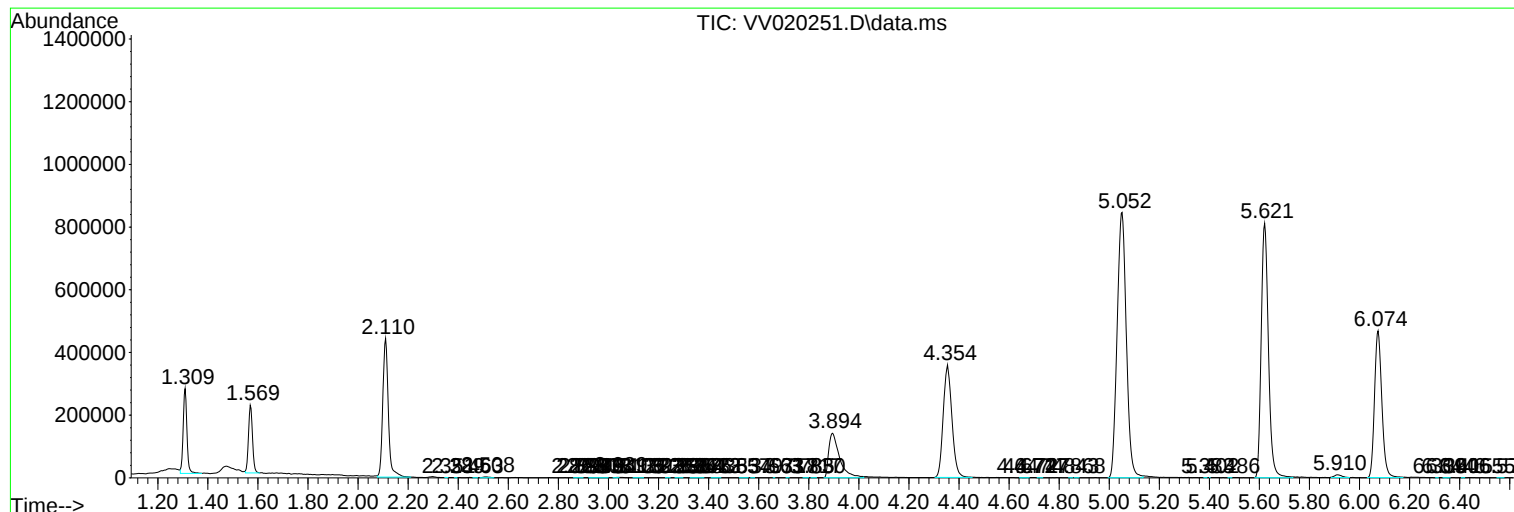

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020251.D
Acq On : 02 Feb 2021 20:26
Operator : SY/MD
Sample : VIBLK82
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
Data File : VV020251.D
Acq On : 02 Feb 2021 20:26
Operator : SY/MD
Sample : VIBLK82
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
