
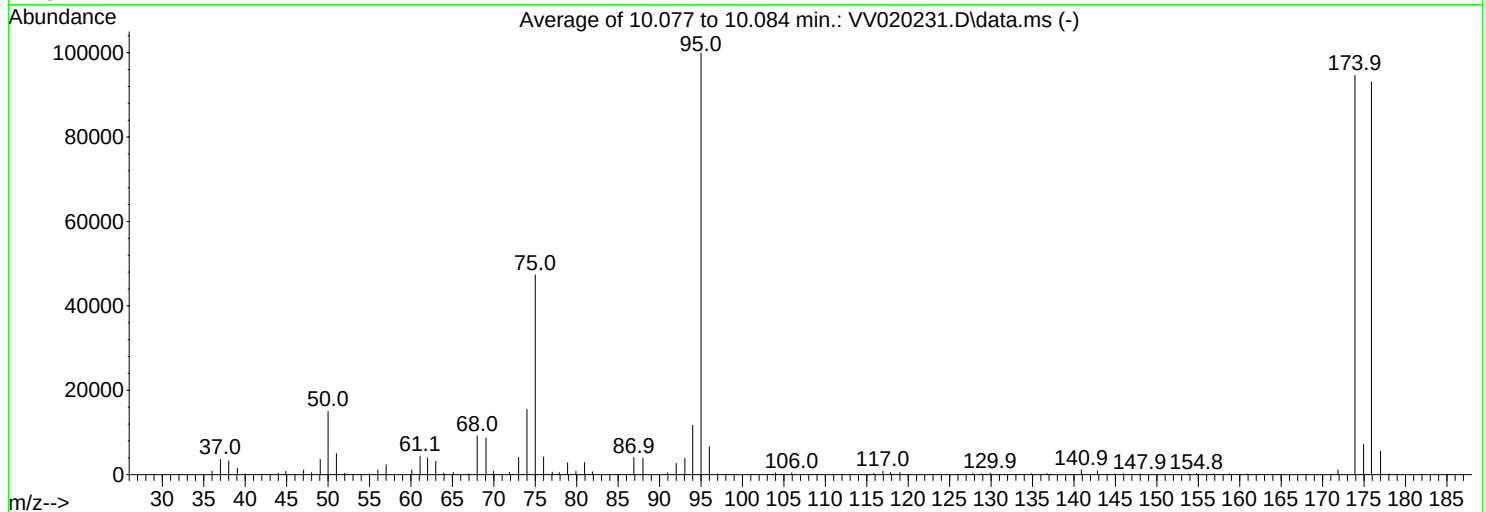


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020221\
 Data File : VV020231.D
 Acq On : 02 Feb 2021 11:09
 Operator : SY/MD
 Sample : BFB84
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB84

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012821WMA.M
 Title : VOC Analysis
 Last Update : Wed Feb 03 02:27:31 2021

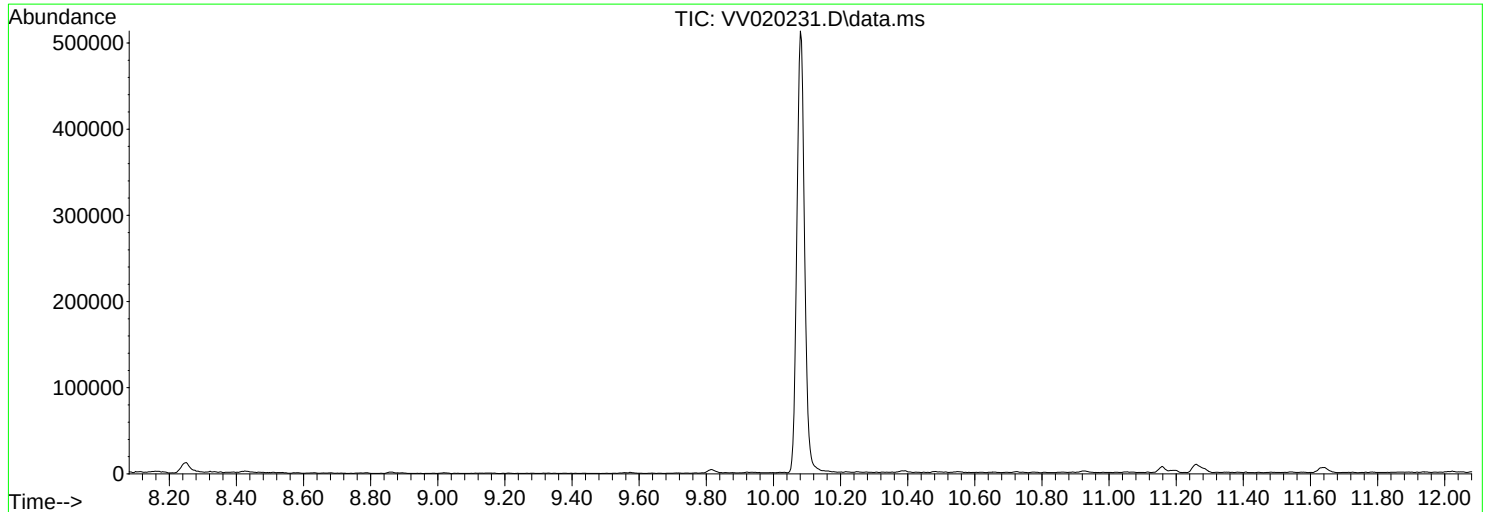

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2783

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.0	15009	PASS
75	95	30	80	47.4	47349	PASS
95	95	100	100	100.0	99960	PASS
96	95	5	9	6.7	6653	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	94.7	94648	PASS
175	174	5	9	7.6	7195	PASS
176	174	95	101	98.3	93045	PASS
177	176	5	9	6.0	5576	PASS

m/z	Abundance
35.00	272.0
36.00	478.0
38.00	190.0
44.10	472.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	1278.0
37.00	3834.0
38.00	3474.0
39.00	1485.0
40.00	304.0
44.00	819.0
44.90	824.0
47.00	1034.0
47.90	436.0
49.00	3431.0
50.00	15067.0
51.00	4844.0
52.00	277.0
55.00	243.0
56.00	1114.0
57.00	2212.0
58.10	139.0
60.10	1110.0
61.10	4121.0
62.00	3875.0
63.00	3147.0
64.00	417.0
65.10	604.0
66.80	216.0
68.00	9007.0
69.10	8251.0
70.00	842.0
71.90	496.0
73.00	3828.0
74.00	14791.0
75.00	47320.0
76.00	3978.0
77.10	567.0
77.90	468.0
78.90	2682.0
79.90	807.0
80.90	2747.0
81.90	722.0
86.90	3975.0
88.00	3716.0
90.90	372.0
92.00	2535.0
93.00	3724.0
94.00	10750.0
95.00	96488.0
96.00	6702.0
97.00	208.0
104.00	373.0
104.70	108.0
105.90	402.0
110.80	134.0
115.10	126.0
115.90	298.0
116.90	771.0
117.80	490.0
119.00	429.0
127.80	325.0
128.90	189.0
129.90	364.0
131.00	137.0
134.90	238.0
136.80	339.0
140.90	1057.0
142.80	827.0
144.00	120.0
145.00	187.0
145.90	251.0
148.00	193.0
153.80	124.0
154.80	263.0
156.80	209.0
158.70	158.0
160.80	145.0
171.80	1093.0
173.90	89088.0
175.00	7002.0
175.90	87128.0
177.00	5432.0
178.00	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	1331.0
37.00	3671.0
38.00	3597.0
39.10	1594.0
40.00	256.0
42.50	123.0
44.00	864.0
44.90	847.0
45.90	110.0
47.10	1087.0
48.00	473.0
49.10	3730.0
50.00	15525.0
51.00	5200.0
52.00	332.0
54.90	228.0
56.00	1143.0
57.00	2401.0
58.00	130.0
60.10	1186.0
61.10	4494.0
62.00	4062.0
63.00	3237.0
63.90	386.0
65.10	531.0
66.90	196.0
67.10	198.0
68.00	9544.0
69.00	8926.0
70.00	827.0
71.90	535.0
73.00	4222.0
74.00	16055.0
75.00	48808.0
76.00	4331.0
77.00	645.0
77.90	515.0
78.90	2942.0
79.90	813.0
81.00	2932.0
81.90	700.0
86.90	4175.0
88.00	4083.0
90.90	473.0
92.00	2720.0
93.00	3897.0
94.00	12154.0
95.00	103520.0
96.00	6912.0
96.90	251.0
104.00	433.0
104.80	122.0
105.90	437.0
110.80	132.0
114.80	122.0
115.10	129.0
115.80	332.0
116.90	889.0
117.80	484.0
119.00	525.0
127.80	382.0
128.80	194.0
129.90	395.0
130.90	143.0
134.90	283.0
136.70	304.0
137.20	167.0
140.90	1195.0
141.90	114.0
142.90	867.0
144.90	237.0
145.90	280.0
148.00	196.0
153.80	150.0
154.80	320.0
156.80	235.0
158.80	187.0
160.90	144.0
171.80	1153.0
173.90	97296.0
175.00	7368.0
175.90	95864.0
177.00	5697.0
178.00	211.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	1316.0
37.00	3333.0
38.10	3277.0
39.10	1432.0
40.00	178.0
40.40	183.0
43.00	118.0
44.00	888.0
44.90	694.0
46.00	154.0
47.00	1051.0
48.10	510.0
49.10	3620.0
50.00	14436.0
51.00	4949.0
52.00	294.0
55.00	172.0
56.00	1088.0
57.00	2442.0
57.90	150.0
60.10	1054.0
61.10	4494.0
62.00	3869.0
63.00	3202.0
63.90	351.0
65.10	521.0
67.10	193.0
68.00	9143.0
69.00	8831.0
69.90	726.0
71.90	535.0
73.00	4297.0
74.00	15589.0
75.00	45920.0
76.00	4257.0
77.00	592.0
77.90	505.0
78.90	2820.0
79.90	825.0
81.00	2849.0
81.90	667.0
85.90	144.0
86.90	4051.0
88.00	3874.0
91.00	497.0
92.00	2704.0
93.10	3990.0
94.00	12208.0
95.00	99872.0
96.00	6346.0
96.90	211.0
104.00	448.0
104.80	148.0
106.00	436.0
110.90	135.0
114.70	129.0
115.10	110.0
115.80	395.0
117.00	860.0
117.90	436.0
119.00	566.0
123.90	109.0
127.80	349.0
128.90	173.0
129.90	396.0
134.90	288.0
136.70	232.0
137.20	155.0
140.90	1187.0
141.90	129.0
142.90	878.0
144.90	260.0
146.00	237.0
147.90	198.0
153.90	141.0
154.80	295.0
156.90	256.0
158.80	199.0
161.00	163.0
171.90	1170.0
173.90	97560.0
174.90	7214.0
175.90	96144.0
177.00	5600.0
178.00	258.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84