


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020222\
Data File : VV024530.D
Acq On : 02 Feb 2022 17:22
Operator : SY/MD
Sample : N1353-04MEDL 10X
Misc : 2.91g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0VE5MEDL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 06:26:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Feb 03 05:56:12 2022
Response via : Initial Calibration

Reviewed By :John Carlone 02/03/2022
Supervised By :Mahesh Dadoda 02/04/2022

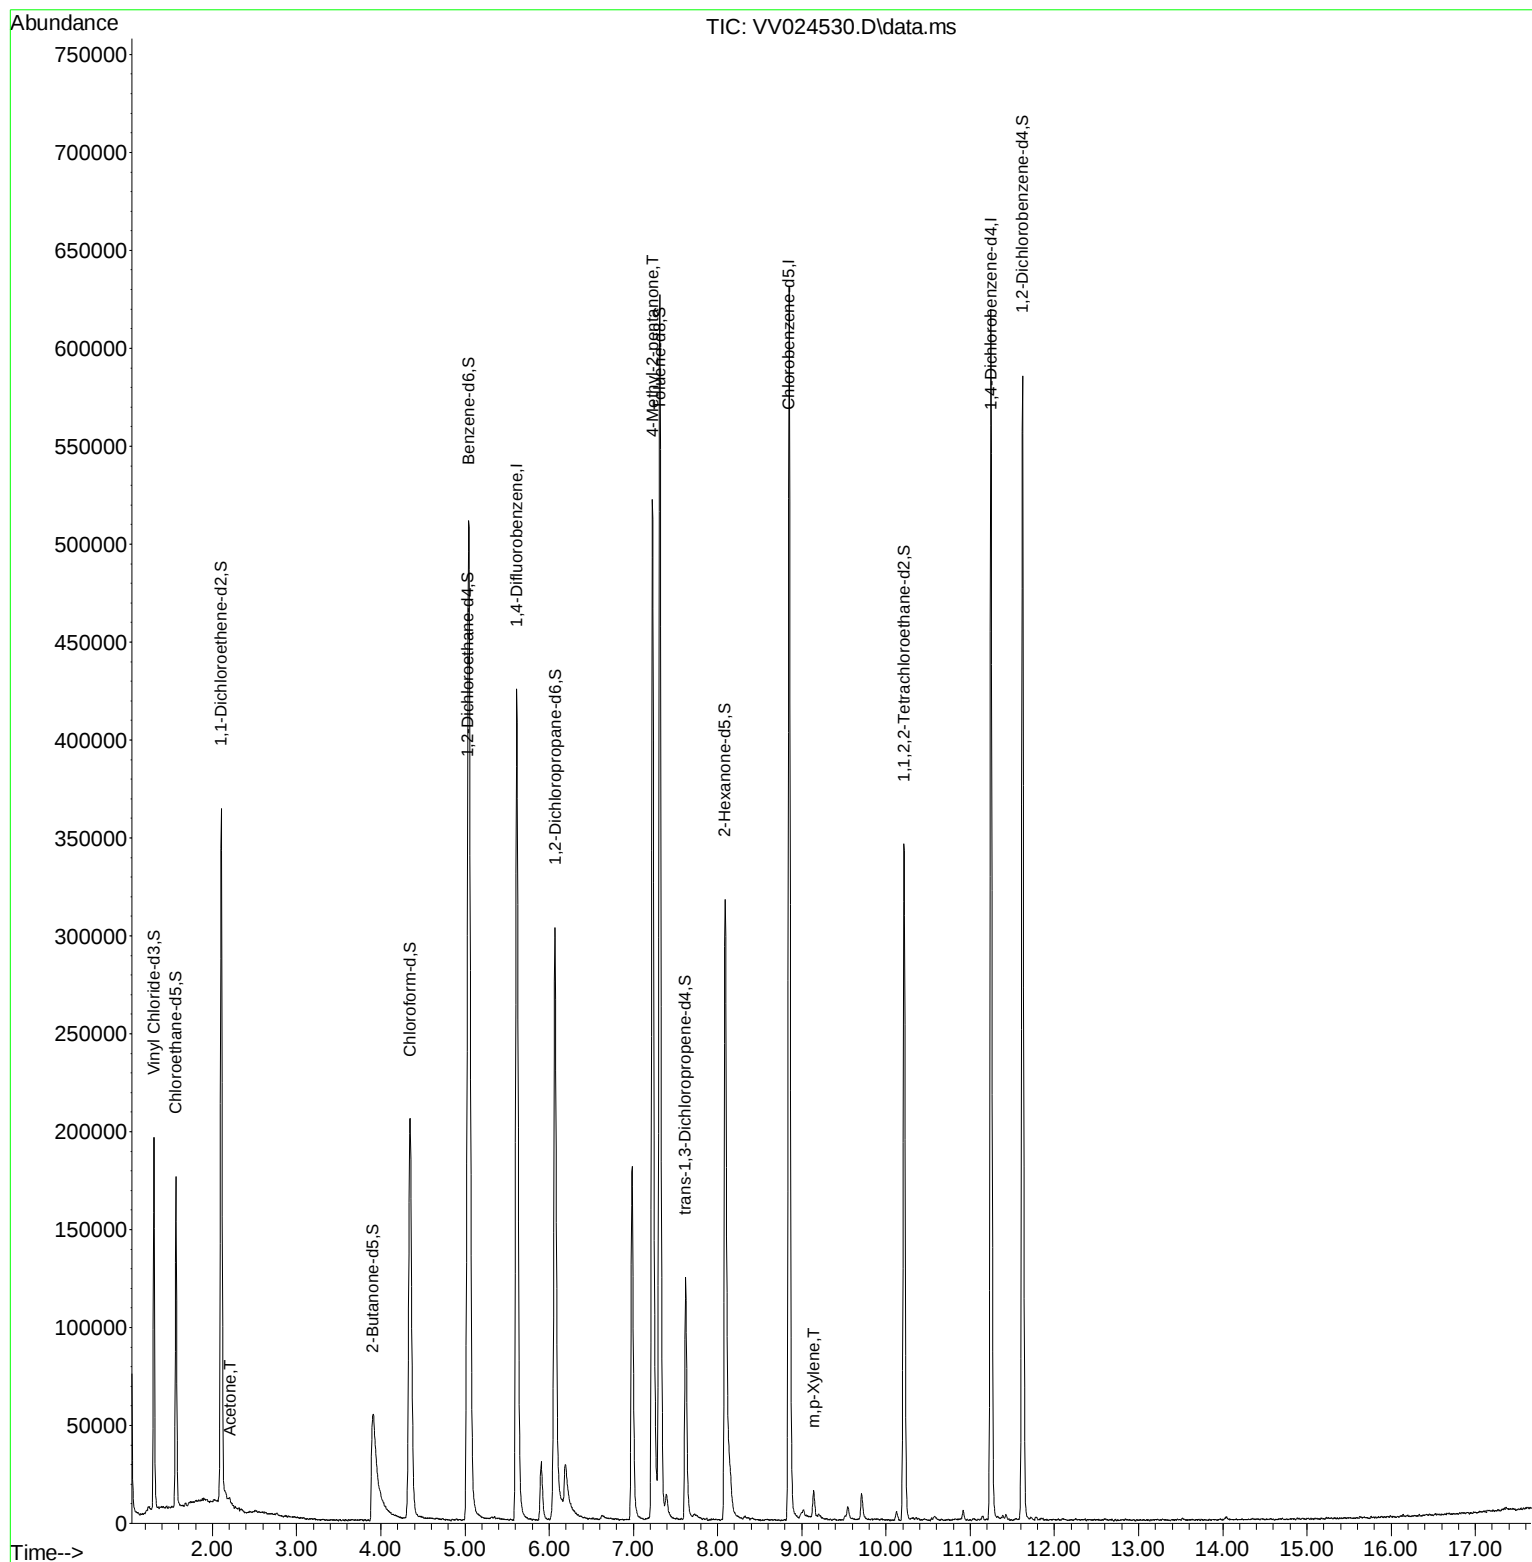




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020222\
 Data File : VV024530.D
 Acq On : 02 Feb 2022 17:22
 Operator : SY/MD
 Sample : N1353-04MEDL 10X
 Misc : 2.91g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0VE5MEDL

Manual IntegrationsAPPROVED

Quant Time: Feb 05 03:30:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Feb 05 00:18:38 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/03/2022
 Supervised By :Mahesh Dadoda 02/04/2022

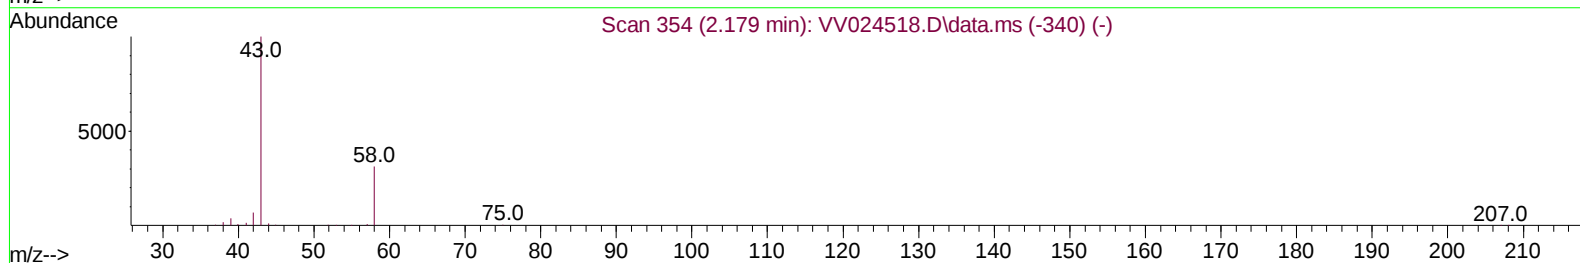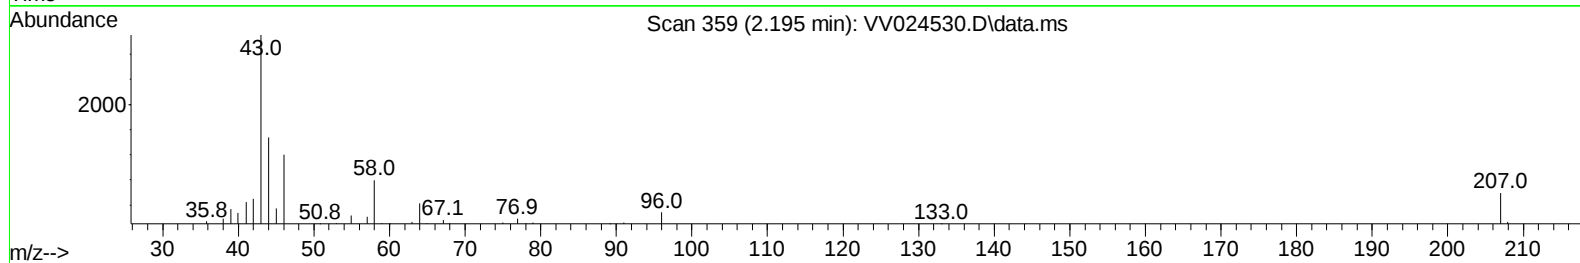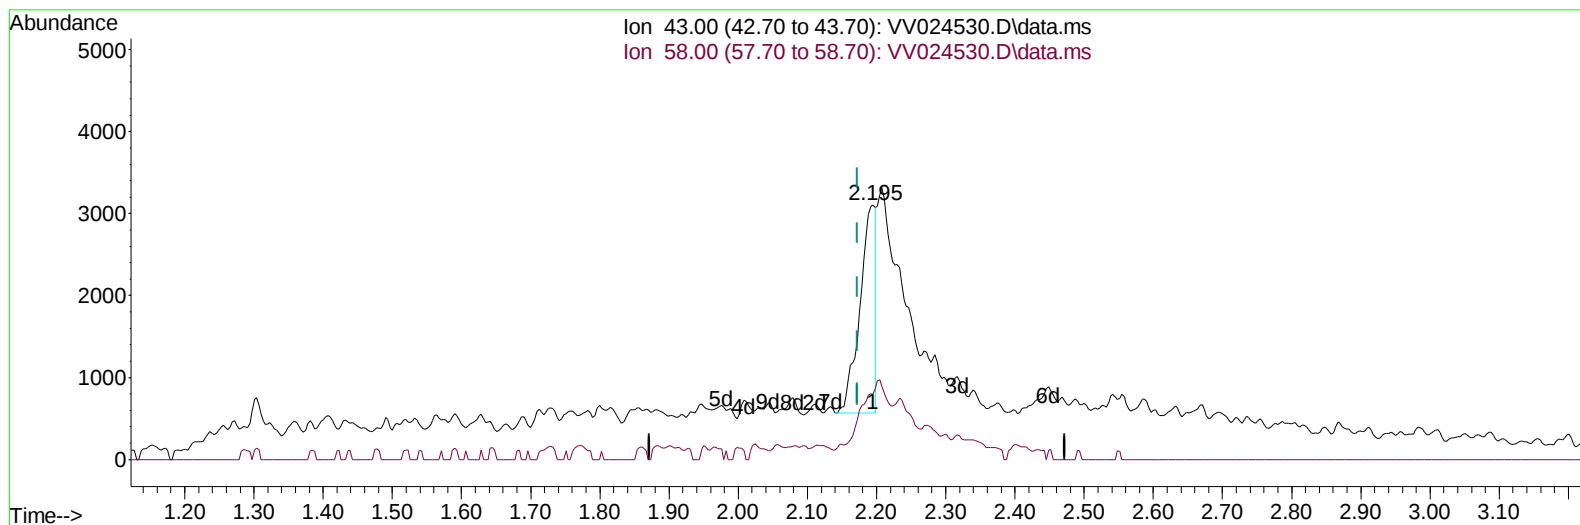

TIC: VV024530.D\data.ms

(13) Acetone (T)

2.195min (+ 0.022) 2.23 ug/L

response 3945

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	21.70
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020222\
 Data File : VV024530.D
 Acq On : 02 Feb 2022 17:22
 Operator : SY/MD
 Sample : N1353-04MEDL 10X
 Misc : 2.91g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COVE5MEDL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 06:26:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Feb 03 05:56:12 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/03/2022
 Supervised By :Mahesh Dadoda 02/04/2022

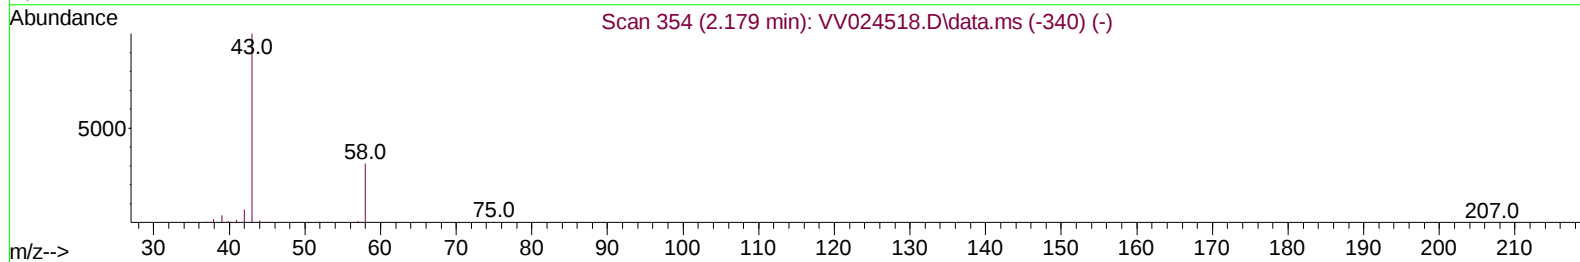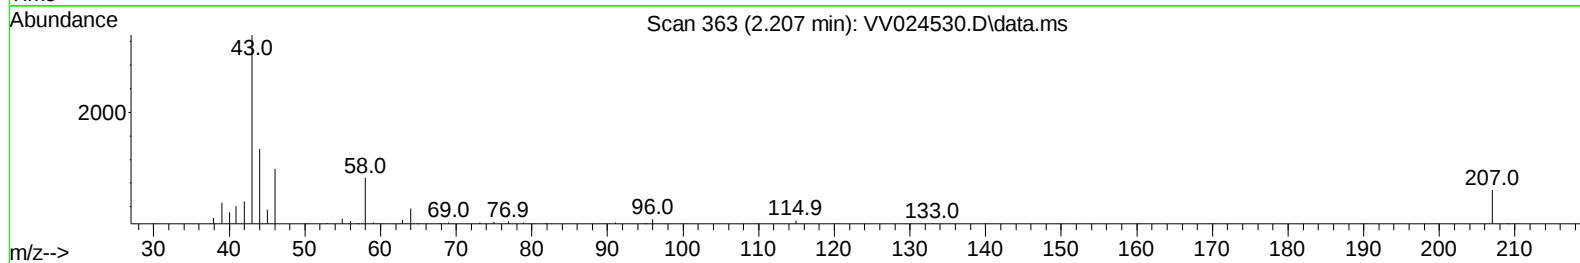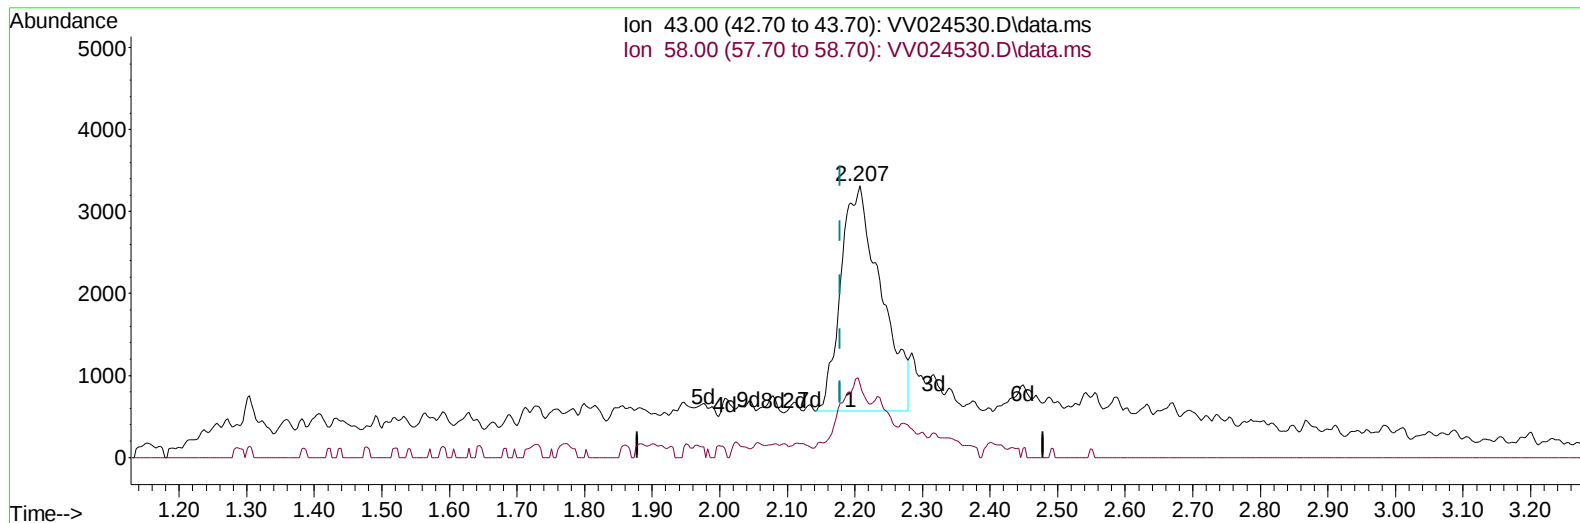

TIC: VV024530.D\data.ms

(13) Acetone (T)

2.207min (+ 0.029) 6.37 ug/L m

response 11269

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	7.60
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020222\
 Data File : VV024530.D
 Acq On : 02 Feb 2022 17:22
 Operator : SY/MD
 Sample : N1353-04MEDL 10X
 Misc : 2.91g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COVE5MEDL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 06:26:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Feb 03 05:56:12 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/03/2022
 Supervised By :Mahesh Dadoda 02/04/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	358411	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	324813	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	142027	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	119625	47.001	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	94.000%	
7) Chloroethane-d5	1.568	69	101717	45.852	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	91.700%	
11) 1,1-Dichloroethene-d2	2.105	63	187600	36.997	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	74.000%	
21) 2-Butanone-d5	3.908	46	154471	91.763	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	91.760%	
24) Chloroform-d	4.346	84	214894	45.974	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.940%	
26) 1,2-Dichloroethane-d4	5.030	65	140113	46.963	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	93.920%	
32) Benzene-d6	5.047	84	435971	47.206	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	94.420%	
36) 1,2-Dichloropropane-d6	6.069	67	141086	47.987	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	95.980%	
41) Toluene-d8	7.313	98	398570	46.892	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	93.780%	
43) trans-1,3-Dichloroprop...	7.619	79	71550	46.247	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	92.500%	
47) 2-Hexanone-d5	8.088	63	124905	100.026	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	100.030%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	167190	47.433	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	94.860%	
66) 1,2-Dichlorobenzene-d4	11.622	152	132649	49.364	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	98.720%	
Target Compounds						
13) Acetone	2.207	43	11269m	6.368	ug/L	
40) 4-Methyl-2-pentanone	7.227	43	369801	108.349	ug/L	99
53) m,p-Xylene	9.143	106	4267	1.041	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed