
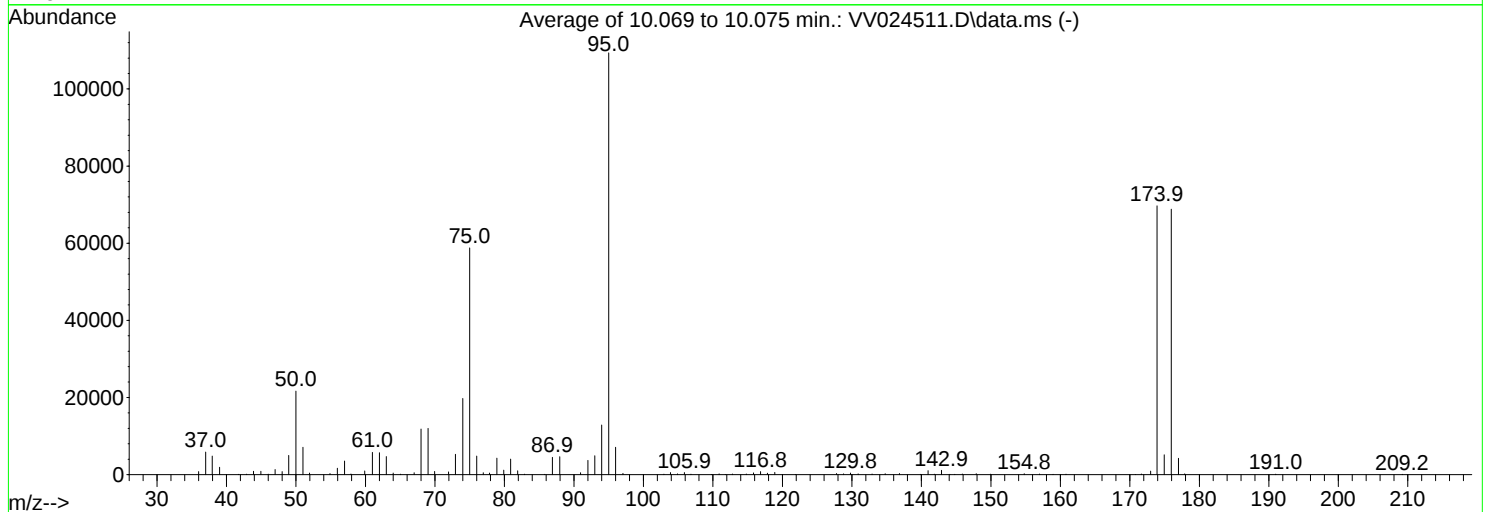


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020222\
 Data File : VV024511.D
 Acq On : 02 Feb 2022 09:05
 Operator : SY/MD
 Sample : BFB261
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB261

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Title : VOC Analysis
 Last Update : Sat Feb 05 00:18:38 2022

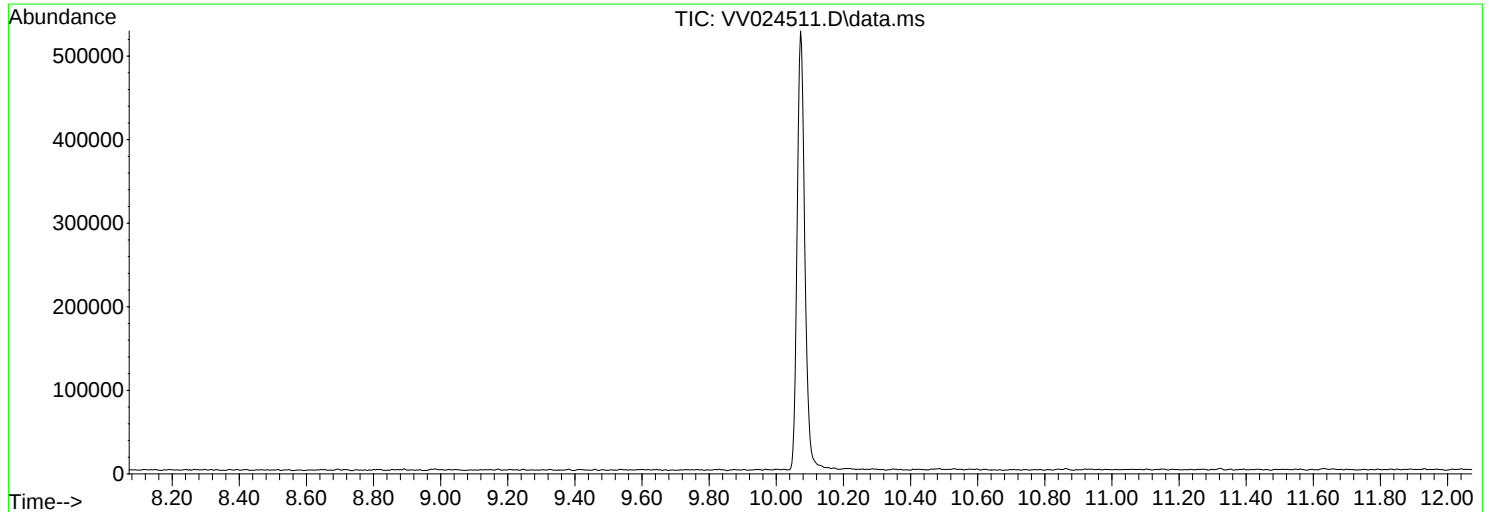

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	21661	PASS
75	95	30	80	53.8	58803	PASS
95	95	100	100	100.0	109360	PASS
96	95	5	9	6.5	7113	PASS
173	174	0.00	2	1.3	900	PASS
174	95	50	120	63.7	69685	PASS
175	174	5	9	7.4	5148	PASS
176	174	95	105	98.8	68824	PASS
177	176	5	10	6.2	4247	PASS

m/z	Abundance
36.10	118.0
37.80	135.0
38.70	144.0
39.20	102.0
39.90	325.0
41.00	338.0
41.70	107.0
42.20	147.0
43.00	258.0
43.90	842.0
44.90	128.0
54.10	123.0
54.90	224.0
55.90	135.0
60.00	110.0
69.10	143.0
72.90	112.0
74.10	111.0
77.00	103.0
96.10	273.0
207.00	822.0
208.00	184.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261

m/z	Abundance
36.00	861.0
37.00	5903.0
38.00	5129.0
39.00	1997.0
39.90	230.0
41.00	228.0
41.90	167.0
42.80	386.0
44.00	1634.0
45.00	924.0
45.90	122.0
47.00	1337.0
48.00	681.0
49.00	4960.0
50.00	21360.0
51.00	7133.0
52.00	466.0
54.90	486.0
56.00	1777.0
57.00	3655.0
57.90	152.0
59.90	1074.0
61.00	5721.0
62.00	5350.0
63.00	4678.0
64.00	433.0
65.10	126.0
67.00	527.0
68.00	11301.0
69.00	11685.0
70.00	870.0
72.00	706.0
73.00	5323.0
74.00	19456.0
75.00	57176.0
76.00	5028.0
77.00	586.0
77.80	358.0
78.90	4226.0
79.90	1185.0
80.90	3975.0
81.90	990.0
82.90	138.0
86.90	4315.0
88.00	4537.0
90.90	451.0
92.00	3654.0
93.00	4616.0
94.00	12340.0
95.00	106232.0
96.00	7240.0
97.00	322.0
103.00	126.0
103.90	511.0
104.90	217.0
105.90	540.0
106.80	119.0
110.90	171.0
112.80	174.0
114.80	189.0
115.80	464.0
116.90	812.0
117.80	333.0
118.90	509.0
127.80	245.0
128.80	202.0
129.80	365.0
130.90	211.0
132.90	122.0
134.80	214.0
136.90	308.0
141.00	909.0
141.90	138.0
142.90	1014.0
145.90	161.0
147.90	239.0
149.90	130.0
154.80	255.0
157.00	104.0
158.90	130.0
160.80	138.0
171.70	148.0
173.00	894.0
173.90	64384.0
174.90	4774.0
176.00	64896.0
177.00	4086.0
177.90	210.0
191.00	120.0
206.90	724.0
208.00	103.0
209.20	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261

m/z	Abundance
36.00	926.0
37.00	6020.0
38.00	5108.0
39.00	2092.0
39.90	304.0
41.00	209.0
41.80	179.0
42.80	417.0
44.00	1743.0
45.00	1016.0
46.00	103.0
47.00	1444.0
48.00	819.0
48.90	5221.0
50.00	22488.0
51.00	7384.0
51.90	440.0
55.00	510.0
56.00	1820.0
57.00	3634.0
57.90	160.0
59.90	1061.0
61.00	5966.0
62.00	5878.0
63.00	4924.0
64.00	407.0
65.10	123.0
67.00	520.0
68.00	12232.0
69.00	12588.0
69.90	858.0
72.00	725.0
73.00	5605.0
74.00	20408.0
75.00	60880.0
76.00	4965.0
77.00	636.0
77.90	427.0
78.90	4454.0
79.90	1178.0
80.90	4158.0
81.90	1066.0
82.90	161.0
85.80	104.0
86.90	4600.0
87.90	4860.0
90.90	489.0
92.00	3861.0
93.00	5058.0
94.00	13232.0
95.00	113112.0
96.00	7582.0
97.10	344.0
103.00	113.0
103.90	532.0
104.90	201.0
105.90	579.0
106.80	113.0
110.90	218.0
112.80	177.0
114.80	150.0
115.90	464.0
116.90	808.0
117.80	413.0
118.90	606.0
127.80	324.0
128.80	213.0
129.80	397.0
130.90	209.0
132.90	169.0
134.80	264.0
136.90	299.0
139.80	103.0
140.90	1083.0
141.80	147.0
142.90	1183.0
144.10	124.0
144.80	119.0
145.90	179.0
147.90	258.0
150.00	147.0
154.80	254.0
157.00	158.0
159.00	101.0
160.80	132.0
171.60	173.0
173.00	942.0
173.90	72032.0
175.00	5298.0
175.90	71240.0
177.00	4429.0
177.90	242.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261

191.00	116.0
207.00	704.0
209.20	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261

m/z	Abundance
36.00	949.0
37.00	5619.0
38.00	4673.0
39.00	1992.0
39.90	384.0
41.00	221.0
41.90	206.0
42.90	390.0
43.90	1735.0
45.00	1041.0
46.10	132.0
47.00	1239.0
48.00	890.0
49.00	4791.0
50.00	21136.0
51.00	6792.0
51.90	401.0
55.00	536.0
56.00	1790.0
57.00	3363.0
57.90	174.0
59.90	1067.0
61.00	5655.0
62.00	5829.0
63.00	4507.0
64.00	391.0
65.00	128.0
67.00	456.0
68.00	11878.0
69.00	12159.0
70.00	813.0
71.90	720.0
73.00	5271.0
74.00	19664.0
75.00	58352.0
76.00	4437.0
76.90	645.0
77.90	485.0
78.90	4153.0
79.90	1072.0
80.90	3986.0
81.90	982.0
82.90	129.0
85.80	127.0
86.90	4565.0
87.90	4587.0
91.00	511.0
92.00	3580.0
93.00	4976.0
94.00	12978.0
95.00	108736.0
96.00	7337.0
97.10	290.0
102.90	113.0
103.90	516.0
104.90	198.0
105.90	549.0
106.90	108.0
109.80	100.0
110.90	205.0
111.80	149.0
112.80	134.0
114.80	126.0
115.90	422.0
116.80	722.0
117.90	429.0
118.90	670.0
121.90	118.0
127.80	364.0
128.80	237.0
129.80	426.0
130.90	166.0
132.90	182.0
134.80	289.0
136.80	266.0
139.90	114.0
140.90	1120.0
141.80	130.0
142.90	1158.0
144.10	147.0
144.80	169.0
145.90	179.0
147.90	261.0
150.00	156.0
154.80	255.0
157.00	194.0
160.80	122.0
170.80	101.0
171.60	172.0
173.00	864.0
173.90	72640.0
175.00	5371.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261

175.90	70336.0
177.00	4225.0
177.90	218.0
191.00	120.0
207.00	754.0
208.00	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261