

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020322\
 Data File : VW024550.D
 Acq On : 03 Feb 2022 16:05
 Operator : SY/MD
 Sample : N1364-10ME
 Misc : 6.16g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Feb 04 03:40:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Feb 03 05:56:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	400654	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	362522	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	158410	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	129148	45.393	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.780%		
7) Chloroethane-d5	1.568	69	116285	46.893	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.780%		
11) 1,1-Dichloroethene-d2	2.105	63	211617	37.334	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.660%		
21) 2-Butanone-d5	3.905	46	183274	97.394	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	97.390%		
24) Chloroform-d	4.346	84	245010	46.890	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.780%		
26) 1,2-Dichloroethane-d4	5.031	65	163125	48.911	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.820%		
32) Benzene-d6	5.050	84	496413	48.159	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.320%		
36) 1,2-Dichloropropane-d6	6.069	67	162205	49.432	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.860%		
41) Toluene-d8	7.314	98	440836	46.470	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.940%		
43) trans-1,3-Dichloroprop...	7.619	79	79591	46.093	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.180%		
47) 2-Hexanone-d5	8.088	63	146231	104.923	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	104.920%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	194296	49.390	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.780%		
66) 1,2-Dichlorobenzene-d4	11.622	152	147534	49.225	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.460%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.986	75	5234	1.172	ug/L #	75
61) 1,2,3-Trichloropropane	11.246	75	22783	7.245	ug/L #	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024550.D
Acq On : 03 Feb 2022 16:05
Operator : SY/MD
Sample : N1364-10ME
Misc : 6.16g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Feb 04 03:40:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Feb 03 05:56:12 2022
Response via : Initial Calibration

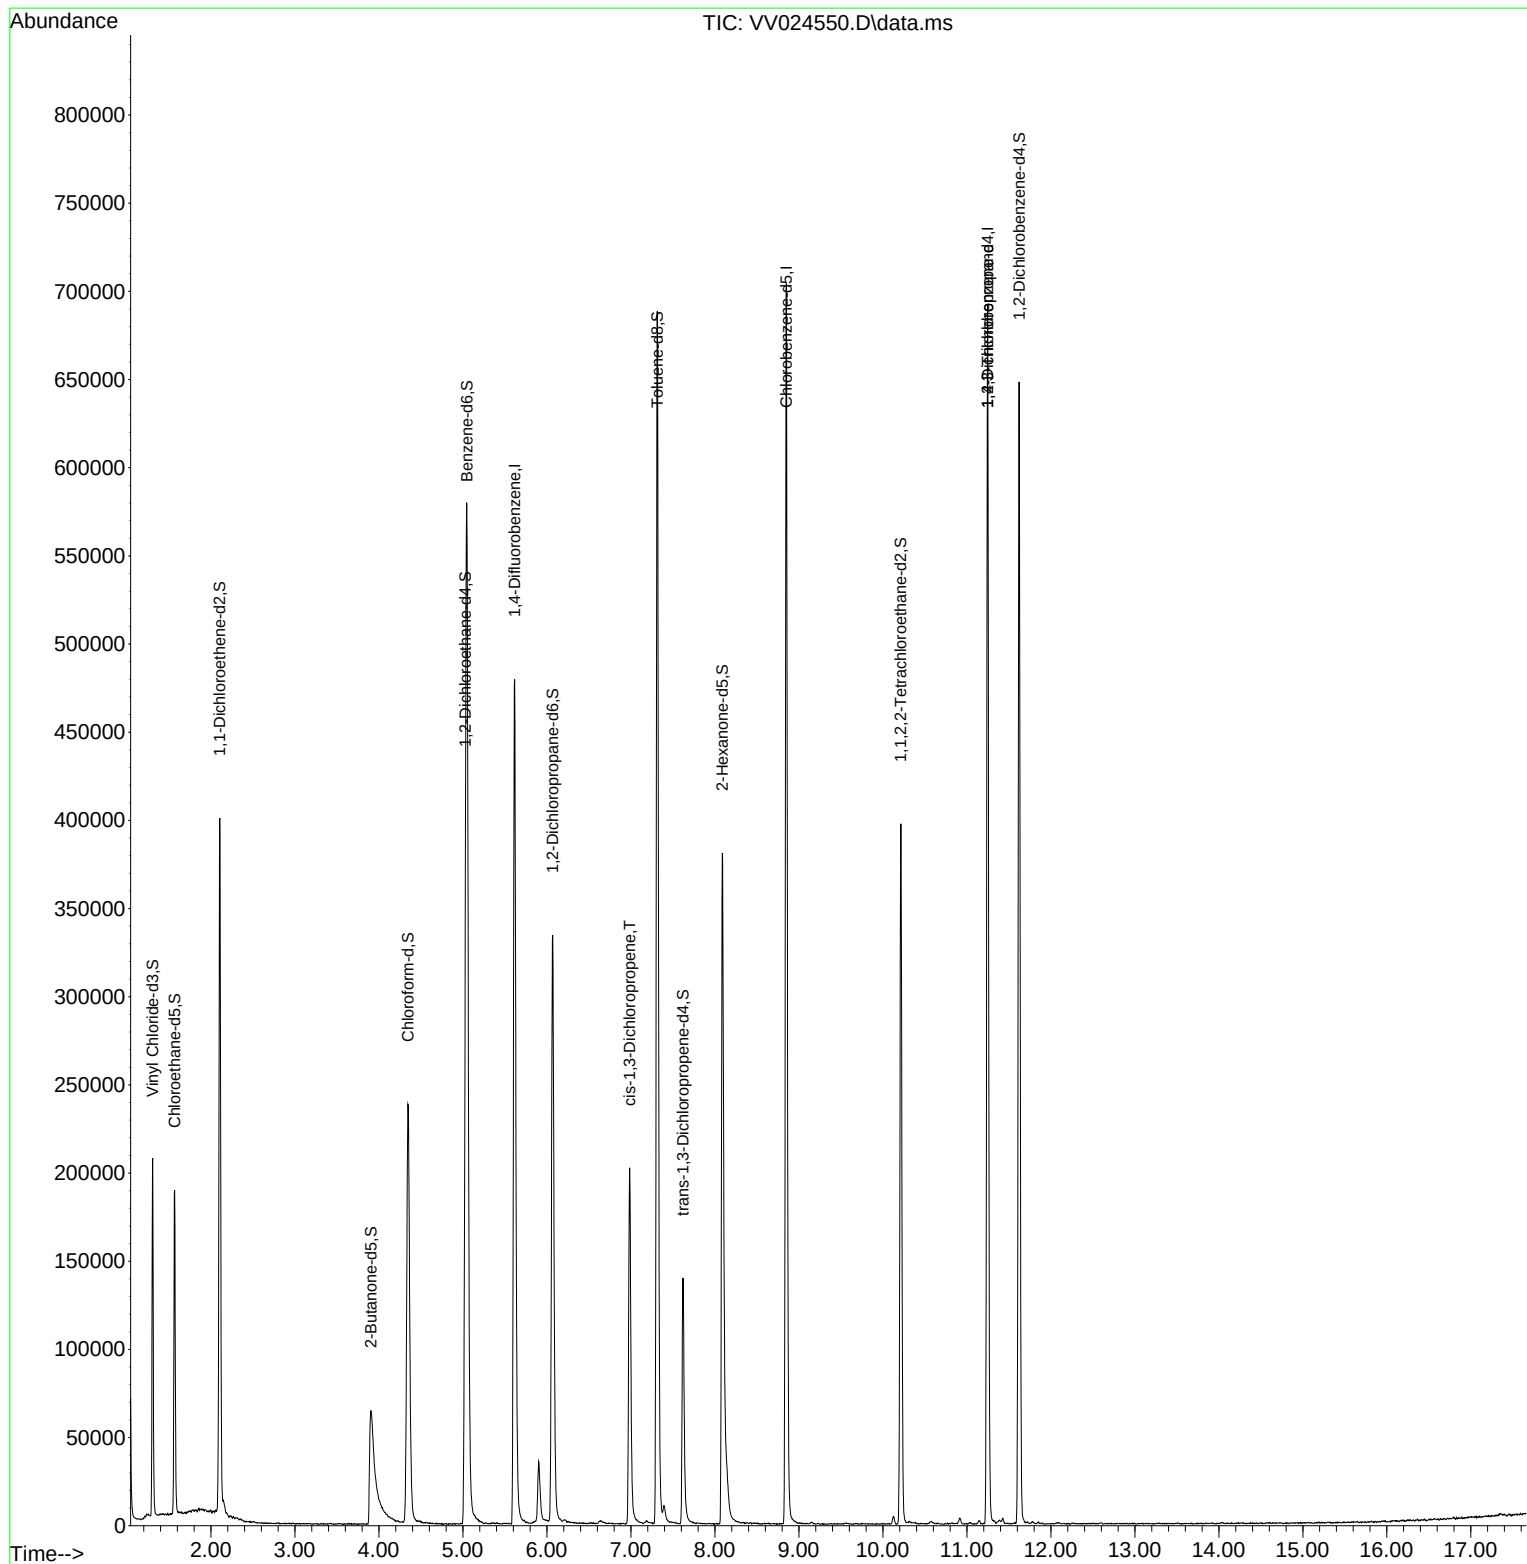

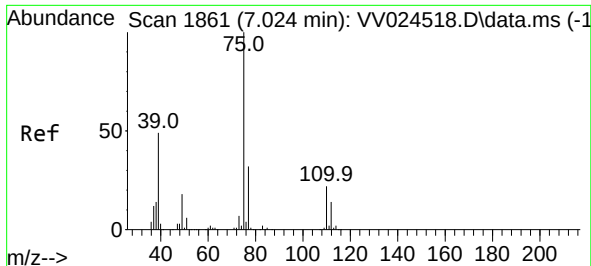

#39

cis-1,3-Dichloropropene

Concen: 1.172 ug/L

RT: 6.986 min Scan# 11

Delta R.T. -0.039 min

Lab File: VV024550.D

Acq: 03 Feb 2022 16:05

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 75 Resp: 5234

Ion Ratio Lower Upper

75 100

77 45.4 22.3 41.3#

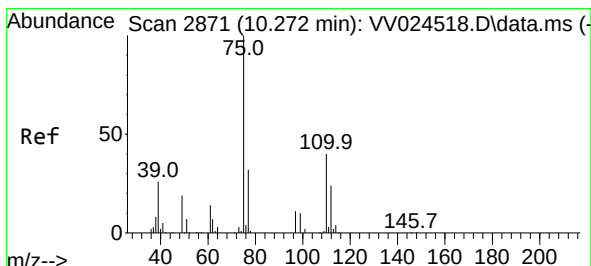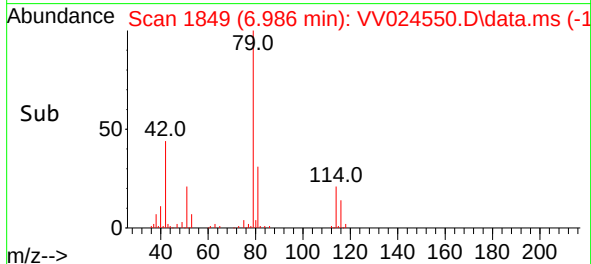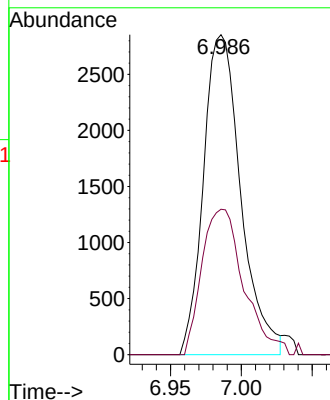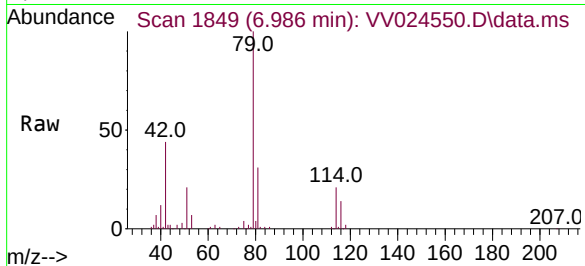

#61

1,2,3-Trichloropropane

Concen: 7.245 ug/L

RT: 11.246 min Scan# 3174

Delta R.T. 0.974 min

Lab File: VV024550.D

Acq: 03 Feb 2022 16:05

Tgt Ion: 75 Resp: 22783

Ion Ratio Lower Upper

75 100

77 33.1 25.8 38.8

110 2.6 30.9 46.3#

