

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
 Data File : VV024540.D
 Acq On : 03 Feb 2022 10:53
 Operator : SY/MD
 Sample : VV0203WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK310

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M

Title : VOC Analysis

Signal : TIC: VV024540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	179514	175042	13.82%	1.790%
2	1.568	157	164	176	rBV	162838	187865	14.83%	1.922%
3	2.108	323	332	364	rVB	320562	488085	38.53%	4.992%
4	2.863	565	567	569	rVB2	347	118	0.01%	0.001%
5	2.880	569	572	573	rBV3	440	282	0.02%	0.003%
6	2.928	584	587	589	rBV	363	283	0.02%	0.003%
7	2.992	605	607	608	rBV	291	129	0.01%	0.001%
8	3.018	612	615	618	rBV3	406	301	0.02%	0.003%
9	3.047	622	624	626	rBV3	364	224	0.02%	0.002%
10	3.101	639	641	642	rBV	272	94	0.01%	0.001%
11	3.146	652	655	657	rBV2	304	238	0.02%	0.002%
12	3.249	684	687	692	rVB2	523	376	0.03%	0.004%
13	3.275	692	695	696	rBV	381	231	0.02%	0.002%
14	3.323	708	710	714	rBV2	230	205	0.02%	0.002%
15	3.442	746	747	749	rBV	300	131	0.01%	0.001%
16	3.458	749	752	753	rVV	288	146	0.01%	0.001%
17	3.558	780	783	784	rBV2	271	134	0.01%	0.001%
18	3.590	788	793	794	rBV3	305	224	0.02%	0.002%
19	3.600	794	796	800	rVB3	410	237	0.02%	0.002%
20	3.619	800	802	803	rBV3	254	106	0.01%	0.001%
21	3.629	803	805	810	rBV3	519	438	0.03%	0.004%
22	3.738	836	839	841	rBV2	177	122	0.01%	0.001%
23	3.754	841	844	846	rBV3	335	202	0.02%	0.002%
24	3.767	846	848	849	rBV	281	89	0.01%	0.001%
25	3.889	874	886	934	rBV2	80031	274382	21.66%	2.806%
26	4.349	1014	1029	1056	rBV	201257	497215	39.25%	5.086%
27	4.654	1122	1124	1125	rVB2	279	71	0.01%	0.001%
28	4.667	1125	1128	1129	rBV2	260	145	0.01%	0.001%
29	4.706	1139	1140	1143	rVB	380	139	0.01%	0.001%
30	4.728	1143	1147	1149	rBV3	440	352	0.03%	0.004%
31	4.822	1172	1176	1178	rBV4	423	292	0.02%	0.003%
32	4.841	1178	1182	1184	rBV3	358	230	0.02%	0.002%
33	4.931	1207	1210	1213	rBV2	302	217	0.02%	0.002%
34	4.950	1213	1216	1219	rVB	416	280	0.02%	0.003%
35	4.969	1219	1222	1225	rBV4	710	485	0.04%	0.005%
36	5.047	1228	1246	1278	rBV2	490246	1266887	100.00%	12.958%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
 Data File : VV024540.D
 Acq On : 03 Feb 2022 10:53
 Operator : SY/MD
 Sample : VV0203WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK310

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Title : VOC Analysis

37	5.288	1319	1321	1325	rBV4	465	376	0.03%	0.004%
38	5.342	1336	1338	1339	rBV	413	198	0.02%	0.002%
39	5.397	1351	1355	1358	rBV5	530	546	0.04%	0.006%
40	5.442	1367	1369	1374	rVB2	500	381	0.03%	0.004%
41	5.471	1374	1378	1380	rBV4	616	505	0.04%	0.005%
42	5.616	1411	1423	1457	rBV	386430	777293	61.35%	7.950%
43	5.905	1502	1513	1531	rBV	28924	61586	4.86%	0.630%
44	6.069	1546	1564	1597	rBV	285613	587450	46.37%	6.009%
45	6.313	1634	1640	1646	rBV4	548	558	0.04%	0.006%
46	6.346	1646	1650	1652	rBV3	397	241	0.02%	0.002%
47	6.442	1677	1680	1684	rVB3	315	269	0.02%	0.003%
48	6.484	1690	1693	1695	rBV	368	200	0.02%	0.002%
49	6.754	1776	1777	1779	rVB	243	68	0.01%	0.001%
50	6.770	1779	1782	1785	rBV3	305	181	0.01%	0.002%
51	6.812	1793	1795	1797	rBV2	225	109	0.01%	0.001%
52	6.850	1805	1807	1809	rBV2	247	123	0.01%	0.001%
53	6.889	1816	1819	1827	rVB3	686	832	0.07%	0.009%
54	6.931	1827	1832	1835	rBV2	319	392	0.03%	0.004%
55	6.985	1835	1849	1879	rBV	174679	322994	25.50%	3.304%
56	7.313	1940	1951	1970	rBV	590208	1027186	81.08%	10.506%
57	7.622	2037	2047	2067	rBV	119474	206652	16.31%	2.114%
58	7.757	2087	2089	2093	rBV2	516	328	0.03%	0.003%
59	7.866	2120	2123	2127	rBV3	302	273	0.02%	0.003%
60	7.918	2137	2139	2140	rBV2	540	239	0.02%	0.002%
61	7.966	2152	2154	2155	rBV	364	170	0.01%	0.002%
62	7.995	2161	2163	2166	rBV2	184	89	0.01%	0.001%
63	8.024	2166	2172	2176	rVB5	622	494	0.04%	0.005%
64	8.047	2176	2179	2181	rBV	407	238	0.02%	0.002%
65	8.088	2181	2192	2229	rBV	339562	651385	51.42%	6.662%
66	8.564	2338	2340	2342	rBV	564	325	0.03%	0.003%
67	8.648	2365	2366	2368	rBV	209	103	0.01%	0.001%
68	8.690	2377	2379	2381	rBV3	402	188	0.01%	0.002%
69	8.809	2413	2416	2418	rBV3	431	280	0.02%	0.003%
70	8.850	2418	2429	2458	rBV	574703	931229	73.51%	9.525%
71	9.387	2589	2596	2598	rBV2	265	361	0.03%	0.004%
72	9.432	2607	2610	2613	rBV2	286	126	0.01%	0.001%
73	9.455	2613	2617	2619	rBV2	418	273	0.02%	0.003%
74	9.542	2639	2644	2647	rBV3	628	656	0.05%	0.007%
75	9.889	2750	2752	2757	rVB4	399	275	0.02%	0.003%
76	10.063	2804	2806	2808	rBV3	288	123	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
 Data File : VV024540.D
 Acq On : 03 Feb 2022 10:53
 Operator : SY/MD
 Sample : VV0203WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK310

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Title : VOC Analysis

77	10.127	2814	2826	2835	rBV2	4603	7543	0.60%	0.077%
78	10.214	2841	2853	2874	rBV	337807	535097	42.24%	5.473%
79	10.439	2919	2923	2924	rBV	287	185	0.01%	0.002%
80	10.468	2930	2932	2937	rBV4	417	303	0.02%	0.003%
81	10.490	2937	2939	2942	rVB3	377	185	0.01%	0.002%
82	10.542	2949	2955	2956	rBV3	581	504	0.04%	0.005%
83	10.828	3040	3044	3051	rVB3	803	825	0.07%	0.008%
84	10.857	3051	3053	3055	rBV3	370	156	0.01%	0.002%
85	10.918	3066	3072	3080	rVB3	3328	4855	0.38%	0.050%
86	10.998	3095	3097	3100	rVB2	314	175	0.01%	0.002%
87	11.024	3100	3105	3108	rBV4	1160	1305	0.10%	0.013%
88	11.114	3131	3133	3136	rBV2	422	288	0.02%	0.003%
89	11.188	3152	3156	3159	rBV4	941	734	0.06%	0.008%
90	11.246	3163	3174	3197	rBV	573147	870720	68.73%	8.906%
91	11.477	3240	3246	3248	rBV4	604	629	0.05%	0.006%
92	11.519	3257	3259	3262	rVB2	496	190	0.01%	0.002%
93	11.542	3263	3266	3269	rBV3	432	262	0.02%	0.003%
94	11.622	3279	3291	3312	rBV	558276	880306	69.49%	9.004%
95	11.882	3370	3372	3375	rBV2	358	196	0.02%	0.002%
96	12.342	3513	3515	3518	rBV2	315	178	0.01%	0.002%
97	12.480	3556	3558	3559	rBV2	313	121	0.01%	0.001%
98	12.583	3588	3590	3593	rBV	536	368	0.03%	0.004%
99	13.734	3946	3948	3949	rBV2	471	214	0.02%	0.002%
100	14.651	4231	4233	4235	rBV	679	312	0.02%	0.003%




Sum of corrected areas: 9776943

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024540.D
Acq On : 03 Feb 2022 10:53
Operator : SY/MD
Sample : VV0203WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

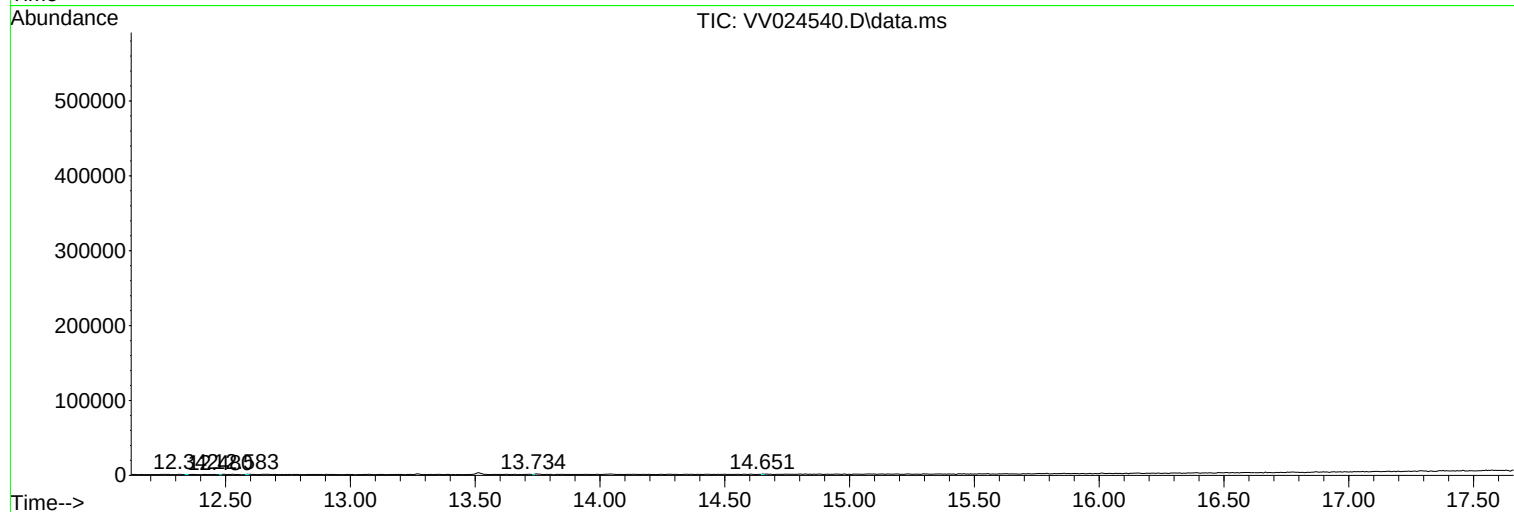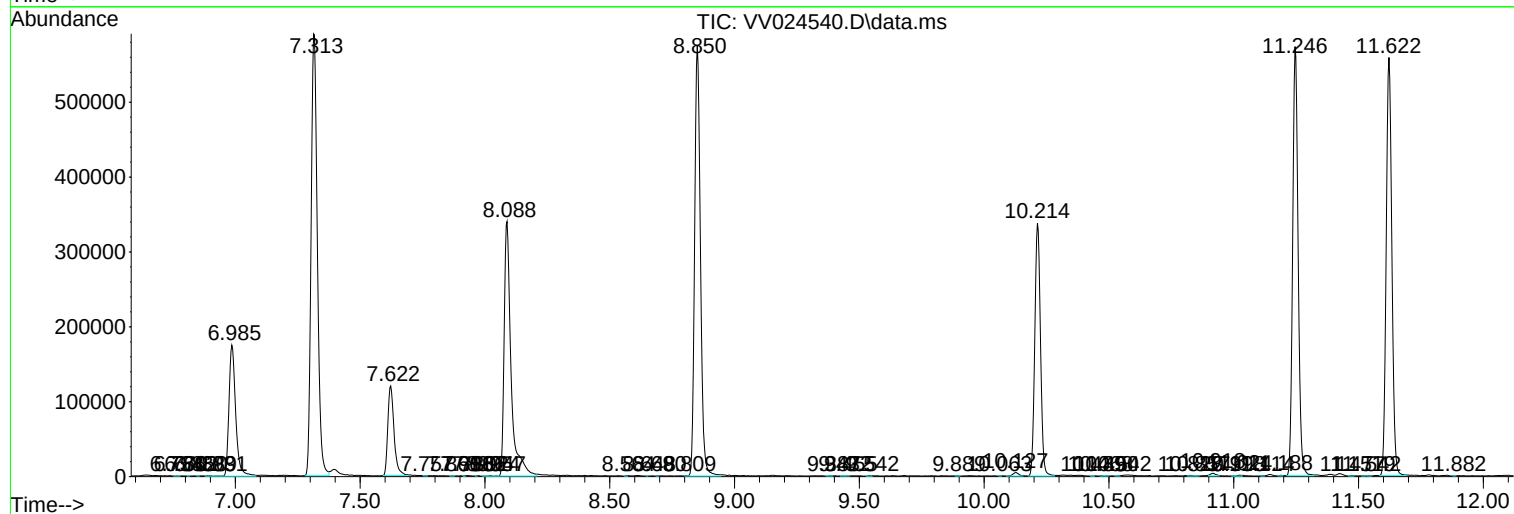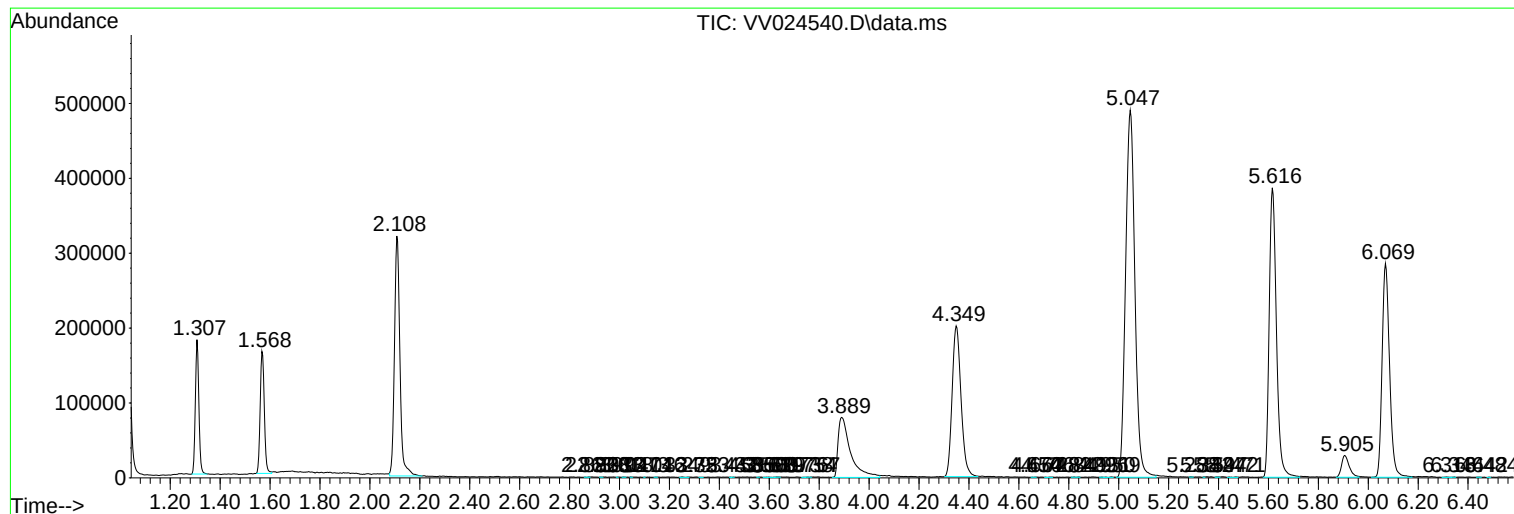

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024540.D
Acq On : 03 Feb 2022 10:53
Operator : SY/MD
Sample : VV0203WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024540.D
Acq On : 03 Feb 2022 10:53
Operator : SY/MD
Sample : VV0203WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc