

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
 Data File : VV024546.D
 Acq On : 03 Feb 2022 14:30
 Operator : SY/MD
 Sample : N1363-16ME
 Misc : 6.20g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGM02ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Title : VOC Analysis

Signal : TIC: VV024546.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	144466	168120	13.65%	1.711%
2	1.564	157	163	181	rVB	130766	176408	14.32%	1.795%
3	2.085	316	325	337	rBV	318623	448298	36.39%	4.561%
4	2.854	559	564	567	rBV3	709	614	0.05%	0.006%
5	3.040	620	622	625	rBV2	568	295	0.02%	0.003%
6	3.076	628	633	637	rBV4	551	500	0.04%	0.005%
7	3.172	656	663	665	rBV4	1636	1903	0.15%	0.019%
8	3.217	675	677	679	rBV3	399	182	0.01%	0.002%
9	3.381	723	728	731	rBV3	414	438	0.04%	0.004%
10	3.429	741	743	744	rBV3	151	69	0.01%	0.001%
11	3.436	744	745	748	rVV2	414	213	0.02%	0.002%
12	3.526	771	773	774	rBV	266	104	0.01%	0.001%
13	3.613	797	800	802	rBV4	353	249	0.02%	0.003%
14	3.651	810	812	813	rBV2	270	131	0.01%	0.001%
15	3.722	832	834	836	rVB2	207	79	0.01%	0.001%
16	3.735	836	838	840	rBV	161	89	0.01%	0.001%
17	3.799	854	858	863	rVB3	496	405	0.03%	0.004%
18	3.828	863	867	870	rBV	420	330	0.03%	0.003%
19	3.844	870	872	873	rBV2	353	125	0.01%	0.001%
20	3.892	877	887	928	rBV	56472	224503	18.22%	2.284%
21	4.336	1011	1025	1057	rVB	193675	489505	39.73%	4.981%
22	4.686	1133	1134	1135	rBV	275	59	0.00%	0.001%
23	4.706	1138	1140	1141	rBV	263	99	0.01%	0.001%
24	4.818	1173	1175	1178	rBV2	223	130	0.01%	0.001%
25	4.831	1178	1179	1180	rBV2	175	49	0.00%	0.000%
26	4.883	1193	1195	1198	rBV2	275	134	0.01%	0.001%
27	4.905	1199	1202	1204	rBV2	333	201	0.02%	0.002%
28	4.937	1207	1212	1217	rVB4	338	405	0.03%	0.004%
29	4.963	1218	1220	1223	rVB2	345	192	0.02%	0.002%
30	5.034	1223	1242	1271	rBV2	494677	1232070	100.00%	12.536%
31	5.252	1308	1310	1311	rBV	482	211	0.02%	0.002%
32	5.330	1325	1334	1349	rBV6	4422	12246	0.99%	0.125%
33	5.542	1398	1400	1402	rVB2	346	101	0.01%	0.001%
34	5.551	1402	1403	1404	rBV2	229	84	0.01%	0.001%
35	5.606	1408	1420	1442	rBV	406621	839228	68.12%	8.539%
36	6.063	1550	1562	1589	rVB	272574	572915	46.50%	5.829%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020322\
 Data File : VW024546.D
 Acq On : 03 Feb 2022 14:30
 Operator : SY/MD
 Sample : N1363-16ME
 Misc : 6.20g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGM02ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Title : VOC Analysis

37	6.982	1837	1848	1880	rBV	160334	316597	25.70%	3.221%
38	7.310	1938	1950	1969	rBV	567215	1016690	82.52%	10.345%
39	7.619	2036	2046	2077	rBV	102525	212007	17.21%	2.157%
40	7.973	2147	2156	2170	rVB	34151	57561	4.67%	0.586%
41	8.050	2179	2180	2181	rBV	265	92	0.01%	0.001%
42	8.120	2183	2202	2241	rVV	167085	609028	49.43%	6.197%
43	8.378	2279	2282	2287	rBV4	713	675	0.05%	0.007%
44	8.526	2323	2328	2332	rBV3	532	604	0.05%	0.006%
45	8.638	2360	2363	2365	rBV2	480	333	0.03%	0.003%
46	8.680	2373	2376	2379	rBV3	389	219	0.02%	0.002%
47	8.747	2395	2397	2398	rBV3	297	149	0.01%	0.002%
48	8.792	2409	2411	2416	rBV4	243	135	0.01%	0.001%
49	8.850	2418	2429	2456	rBV	549128	1038318	84.27%	10.565%
50	9.127	2513	2515	2516	rBV2	498	182	0.01%	0.002%
51	9.136	2516	2518	2521	rBV2	437	317	0.03%	0.003%
52	9.217	2540	2543	2544	rBV	307	173	0.01%	0.002%
53	9.355	2584	2586	2587	rBV	236	83	0.01%	0.001%
54	9.384	2591	2595	2598	rBV2	444	486	0.04%	0.005%
55	9.432	2608	2610	2612	rVB	275	112	0.01%	0.001%
56	9.445	2612	2614	2617	rBV4	205	68	0.01%	0.001%
57	9.461	2617	2619	2621	rVB	267	123	0.01%	0.001%
58	9.574	2652	2654	2658	rVB4	308	135	0.01%	0.001%
59	9.950	2769	2771	2772	rBV	372	144	0.01%	0.001%
60	9.989	2781	2783	2785	rBV2	355	219	0.02%	0.002%
61	10.030	2793	2796	2798	rBV3	289	181	0.01%	0.002%
62	10.066	2805	2807	2808	rBV3	247	130	0.01%	0.001%
63	10.127	2817	2826	2835	rBV4	4075	6907	0.56%	0.070%
64	10.220	2843	2855	2879	rBV	290803	518270	42.06%	5.273%
65	10.429	2917	2920	2921	rBV3	345	163	0.01%	0.002%
66	10.751	3015	3020	3022	rBV4	511	483	0.04%	0.005%
67	10.918	3065	3072	3084	rVB9	3523	6287	0.51%	0.064%
68	11.030	3099	3107	3115	rVB5	1104	1827	0.15%	0.019%
69	11.066	3115	3118	3119	rBV2	306	154	0.01%	0.002%
70	11.143	3136	3142	3153	rVB4	2376	3351	0.27%	0.034%
71	11.249	3163	3175	3196	rBV	647286	979822	79.53%	9.969%
72	11.625	3280	3292	3308	rBV	553978	881816	71.57%	8.972%
73	11.818	3350	3352	3355	rBV2	536	307	0.02%	0.003%
74	12.033	3417	3419	3420	rBV	304	127	0.01%	0.001%
75	12.342	3511	3515	3516	rBV3	810	533	0.04%	0.005%
76	12.397	3530	3532	3537	rBV3	338	332	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
 Data File : VV024546.D
 Acq On : 03 Feb 2022 14:30
 Operator : SY/MD
 Sample : N1363-16ME
 Misc : 6.20g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGM02ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M

Title : VOC Analysis

77	12.445	3544	3547	3552	rBV4	643	623	0.05%	0.006%
78	12.519	3568	3570	3573	rBV	395	229	0.02%	0.002%
79	12.561	3581	3583	3586	rBV	514	373	0.03%	0.004%
80	13.258	3797	3800	3801	rBV2	339	197	0.02%	0.002%
81	13.863	3985	3988	3990	rBV2	406	266	0.02%	0.003%
82	14.699	4247	4248	4252	rVB3	514	283	0.02%	0.003%
83	15.246	4416	4418	4422	rBV	588	474	0.04%	0.005%




Sum of corrected areas: 9828269

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024546.D
Acq On : 03 Feb 2022 14:30
Operator : SY/MD
Sample : N1363-16ME
Misc : 6.20g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGM02ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

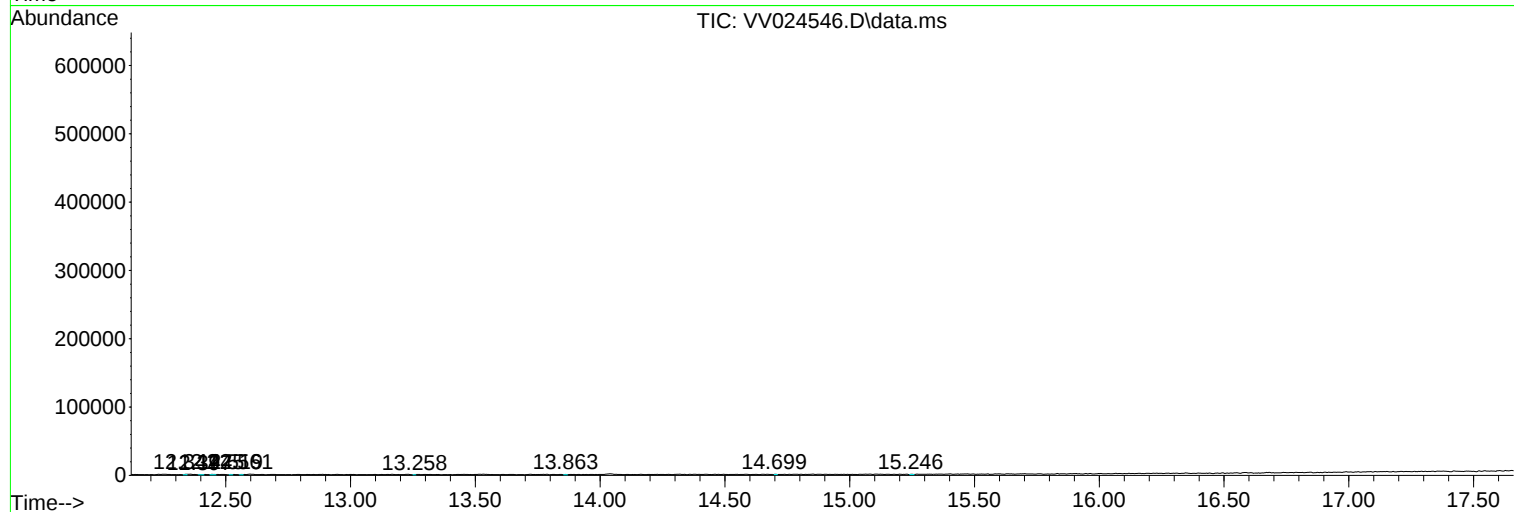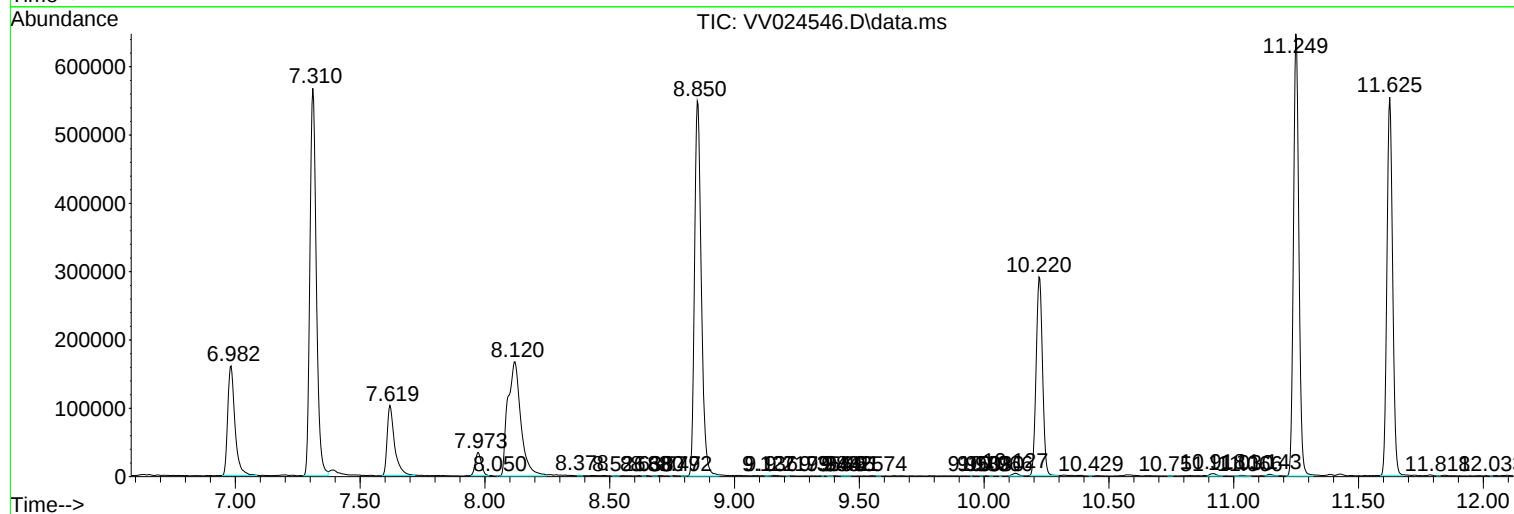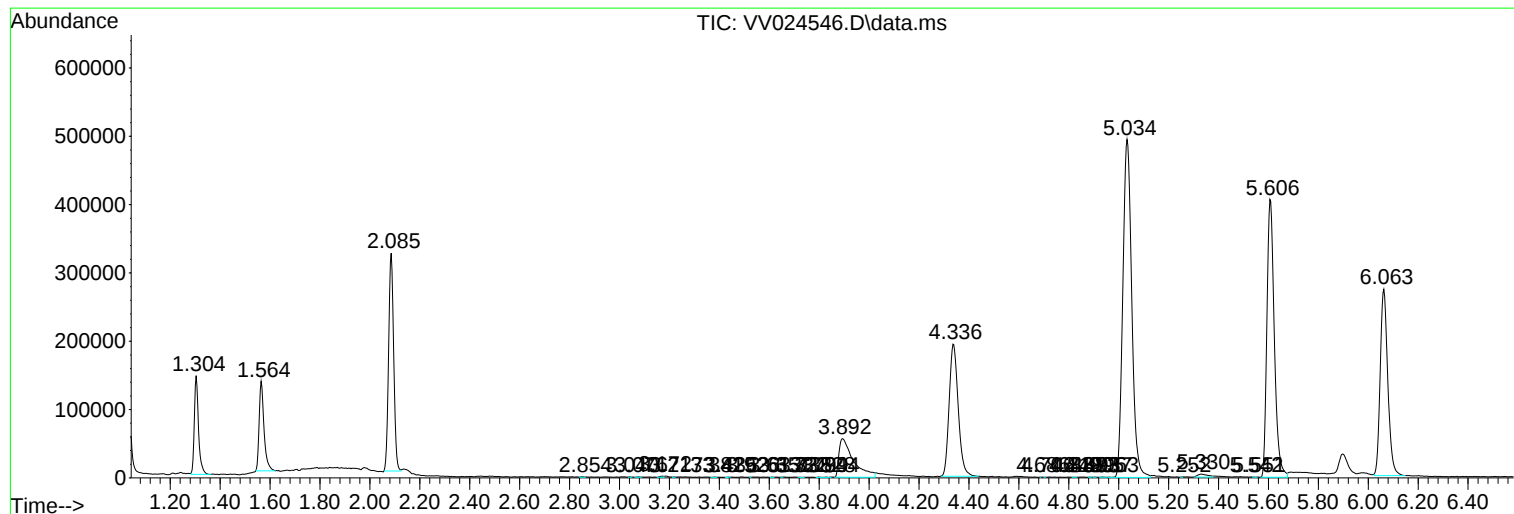

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024546.D
Acq On : 03 Feb 2022 14:30
Operator : SY/MD
Sample : N1363-16ME
Misc : 6.20g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGM02ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024546.D
Acq On : 03 Feb 2022 14:30
Operator : SY/MD
Sample : N1363-16ME
Misc : 6.20g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGM02ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc