

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
 Data File : VV024547.D
 Acq On : 03 Feb 2022 14:54
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Title : VOC Analysis

Signal : TIC: VV024547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rVB	171022	211342	13.96%	1.764%
2	1.564	156	163	182	rBV	130949	198534	13.11%	1.658%
3	2.092	319	327	338	rVB	263378	351272	23.20%	2.933%
4	3.310	704	706	710	rBV	313	199	0.01%	0.002%
5	3.371	722	725	733	rVB5	614	672	0.04%	0.006%
6	3.452	746	750	752	rBV4	224	139	0.01%	0.001%
7	3.471	754	756	758	rBV	335	152	0.01%	0.001%
8	3.513	768	769	770	rBV	277	90	0.01%	0.001%
9	3.555	780	782	784	rBV3	326	207	0.01%	0.002%
10	3.571	784	787	788	rBV3	355	212	0.01%	0.002%
11	3.606	795	798	801	rBV	179	133	0.01%	0.001%
12	3.648	807	811	813	rVB3	380	230	0.02%	0.002%
13	3.664	813	816	817	rBV2	197	98	0.01%	0.001%
14	3.719	825	833	834	rBV3	411	403	0.03%	0.003%
15	3.757	842	845	847	rBV4	537	417	0.03%	0.003%
16	3.818	862	864	865	rBV	243	121	0.01%	0.001%
17	3.921	883	896	928	rBV2	42488	235419	15.55%	1.965%
18	4.342	1013	1027	1056	rVB	227300	592939	39.16%	4.950%
19	5.040	1226	1244	1274	rBV2	606008	1514077	100.00%	12.641%
20	5.609	1409	1421	1457	rBV	502105	1072184	70.81%	8.951%
21	6.066	1551	1563	1592	rVB	326954	692139	45.71%	5.778%
22	6.985	1838	1849	1881	rBV	190961	388506	25.66%	3.244%
23	7.236	1918	1927	1934	rBV2	48913	98194	6.49%	0.820%
24	7.313	1943	1951	1971	rVB	688804	1241223	81.98%	10.363%
25	7.622	2037	2047	2080	rVB	120367	260740	17.22%	2.177%
26	7.969	2151	2155	2157	rBV3	605	438	0.03%	0.004%
27	8.050	2177	2180	2181	rBV2	417	222	0.01%	0.002%
28	8.127	2185	2204	2248	rBV	197656	772141	51.00%	6.446%
29	8.509	2320	2323	2327	rBV4	537	409	0.03%	0.003%
30	8.532	2329	2330	2335	rVB3	673	339	0.02%	0.003%
31	8.606	2351	2353	2354	rBV3	434	159	0.01%	0.001%
32	8.683	2373	2377	2382	rBV6	423	419	0.03%	0.003%
33	8.792	2408	2411	2415	rBV2	355	234	0.02%	0.002%
34	8.853	2418	2430	2456	rBV	667132	1306984	86.32%	10.912%
35	9.017	2476	2481	2483	rBV4	1293	1343	0.09%	0.011%
36	9.146	2516	2521	2537	rVB2	7627	13413	0.89%	0.112%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020322\
 Data File : VW024547.D
 Acq On : 03 Feb 2022 14:54
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Title : VOC Analysis

37	9.361	2586	2588	2594	rVB3	591	481	0.03%	0.004%
38	9.394	2594	2598	2602	rBV4	562	428	0.03%	0.004%
39	9.432	2608	2610	2612	rBV2	281	194	0.01%	0.002%
40	9.471	2619	2622	2623	rBV2	512	235	0.02%	0.002%
41	9.503	2630	2632	2635	rVB3	444	261	0.02%	0.002%
42	9.519	2635	2637	2639	rBV	315	113	0.01%	0.001%
43	9.551	2639	2647	2659	rBV8	2628	4940	0.33%	0.041%
44	9.667	2680	2683	2684	rBV2	342	230	0.02%	0.002%
45	9.722	2692	2700	2719	rBV	20407	37829	2.50%	0.316%
46	9.976	2776	2779	2783	rBV3	551	457	0.03%	0.004%
47	10.127	2818	2826	2836	rVB4	4989	8072	0.53%	0.067%
48	10.165	2836	2838	2841	rBV3	505	232	0.02%	0.002%
49	10.223	2843	2856	2878	rBV	369928	647175	42.74%	5.403%
50	10.423	2914	2918	2921	rVB4	521	427	0.03%	0.004%
51	10.458	2922	2929	2933	rBV3	1204	1346	0.09%	0.011%
52	10.545	2952	2956	2958	rBV3	855	790	0.05%	0.007%
53	10.715	3007	3009	3014	rBV5	434	344	0.02%	0.003%
54	10.741	3014	3017	3019	rBV2	450	321	0.02%	0.003%
55	10.757	3019	3022	3027	rVV5	472	463	0.03%	0.004%
56	10.799	3032	3035	3037	rBV2	416	309	0.02%	0.003%
57	10.869	3050	3057	3058	rBV6	900	780	0.05%	0.007%
58	10.995	3095	3096	3099	rVB2	345	179	0.01%	0.001%
59	11.008	3099	3100	3102	rVB	230	89	0.01%	0.001%
60	11.043	3102	3111	3115	rBV5	1323	2193	0.14%	0.018%
61	11.095	3123	3127	3132	rBV4	507	518	0.03%	0.004%
62	11.114	3132	3133	3134	rBV4	216	63	0.00%	0.001%
63	11.149	3134	3144	3152	rBV7	2304	4020	0.27%	0.034%
64	11.252	3164	3176	3197	rBV	792747	1222812	80.76%	10.209%
65	11.522	3257	3260	3261	rBV	322	188	0.01%	0.002%
66	11.625	3280	3292	3314	rBV	692577	1074761	70.98%	8.973%
67	11.757	3331	3333	3334	rBV	699	238	0.02%	0.002%
68	11.966	3394	3398	3399	rBV	502	295	0.02%	0.002%
69	12.075	3431	3432	3435	rBV2	475	330	0.02%	0.003%
70	12.204	3470	3472	3473	rBV2	355	160	0.01%	0.001%
71	12.252	3479	3487	3490	rBV4	1248	1558	0.10%	0.013%
72	12.284	3495	3497	3498	rBV	322	109	0.01%	0.001%
73	12.352	3514	3518	3521	rBV3	659	575	0.04%	0.005%
74	12.467	3551	3554	3557	rBV2	667	506	0.03%	0.004%
75	12.738	3634	3638	3642	rBV2	553	428	0.03%	0.004%
76	12.779	3645	3651	3653	rBV4	528	512	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
 Data File : VV024547.D
 Acq On : 03 Feb 2022 14:54
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Title : VOC Analysis

77	12.824	3662	3665	3667	rBV3	377	255	0.02%	0.002%
78	12.956	3701	3706	3708	rBV3	449	396	0.03%	0.003%
79	13.053	3732	3736	3739	rBV3	533	440	0.03%	0.004%
80	13.075	3742	3743	3747	rBV	242	147	0.01%	0.001%
81	13.107	3751	3753	3754	rBV	220	107	0.01%	0.001%
82	13.442	3853	3857	3859	rBV2	336	223	0.01%	0.002%
83	13.503	3872	3876	3878	rBV3	752	466	0.03%	0.004%
84	13.580	3893	3900	3902	rBV3	444	488	0.03%	0.004%
85	13.660	3923	3925	3926	rBV	461	115	0.01%	0.001%
86	13.811	3970	3972	3974	rBV2	265	148	0.01%	0.001%
87	14.046	4034	4045	4050	rBV5	1632	2942	0.19%	0.025%
88	14.191	4089	4090	4093	rBV3	319	213	0.01%	0.002%
89	14.262	4109	4112	4117	rBV2	501	478	0.03%	0.004%
90	14.397	4151	4154	4155	rBV	624	351	0.02%	0.003%
91	14.631	4225	4227	4233	rBV3	362	401	0.03%	0.003%


Sum of corrected areas: 11977874

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024547.D
Acq On : 03 Feb 2022 14:54
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

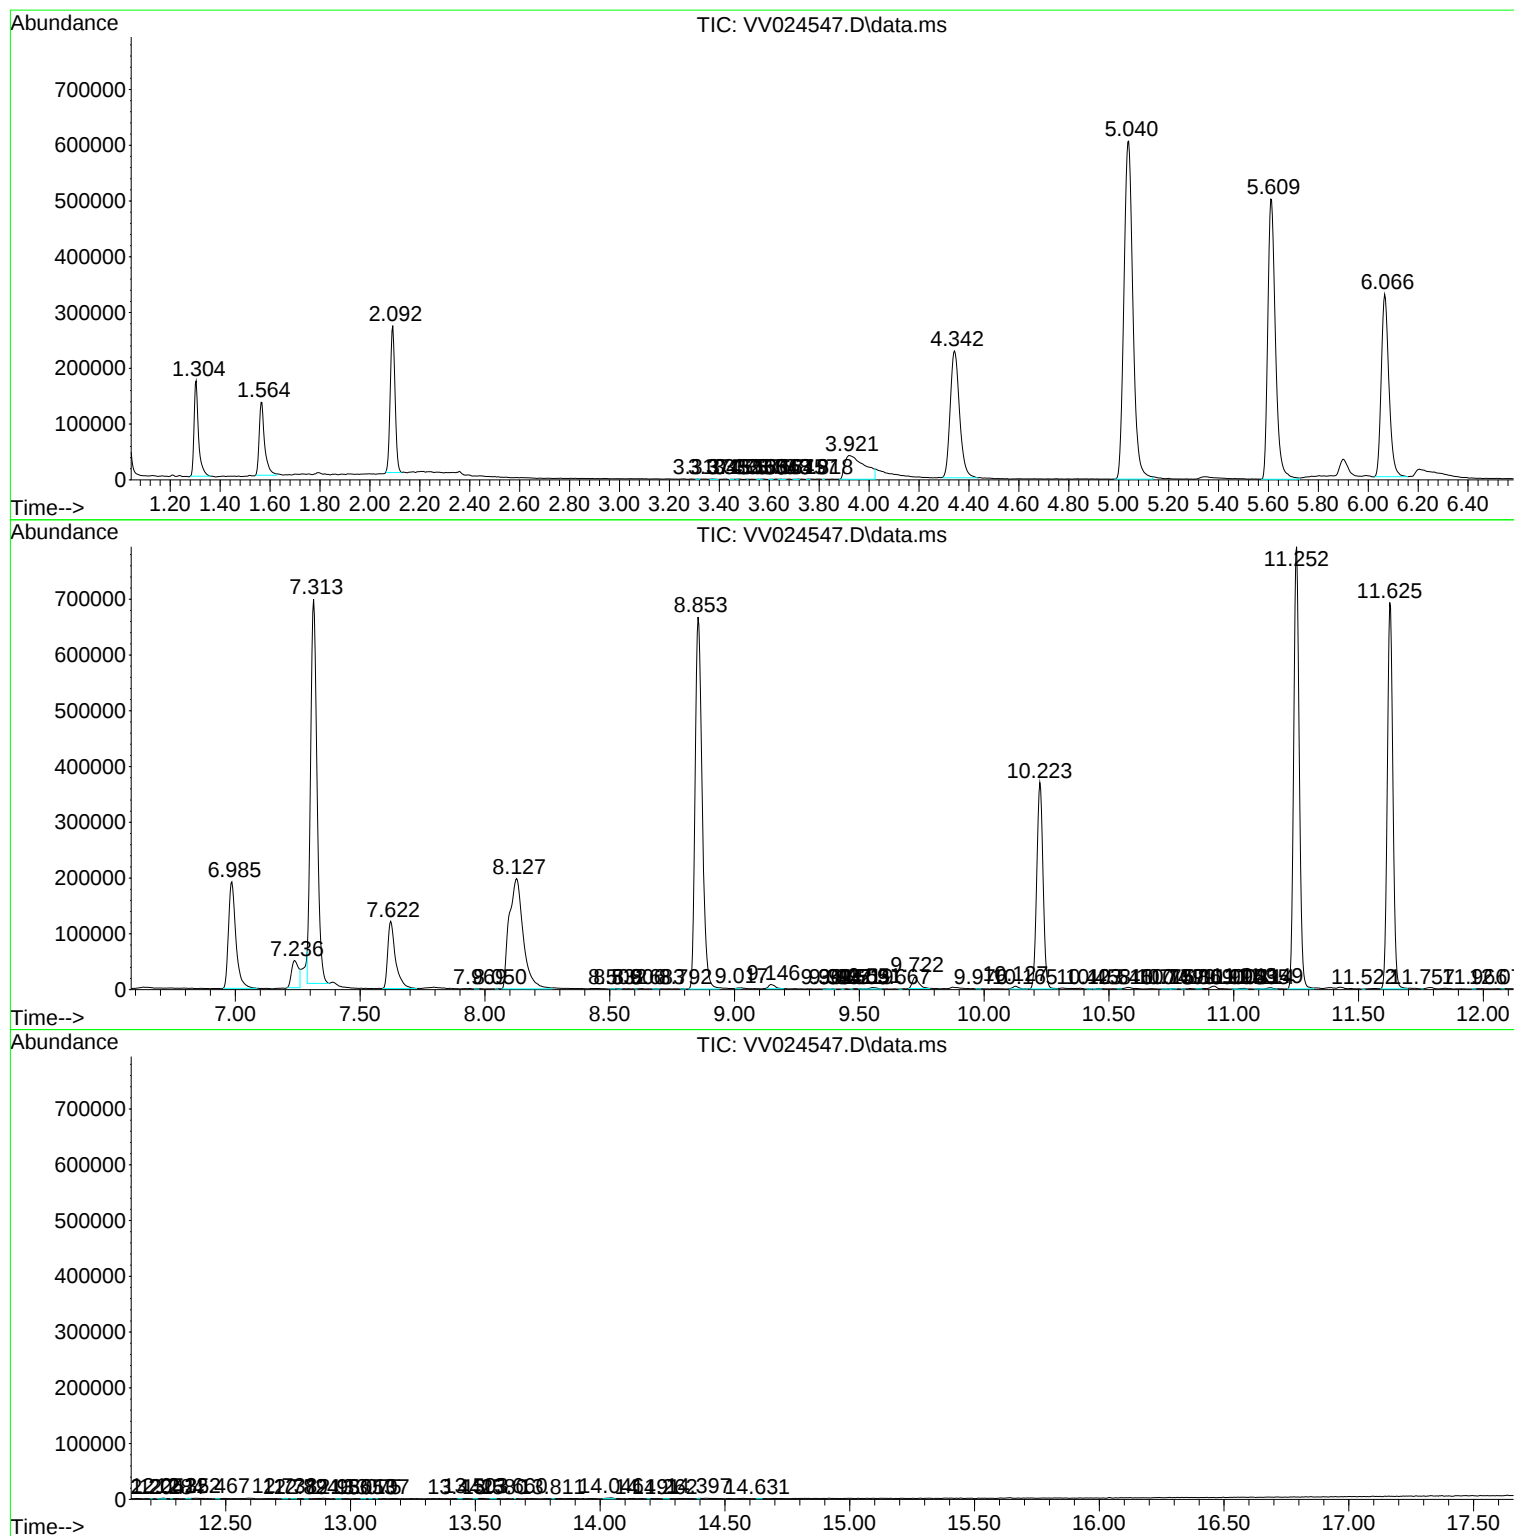

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024547.D
Acq On : 03 Feb 2022 14:54
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024547.D
Acq On : 03 Feb 2022 14:54
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc