

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
 Data File : VV024548.D
 Acq On : 03 Feb 2022 15:17
 Operator : SY/MD
 Sample : N1352-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Title : VOC Analysis

Signal : TIC: VV024548.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	170862	170675	14.27%	1.856%
2	1.568	157	164	176	rBV	149358	165171	13.81%	1.796%
3	2.108	323	332	346	rBV	307872	439576	36.75%	4.779%
4	2.558	469	472	474	rBV3	671	484	0.04%	0.005%
5	2.844	559	561	564	rBV2	574	310	0.03%	0.003%
6	2.870	564	569	574	rBV5	637	662	0.06%	0.007%
7	2.905	575	580	584	rVV5	414	462	0.04%	0.005%
8	3.130	647	650	651	rBV	261	117	0.01%	0.001%
9	3.243	682	685	686	rBV3	165	93	0.01%	0.001%
10	3.307	703	705	708	rVB3	477	167	0.01%	0.002%
11	3.397	729	733	736	rBV3	560	512	0.04%	0.006%
12	3.474	755	757	760	rBV2	285	193	0.02%	0.002%
13	3.545	776	779	784	rVB5	689	643	0.05%	0.007%
14	3.574	786	788	791	rBV2	295	228	0.02%	0.002%
15	3.587	791	792	794	rBV	207	95	0.01%	0.001%
16	3.629	803	805	807	rVB2	209	79	0.01%	0.001%
17	3.728	834	836	842	rVB3	477	346	0.03%	0.004%
18	3.754	842	844	846	rBV2	385	218	0.02%	0.002%
19	3.776	849	851	853	rBV2	276	156	0.01%	0.002%
20	3.831	866	868	870	rBV2	304	166	0.01%	0.002%
21	3.867	877	879	881	rVB3	303	145	0.01%	0.002%
22	3.905	881	891	929	rBV2	46858	210018	17.56%	2.283%
23	4.349	1014	1029	1053	rBV	186943	467115	39.05%	5.079%
24	4.657	1122	1125	1127	rBV2	438	260	0.02%	0.003%
25	4.754	1153	1155	1157	rBV	340	156	0.01%	0.002%
26	4.767	1157	1159	1169	rVB4	513	572	0.05%	0.006%
27	4.879	1191	1194	1196	rBV2	363	190	0.02%	0.002%
28	4.892	1196	1198	1201	rVB2	440	241	0.02%	0.003%
29	4.918	1201	1206	1208	rBV2	439	284	0.02%	0.003%
30	4.934	1208	1211	1212	rBV2	453	256	0.02%	0.003%
31	4.973	1216	1223	1225	rBV2	329	279	0.02%	0.003%
32	4.985	1225	1227	1228	rBV2	184	54	0.00%	0.001%
33	5.047	1228	1246	1294	rBV2	463614	1196094	100.00%	13.005%
34	5.493	1381	1385	1390	rBV4	639	764	0.06%	0.008%
35	5.538	1396	1399	1400	rBV	358	162	0.01%	0.002%
36	5.548	1400	1402	1404	rVB	424	212	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
 Data File : VV024548.D
 Acq On : 03 Feb 2022 15:17
 Operator : SY/MD
 Sample : N1352-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Title : VOC Analysis

37	5.616	1411	1423	1451	rBV	395696	795576	66.51%	8.650%
38	6.069	1552	1564	1595	rVB	267488	545129	45.58%	5.927%
39	6.509	1697	1701	1706	rBV3	944	1228	0.10%	0.013%
40	6.902	1822	1823	1826	rVB	357	163	0.01%	0.002%
41	6.918	1826	1828	1830	rBV	406	193	0.02%	0.002%
42	6.985	1839	1849	1871	rBV	161883	293429	24.53%	3.190%
43	7.313	1940	1951	1970	rBV	544755	957871	80.08%	10.415%
44	7.622	2037	2047	2070	rBV	108173	190977	15.97%	2.076%
45	7.844	2113	2116	2121	rVB3	739	625	0.05%	0.007%
46	8.091	2182	2193	2232	rBV	286015	601436	50.28%	6.539%
47	8.480	2311	2314	2317	rVB3	434	231	0.02%	0.003%
48	8.548	2332	2335	2337	rBV2	425	294	0.02%	0.003%
49	8.590	2347	2348	2350	rBV	343	142	0.01%	0.002%
50	8.619	2354	2357	2360	rBV4	528	433	0.04%	0.005%
51	8.757	2398	2400	2404	rVB2	334	148	0.01%	0.002%
52	8.850	2418	2429	2448	rBV	589780	940437	78.63%	10.225%
53	9.005	2475	2477	2478	rBV2	447	186	0.02%	0.002%
54	9.210	2539	2541	2546	rVB4	381	211	0.02%	0.002%
55	9.246	2549	2552	2556	rBV3	532	466	0.04%	0.005%
56	9.384	2591	2595	2597	rBV3	408	301	0.03%	0.003%
57	9.435	2610	2611	2613	rBV2	245	93	0.01%	0.001%
58	9.455	2613	2617	2618	rBV2	361	264	0.02%	0.003%
59	9.731	2700	2703	2704	rBV2	230	120	0.01%	0.001%
60	9.747	2705	2708	2709	rVV	327	180	0.02%	0.002%
61	9.857	2740	2742	2744	rBV3	349	188	0.02%	0.002%
62	9.934	2763	2766	2769	rBV3	542	406	0.03%	0.004%
63	10.069	2806	2808	2809	rVB	233	62	0.01%	0.001%
64	10.127	2818	2826	2834	rVB3	3593	5683	0.48%	0.062%
65	10.165	2834	2838	2839	rBV3	203	130	0.01%	0.001%
66	10.214	2842	2853	2873	rVV	316413	496057	41.47%	5.394%
67	10.468	2927	2932	2934	rBV3	553	577	0.05%	0.006%
68	10.525	2946	2950	2951	rBV2	541	318	0.03%	0.003%
69	10.580	2960	2967	2974	rBV5	1441	2317	0.19%	0.025%
70	10.760	3019	3023	3025	rBV2	404	317	0.03%	0.003%
71	10.805	3035	3037	3041	rBV4	503	314	0.03%	0.003%
72	10.914	3064	3071	3078	rBV5	2788	4391	0.37%	0.048%
73	11.024	3098	3105	3106	rBV2	776	634	0.05%	0.007%
74	11.143	3136	3142	3151	rBV4	1681	2370	0.20%	0.026%
75	11.246	3163	3174	3194	rBV	565109	871885	72.89%	9.480%
76	11.467	3238	3243	3244	rBV	625	420	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
 Data File : VV024548.D
 Acq On : 03 Feb 2022 15:17
 Operator : SY/MD
 Sample : N1352-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M

Title : VOC Analysis

77	11.622	3279	3291	3315	rBV	525506	821030	68.64%	8.927%
78	11.834	3353	3357	3359	rBV2	564	526	0.04%	0.006%
79	11.966	3396	3398	3401	rBV2	402	200	0.02%	0.002%
80	12.358	3518	3520	3522	rBV2	380	179	0.01%	0.002%
81	12.577	3585	3588	3589	rBV2	436	225	0.02%	0.002%
82	13.101	3749	3751	3753	rBV3	359	163	0.01%	0.002%
83	13.136	3758	3762	3766	rBV3	341	371	0.03%	0.004%
84	13.178	3771	3775	3778	rBV3	505	420	0.04%	0.005%
85	13.249	3795	3797	3800	rBV2	392	247	0.02%	0.003%
86	14.384	4146	4150	4152	rBV3	758	561	0.05%	0.006%




Sum of corrected areas: 9197279

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024548.D
Acq On : 03 Feb 2022 15:17
Operator : SY/MD
Sample : N1352-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

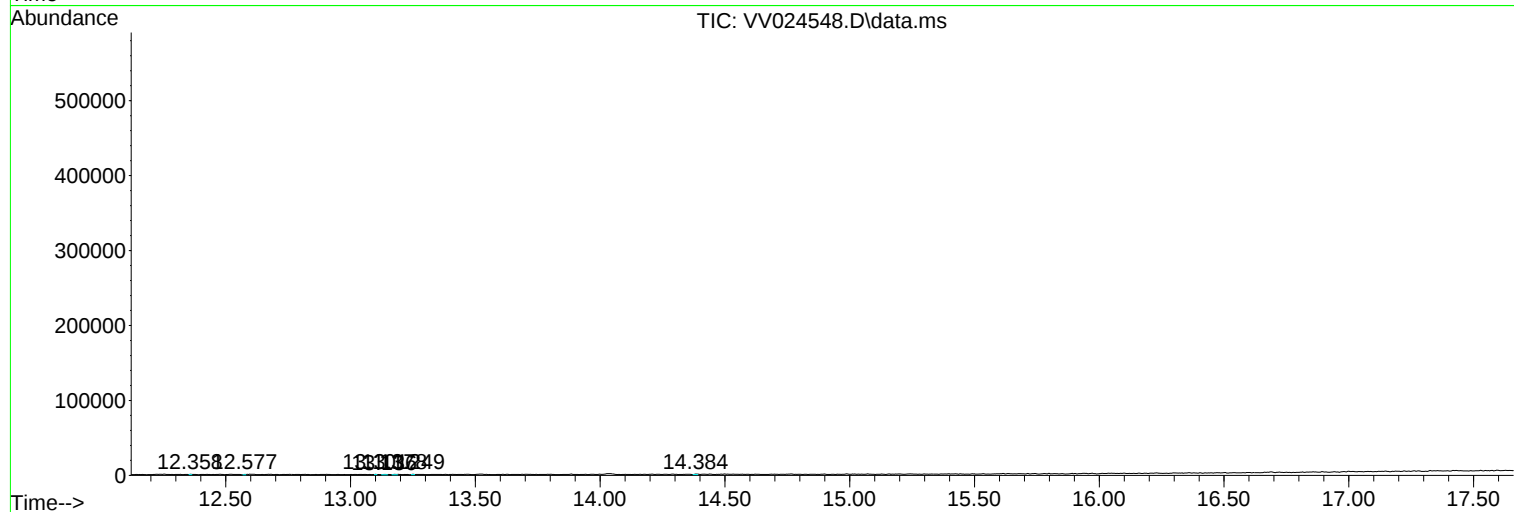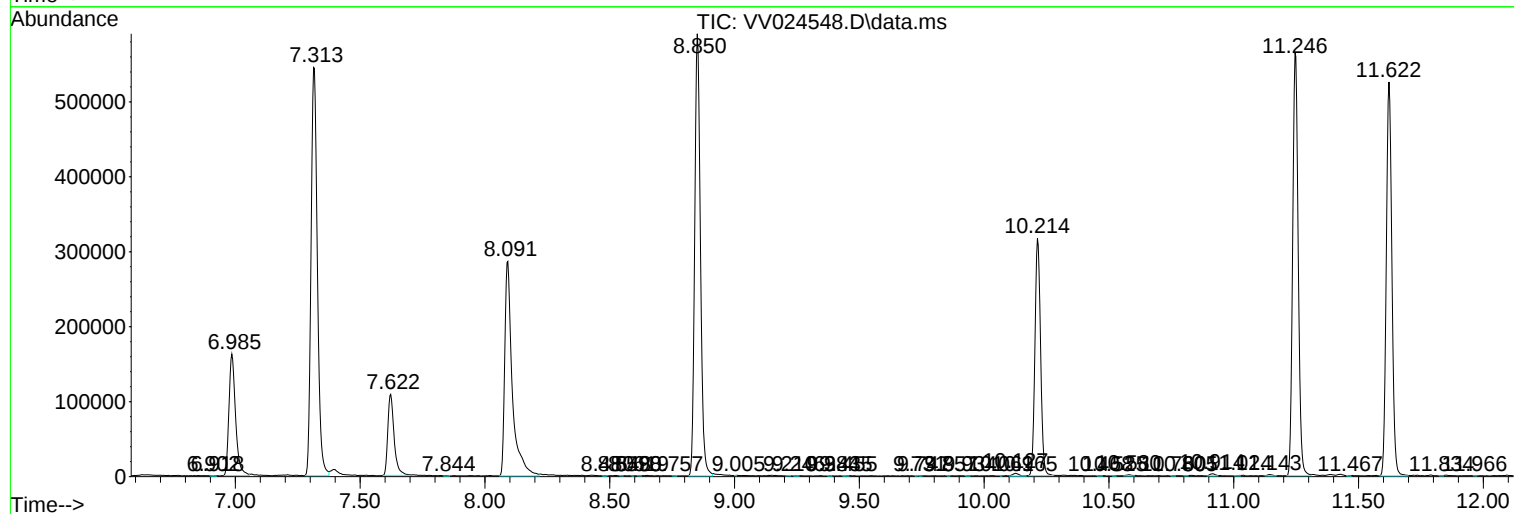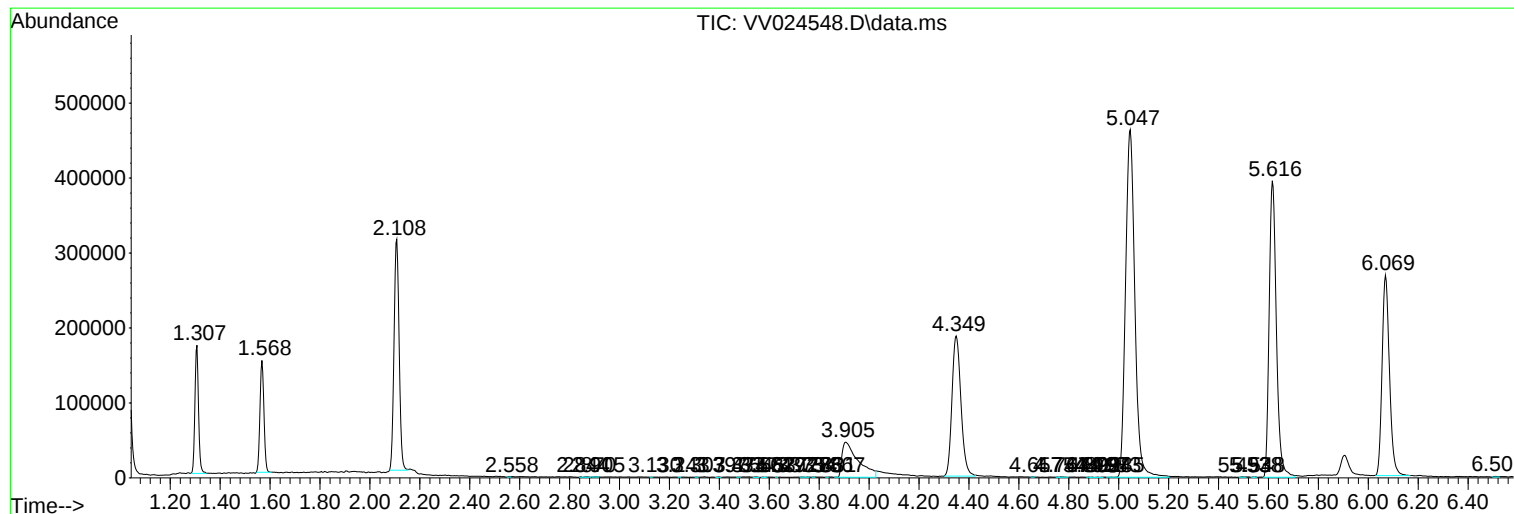

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024548.D
Acq On : 03 Feb 2022 15:17
Operator : SY/MD
Sample : N1352-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024548.D
Acq On : 03 Feb 2022 15:17
Operator : SY/MD
Sample : N1352-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc