

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
 Data File : VV024551.D
 Acq On : 03 Feb 2022 16:29
 Operator : SY/MD
 Sample : N1364-09ME 10X
 Misc : 6.13g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGM14ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Title : VOC Analysis

Signal : TIC: VV024551.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	170845	174499	14.22%	1.759%
2	1.568	157	164	175	rVB	157781	177522	14.47%	1.790%
3	2.105	322	331	346	rBV	330851	467763	38.12%	4.716%
4	2.674	506	508	511	rBV	404	193	0.02%	0.002%
5	2.725	522	524	529	rVB2	545	388	0.03%	0.004%
6	2.941	589	591	593	rBV2	341	200	0.02%	0.002%
7	3.243	681	685	688	rVB2	507	408	0.03%	0.004%
8	3.278	694	696	698	rBV3	395	102	0.01%	0.001%
9	3.368	720	724	729	rBV4	579	529	0.04%	0.005%
10	3.468	753	755	758	rBV3	318	185	0.02%	0.002%
11	3.487	759	761	762	rBV	273	102	0.01%	0.001%
12	3.690	822	824	826	rBV2	200	77	0.01%	0.001%
13	3.799	855	858	861	rBV3	476	395	0.03%	0.004%
14	3.908	881	892	932	rBV	52611	231824	18.89%	2.337%
15	4.349	1014	1029	1061	rVB	194828	483552	39.41%	4.875%
16	4.648	1119	1122	1124	rBV2	347	188	0.02%	0.002%
17	4.725	1144	1146	1148	rBV2	264	146	0.01%	0.001%
18	4.789	1163	1166	1168	rBV3	435	279	0.02%	0.003%
19	4.812	1171	1173	1178	rVB3	603	429	0.03%	0.004%
20	4.860	1178	1188	1190	rBV3	492	776	0.06%	0.008%
21	4.892	1195	1198	1203	rBV2	606	358	0.03%	0.004%
22	4.921	1203	1207	1210	rBV4	492	457	0.04%	0.005%
23	4.937	1210	1212	1214	rBV	301	180	0.01%	0.002%
24	4.976	1220	1224	1226	rBV3	256	176	0.01%	0.002%
25	5.043	1228	1245	1271	rBV2	482421	1227132	100.00%	12.372%
26	5.433	1364	1366	1372	rVB3	707	575	0.05%	0.006%
27	5.497	1383	1386	1394	rVB3	515	650	0.05%	0.007%
28	5.555	1402	1404	1405	rBV	248	98	0.01%	0.001%
29	5.616	1410	1423	1449	rBV	419568	843248	68.72%	8.502%
30	5.908	1503	1514	1534	rVB8	39173	90234	7.35%	0.910%
31	6.069	1551	1564	1594	rVB	278610	570603	46.50%	5.753%
32	6.985	1838	1849	1872	rBV	168035	308040	25.10%	3.106%
33	7.313	1940	1951	1970	rBV	572398	994777	81.07%	10.029%
34	7.622	2037	2047	2068	rBV	111086	199320	16.24%	2.010%
35	7.889	2127	2130	2133	rBV4	386	247	0.02%	0.002%
36	7.976	2145	2157	2175	rBV	109539	182953	14.91%	1.845%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020322\
 Data File : VW024551.D
 Acq On : 03 Feb 2022 16:29
 Operator : SY/MD
 Sample : N1364-09ME 10X
 Misc : 6.13g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGM14ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Title : VOC Analysis

37	8.092	2183	2193	2236	rBV	299470	636398	51.86%	6.416%
38	8.657	2365	2369	2374	rBV3	301	270	0.02%	0.003%
39	8.799	2409	2413	2416	rBV3	482	291	0.02%	0.003%
40	8.850	2417	2429	2453	rVV	623247	993242	80.94%	10.014%
41	9.233	2547	2548	2549	rBV	260	92	0.01%	0.001%
42	9.288	2562	2565	2569	rBV4	268	272	0.02%	0.003%
43	9.416	2602	2605	2609	rVB2	447	349	0.03%	0.004%
44	9.452	2614	2616	2618	rBV2	210	113	0.01%	0.001%
45	9.712	2695	2697	2700	rBV3	505	333	0.03%	0.003%
46	9.773	2711	2716	2719	rBV2	511	459	0.04%	0.005%
47	9.828	2731	2733	2736	rBV3	438	321	0.03%	0.003%
48	9.892	2750	2753	2759	rBV4	464	364	0.03%	0.004%
49	9.953	2769	2772	2773	rBV2	229	139	0.01%	0.001%
50	10.005	2786	2788	2789	rBV	439	186	0.02%	0.002%
51	10.130	2815	2827	2835	rBV6	3418	6076	0.50%	0.061%
52	10.165	2835	2838	2840	rBV3	389	216	0.02%	0.002%
53	10.214	2841	2853	2871	rBV	332854	524155	42.71%	5.285%
54	10.423	2916	2918	2919	rBV	301	92	0.01%	0.001%
55	10.452	2924	2927	2931	rVV5	569	626	0.05%	0.006%
56	10.493	2935	2940	2941	rBV3	300	247	0.02%	0.002%
57	10.558	2955	2960	2961	rBV3	610	543	0.04%	0.005%
58	10.728	3010	3013	3019	rVB2	412	343	0.03%	0.003%
59	10.815	3038	3040	3041	rBV2	376	176	0.01%	0.002%
60	10.915	3065	3071	3080	rVB7	2912	4977	0.41%	0.050%
61	10.953	3080	3083	3085	rBV2	421	234	0.02%	0.002%
62	11.034	3102	3108	3111	rBV2	831	981	0.08%	0.010%
63	11.246	3163	3174	3193	rBV	600628	929894	75.78%	9.375%
64	11.535	3262	3264	3270	rVB4	664	590	0.05%	0.006%
65	11.561	3270	3272	3274	rBV	425	248	0.02%	0.003%
66	11.622	3279	3291	3311	rBV	546955	854754	69.65%	8.618%
67	11.780	3338	3340	3345	rVB3	882	651	0.05%	0.007%
68	12.050	3422	3424	3429	rBV2	431	305	0.02%	0.003%
69	12.136	3448	3451	3453	rBV3	472	378	0.03%	0.004%
70	12.706	3626	3628	3632	rBV2	560	396	0.03%	0.004%
71	12.931	3696	3698	3699	rBV2	340	186	0.02%	0.002%
72	13.342	3824	3826	3829	rBV3	427	219	0.02%	0.002%
73	13.641	3917	3919	3924	rBV4	411	248	0.02%	0.003%
74	13.702	3935	3938	3939	rBV	502	280	0.02%	0.003%
75	14.599	4215	4217	4221	rBV3	519	376	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024551.D
Acq On : 03 Feb 2022 16:29
Operator : SY/MD
Sample : N1364-09ME 10X
Misc : 6.13g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGM14ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M

Title : VOC Analysis


Sum of corrected areas: 9918625

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024551.D
Acq On : 03 Feb 2022 16:29
Operator : SY/MD
Sample : N1364-09ME 10X
Misc : 6.13g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGM14ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

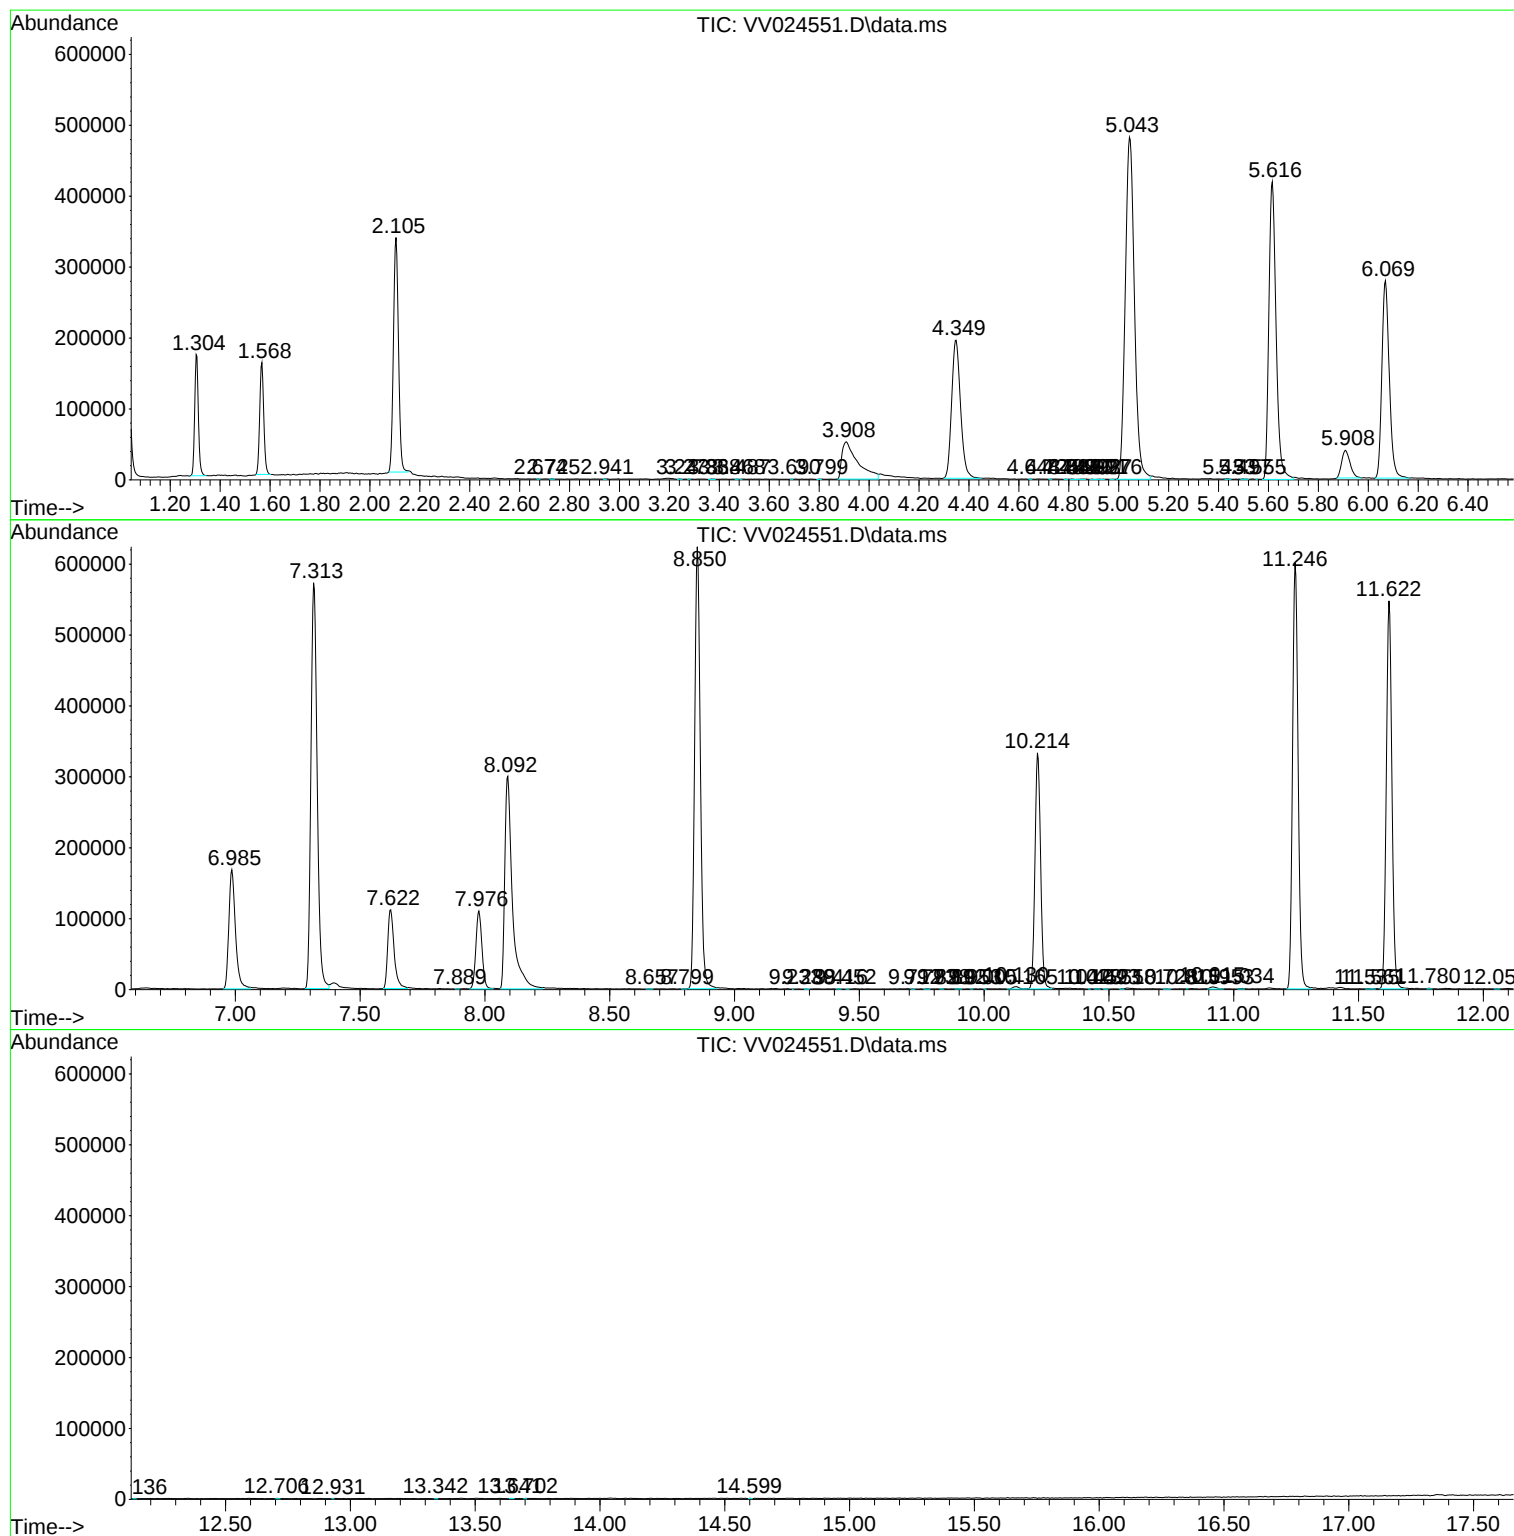

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024551.D
Acq On : 03 Feb 2022 16:29
Operator : SY/MD
Sample : N1364-09ME 10X
Misc : 6.13g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGM14ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
Data File : VV024551.D
Acq On : 03 Feb 2022 16:29
Operator : SY/MD
Sample : N1364-09ME 10X
Misc : 6.13g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGM14ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
