
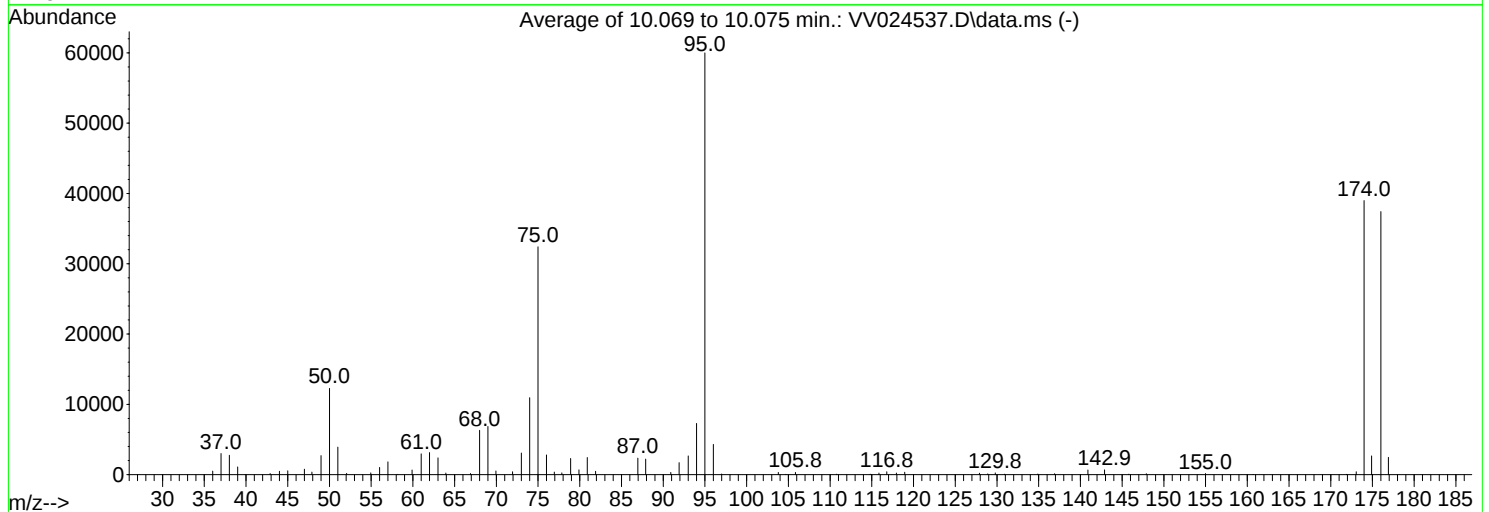


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020322\
 Data File : VV024537.D
 Acq On : 03 Feb 2022 08:58
 Operator : SY/MD
 Sample : BFB262
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB262

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM020222WMA.M
 Title : VOC Analysis
 Last Update : Sat Feb 05 00:18:38 2022

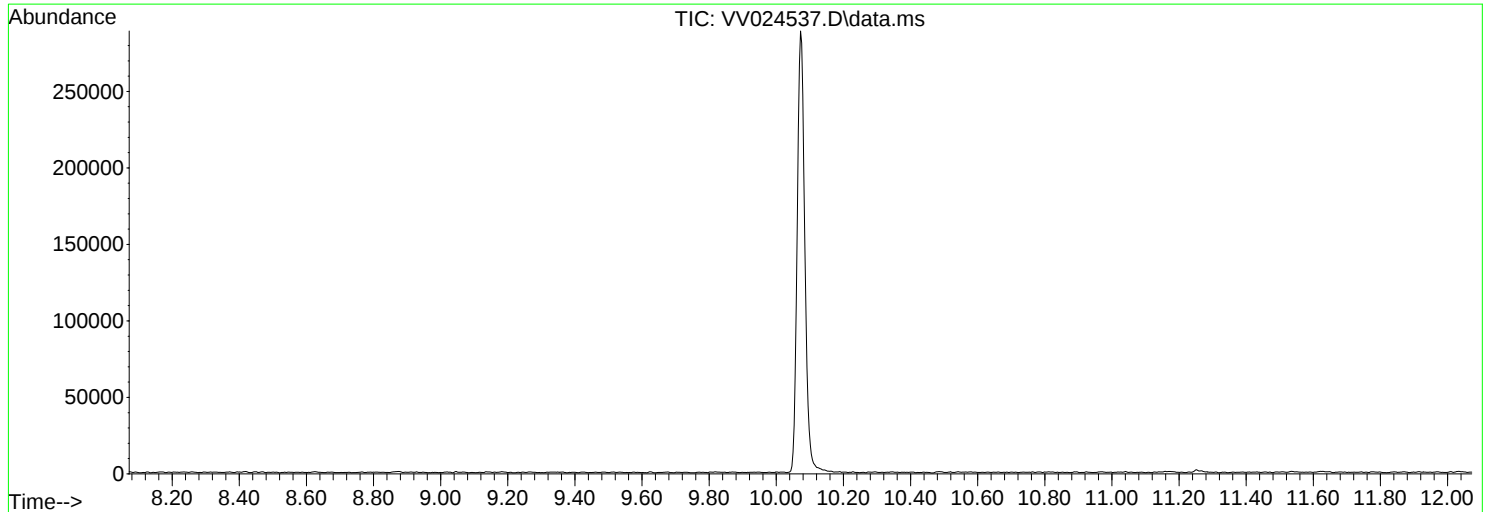

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	12277	PASS
75	95	30	80	54.0	32411	PASS
95	95	100	100	100.0	60005	PASS
96	95	5	9	7.2	4311	PASS
173	174	0.00	2	1.0	407	PASS
174	95	50	120	65.0	39000	PASS
175	174	5	9	6.9	2674	PASS
176	174	95	105	95.9	37411	PASS
177	176	5	10	6.6	2456	PASS

Scan 2797 (10.034 min): VV024537.D\data.ms
BFB262

m/z	Abundance
39.90	136.0
42.10	107.0
44.00	427.0
207.00	275.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
36.00	469.0
37.00	2885.0
38.00	2641.0
39.00	1128.0
39.90	153.0
42.90	182.0
44.00	925.0
45.00	529.0
47.00	773.0
47.90	339.0
49.00	2734.0
50.00	12124.0
51.00	3820.0
52.10	190.0
54.90	248.0
56.00	940.0
57.00	1812.0
59.90	707.0
61.00	2894.0
62.00	2964.0
63.00	2429.0
64.00	215.0
66.90	171.0
68.00	6197.0
69.00	6600.0
69.90	503.0
72.00	412.0
73.00	3025.0
74.00	10438.0
75.00	31640.0
76.00	2649.0
76.90	355.0
77.80	249.0
78.90	2316.0
79.90	687.0
80.90	2256.0
81.90	485.0
86.90	2097.0
87.90	2144.0
90.90	314.0
91.90	1565.0
93.00	2677.0
94.00	6997.0
95.00	57760.0
96.00	4207.0
103.80	317.0
105.90	270.0
115.90	227.0
116.80	414.0
117.90	225.0
119.00	316.0
127.90	177.0
128.90	113.0
129.80	258.0
130.90	100.0
136.90	121.0
140.90	564.0
142.90	585.0
145.80	107.0
147.90	137.0
155.00	154.0
173.10	387.0
174.00	36896.0
174.90	2554.0
176.00	34616.0
176.90	2294.0
206.90	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
36.00	516.0
37.00	3050.0
38.00	2857.0
39.00	1121.0
40.00	157.0
42.90	163.0
44.00	965.0
45.00	569.0
47.00	793.0
47.90	387.0
49.00	2793.0
50.00	12662.0
51.00	4108.0
52.00	195.0
55.00	283.0
56.00	1067.0
57.00	1881.0
58.20	114.0
59.90	695.0
61.00	3037.0
62.00	3246.0
63.00	2508.0
63.90	211.0
66.90	156.0
68.00	6502.0
69.00	7108.0
69.90	529.0
72.00	434.0
73.00	3199.0
74.00	11338.0
75.00	33432.0
76.00	2870.0
76.90	381.0
77.80	244.0
78.90	2358.0
79.90	701.0
80.90	2533.0
81.90	480.0
87.00	2378.0
87.90	2328.0
90.90	333.0
91.90	1742.0
93.00	2759.0
94.00	7519.0
95.00	62160.0
96.00	4499.0
97.00	130.0
103.80	335.0
105.80	325.0
110.80	110.0
114.80	104.0
115.80	244.0
116.80	410.0
118.00	248.0
118.90	359.0
127.90	209.0
128.90	122.0
129.80	267.0
130.90	110.0
134.90	143.0
136.90	138.0
140.90	669.0
142.90	742.0
145.80	113.0
147.90	147.0
155.00	175.0
160.70	104.0
173.10	422.0
174.00	40328.0
174.90	2719.0
176.00	38728.0
176.90	2567.0
206.90	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
36.00	502.0
37.00	3046.0
38.00	2756.0
39.00	1052.0
40.00	156.0
42.90	142.0
44.00	826.0
45.00	536.0
47.00	780.0
47.90	402.0
49.00	2602.0
50.00	12044.0
51.00	3852.0
52.00	196.0
55.00	258.0
56.00	1040.0
57.00	1799.0
59.90	587.0
61.00	2924.0
62.00	3185.0
63.00	2264.0
63.90	227.0
66.90	130.0
68.00	6194.0
69.00	6864.0
70.00	529.0
71.90	417.0
73.00	2977.0
74.00	11104.0
75.00	32160.0
76.00	2883.0
77.00	380.0
77.90	229.0
78.90	2243.0
79.90	662.0
80.90	2502.0
81.90	461.0
87.00	2572.0
87.90	2139.0
90.90	301.0
91.90	1827.0
93.00	2583.0
94.00	7321.0
95.00	60096.0
96.00	4228.0
97.00	138.0
103.80	309.0
104.70	120.0
105.80	374.0
110.80	102.0
114.80	108.0
115.80	228.0
116.80	385.0
118.00	239.0
118.90	345.0
127.90	225.0
128.90	129.0
129.80	243.0
134.90	164.0
136.90	147.0
140.90	722.0
142.90	742.0
147.90	132.0
155.00	164.0
171.90	129.0
173.00	411.0
174.00	39776.0
174.90	2748.0
176.00	38888.0
176.90	2507.0
207.00	190.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262