

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
 Data File : VV038590.D
 Acq On : 03 Feb 2025 16:54
 Operator : SY/MD
 Sample : Q1226-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Feb 04 07:34:00 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5686	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	6201	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2824	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2292	0.400	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	80.000%
4) 1,2-Dichloroethane-d4	4.969	65	2011	0.439	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	88.000%
7) 1,2-Dichloropropane-d6	5.995	67	2431	0.399	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	80.000%
8) Toluene-d8	7.254	98	4553	0.373	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	74.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2239	0.431	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	86.000%
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.280	62	427	0.058	ug/L #	1
6) Trichloroethene	5.828	95	58038	11.331	ug/L	94
9) 1,2-Dibromoethane	8.321	107	19	0.005	ug/L #	70
12) 1,2,3-Trichloropropane	10.197	75	6	0.002	ug/L #	1
13) 1,2-Dibromo-3-chloropr...	12.374	75	13	0.026	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
Data File : VV038590.D
Acq On : 03 Feb 2025 16:54
Operator : SY/MD
Sample : Q1226-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Feb 04 07:34:00 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration




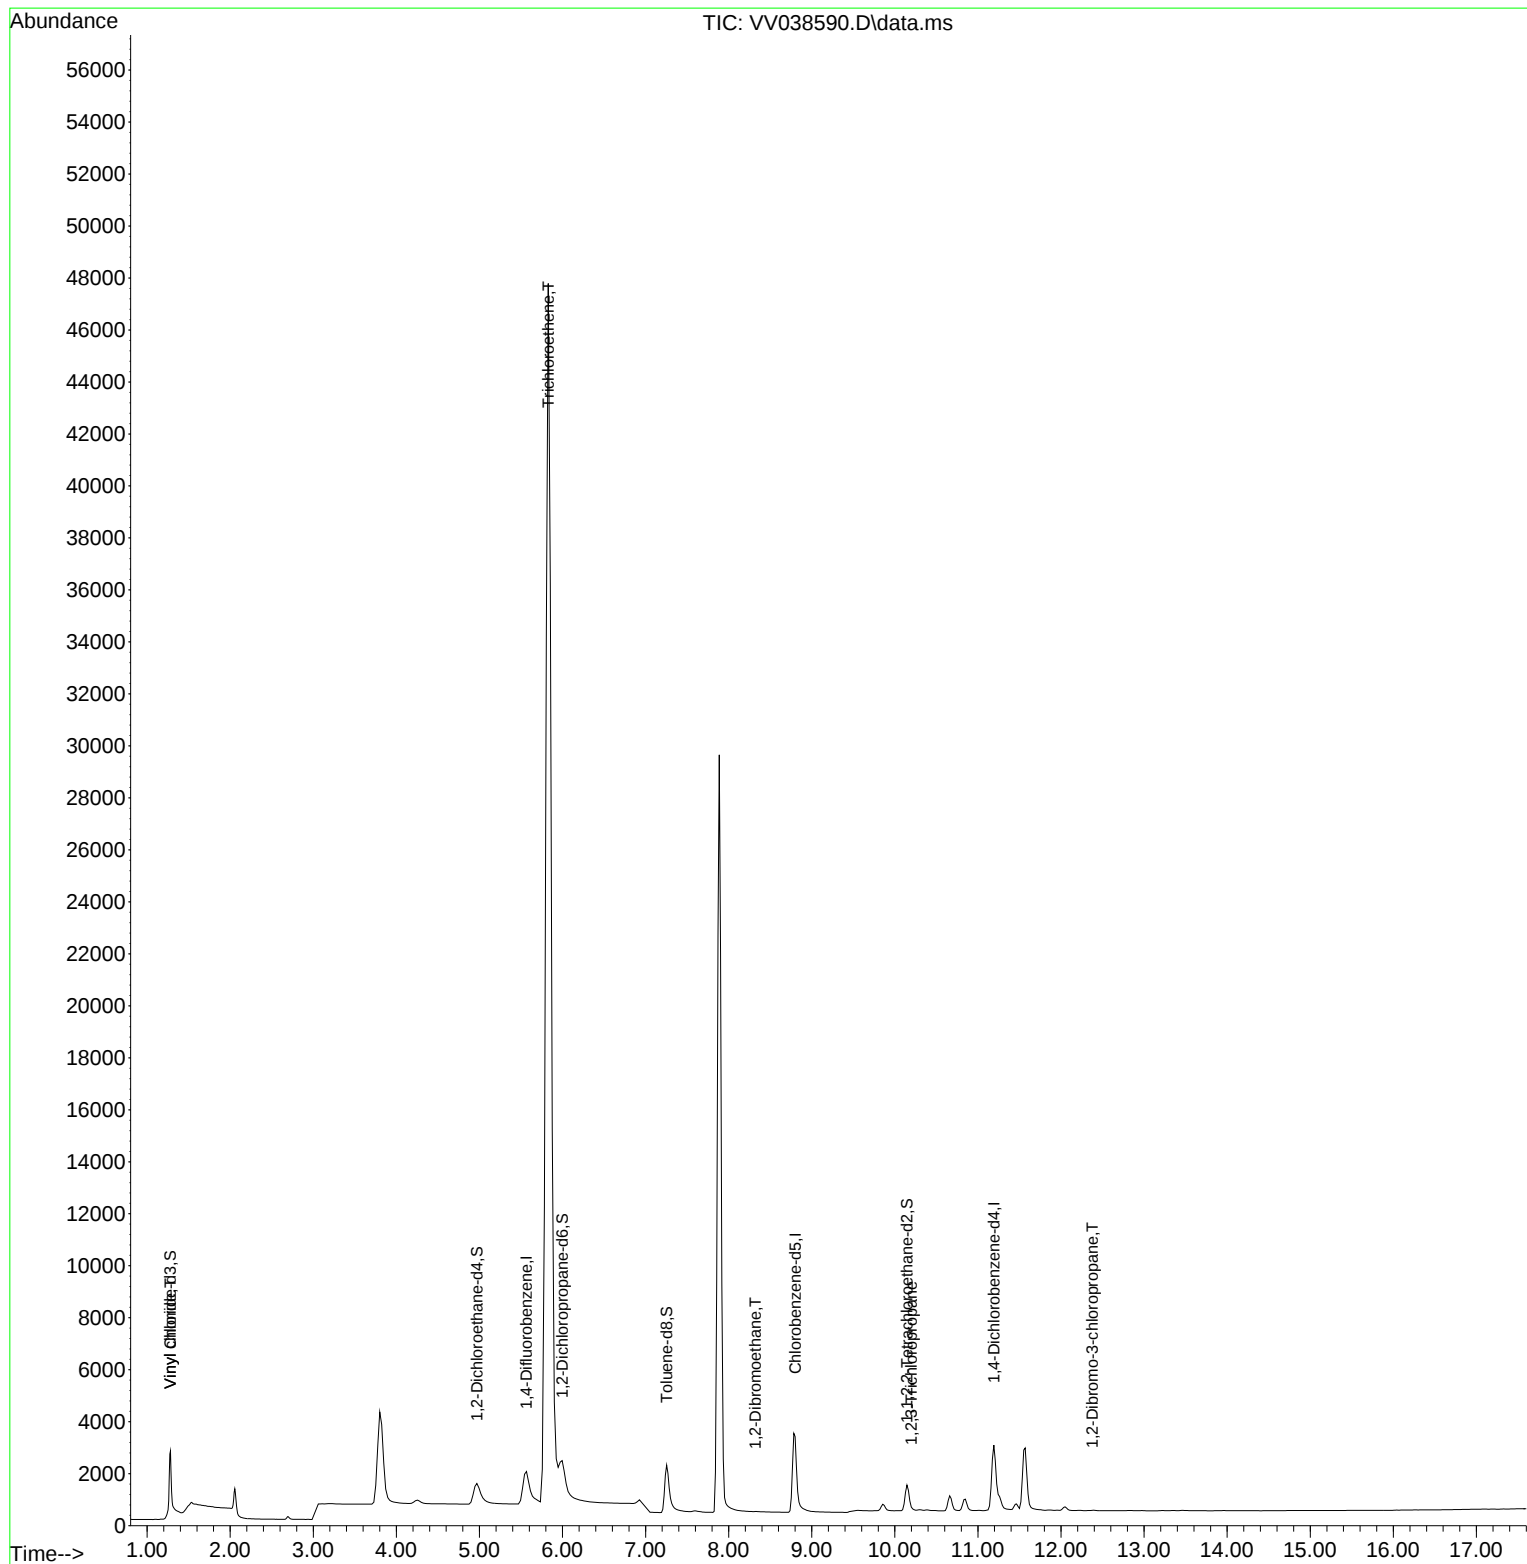


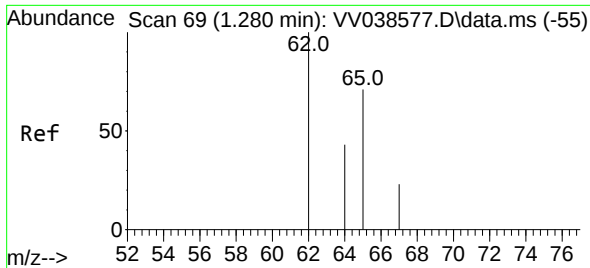

#3
 Vinyl chloride
 Concen: 0.058 ug/L
 RT: 1.280 min Scan# 69
 Delta R.T. 0.000 min
 Lab File: VV038590.D
 Acq: 03 Feb 2025 16:54




Instrument :
 MSVOA_V
 ClientSampleId :


Tgt Ion: 62 Resp: 427
 Ion Ratio Lower Upper
 62 100
 64 197.7 24.4 45.2#

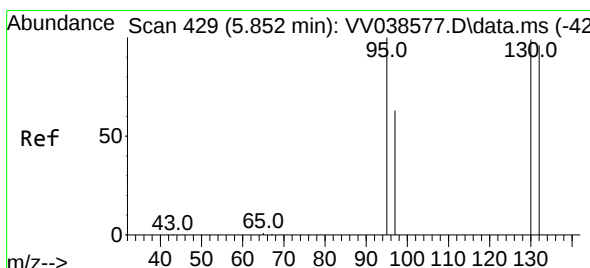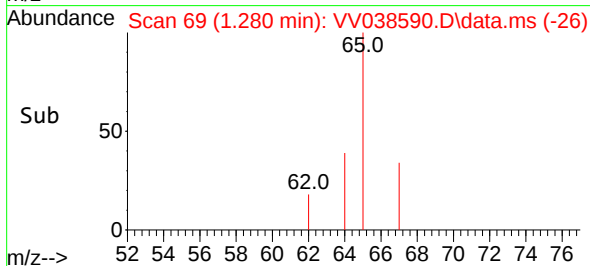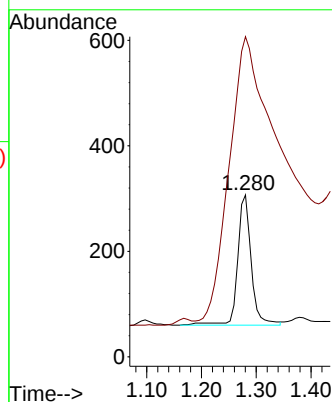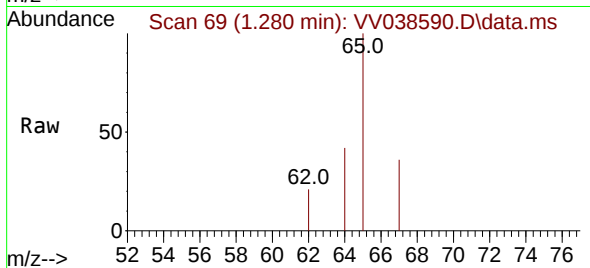

#6
 Trichloroethene
 Concen: 11.331 ug/L
 RT: 5.828 min Scan# 428
 Delta R.T. -0.024 min
 Lab File: VV038590.D
 Acq: 03 Feb 2025 16:54


Tgt Ion: 95 Resp: 58038
 Ion Ratio Lower Upper
 95 100
 97 65.8 47.9 88.9
 132 104.9 68.2 126.6
 130 107.1 69.7 129.5

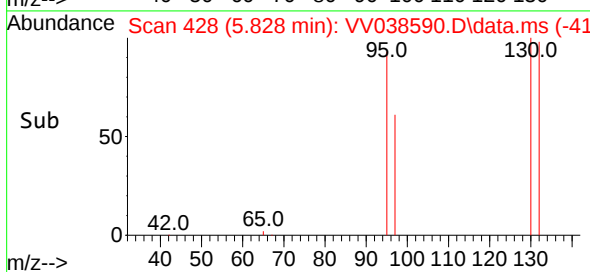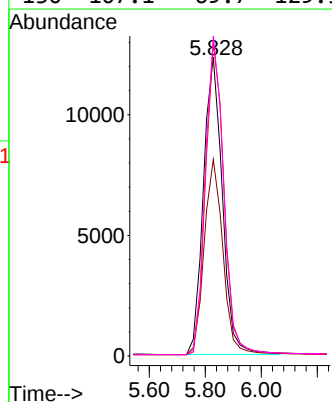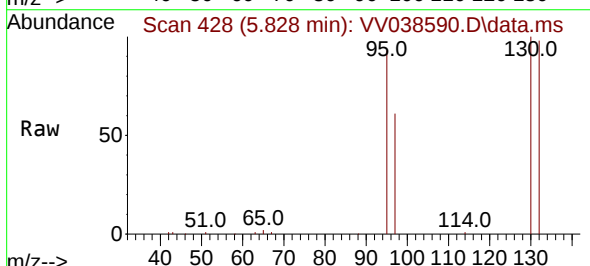



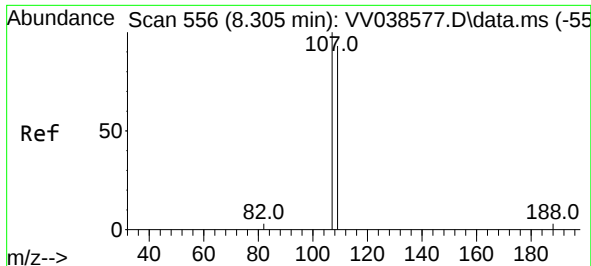


#9
1,2-Dibromoethane
Concen: 0.005 ug/L
RT: 8.321 min Scan# 557
Delta R.T. 0.016 min
Lab File: VV038590.D
Acq: 03 Feb 2025 16:54

Instrument :
MSVOA_V
ClientSampleId :



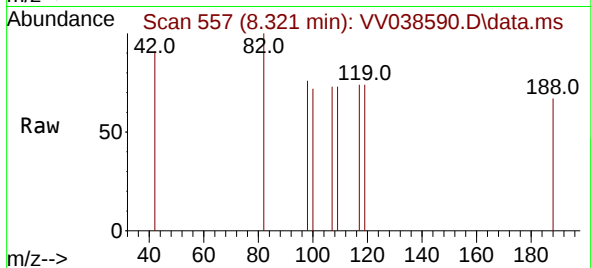



Tgt Ion:107 Resp: 19
Ion Ratio Lower Upper
107 100
109 100.0 66.3 123.1
188 91.2 11.9 17.9#

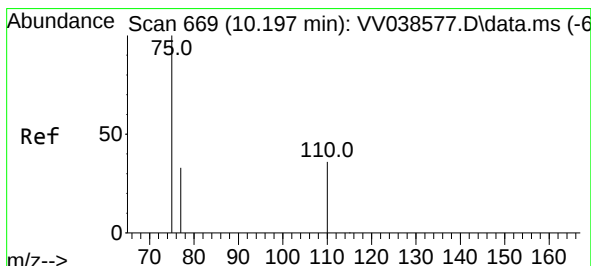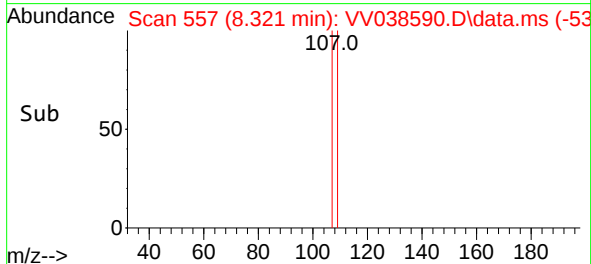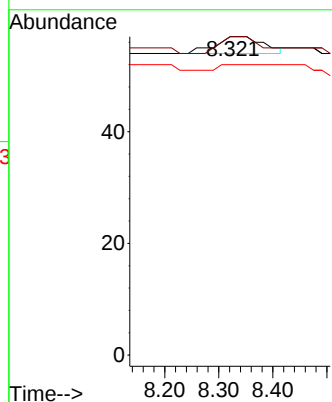

#12
1,2,3-Trichloropropane
Concen: 0.002 ug/L
RT: 10.197 min Scan# 669
Delta R.T. 0.000 min
Lab File: VV038590.D
Acq: 03 Feb 2025 16:54


Tgt Ion: 75 Resp: 6
Ion Ratio Lower Upper
75 100
110 150.0 32.7 49.1#
77 50.0 26.3 39.5#

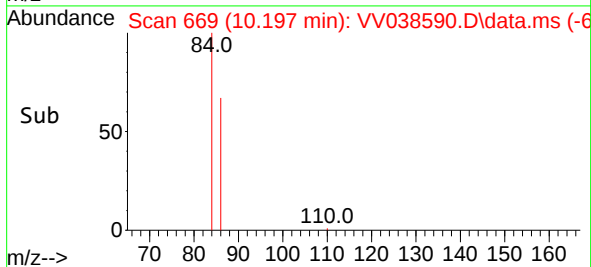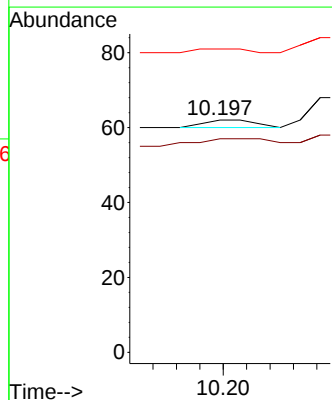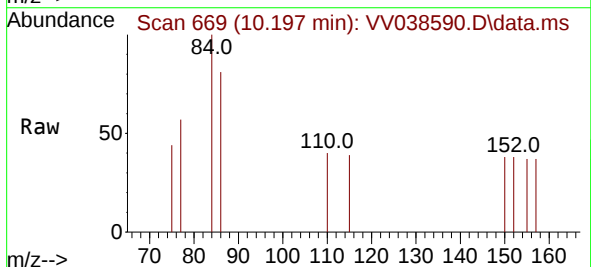

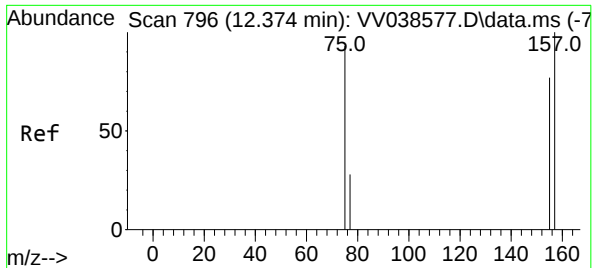

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.026 ug/L
 RT: 12.374 min Scan# 796
 Delta R.T. 0.000 min
 Lab File: VV038590.D
 Acq: 03 Feb 2025 16:54

Instrument :
 MSVOA_V
 ClientSampleId :

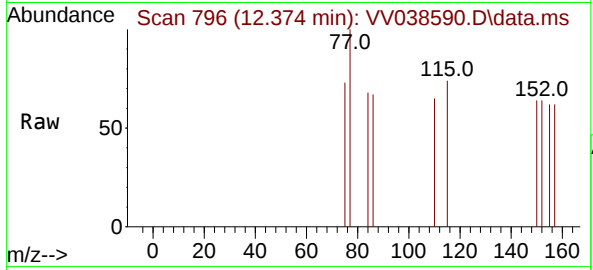

Tgt Ion: 75 Resp: 13

Ion	Ratio	Lower	Upper
75	100		
157	85.5	77.0	115.6
155	85.5	68.2	102.2

