

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
 Data File : VV038597.D
 Acq On : 03 Feb 2025 19:44
 Operator : SY/MD
 Sample : Q1226-26
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Feb 04 07:35:16 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	6849	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	6902	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	3173	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2624	0.380	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	76.000%
4) 1,2-Dichloroethane-d4	4.969	65	2338	0.424	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	84.000%
7) 1,2-Dichloropropane-d6	5.995	67	2885	0.425	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	86.000%
8) Toluene-d8	7.254	98	5453	0.401	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	80.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2539	0.439	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	88.000%
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.280	62	69	0.008	ug/L #	1
6) Trichloroethene	5.876	95	97	0.017	ug/L #	91
9) 1,2-Dibromoethane	8.336	107	34	0.008	ug/L #	72
12) 1,2,3-Trichloropropane	10.197	75	12	0.003	ug/L #	24
13) 1,2-Dibromo-3-chloropr...	12.288	75	2	0.004	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
Data File : VV038597.D
Acq On : 03 Feb 2025 19:44
Operator : SY/MD
Sample : Q1226-26
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Feb 04 07:35:16 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

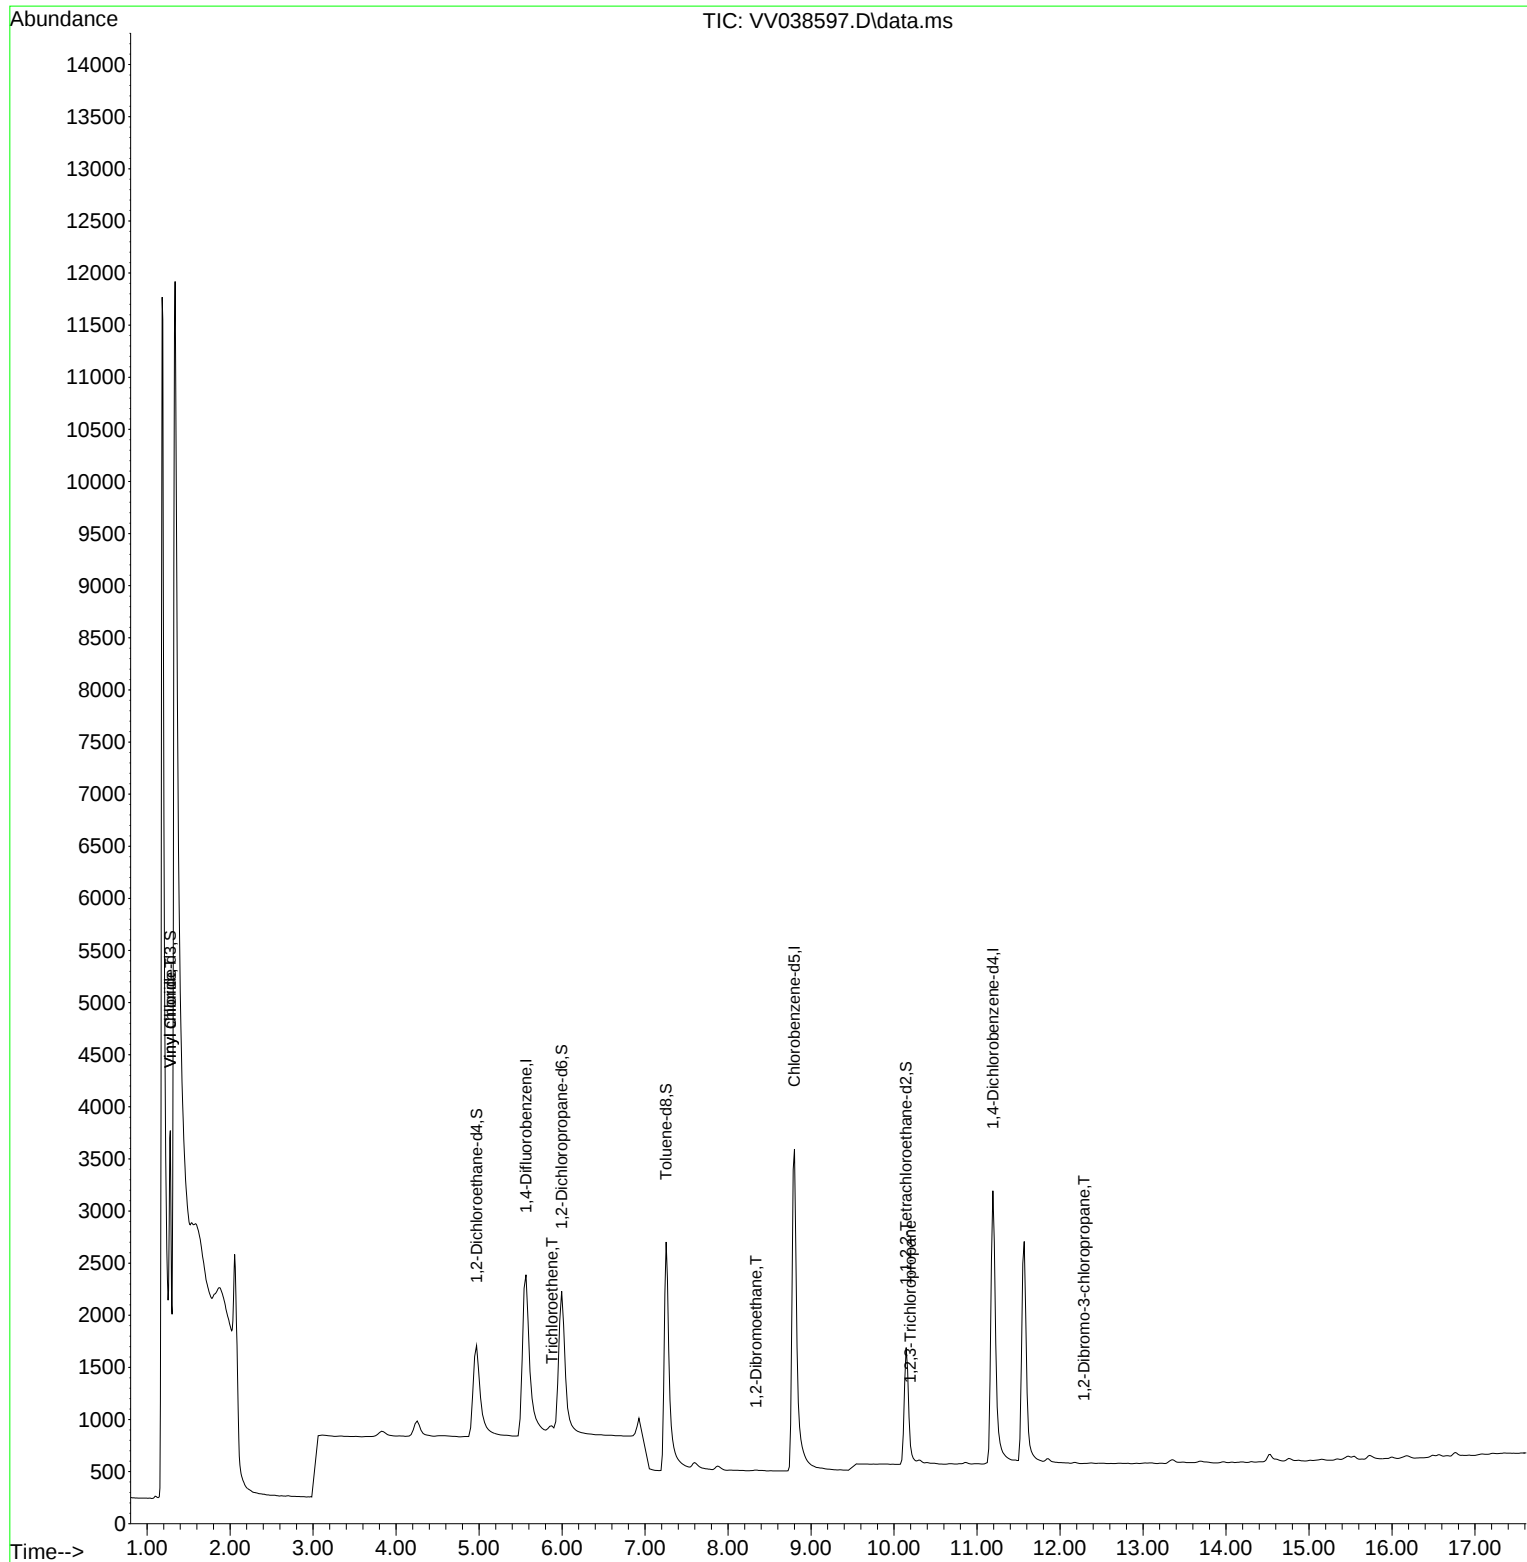

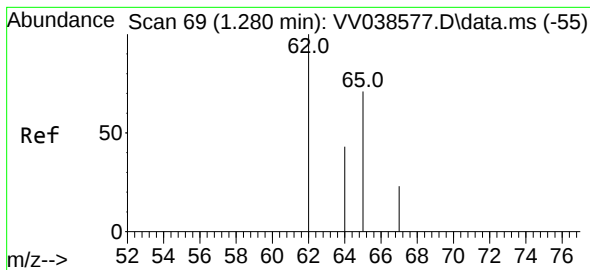

#3

Vinyl chloride

Concen: 0.008 ug/L

RT: 1.280 min Scan# 69

Delta R.T. 0.000 min

Lab File: VV038597.D

Acq: 03 Feb 2025 19:44

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 62 Resp: 69

Ion Ratio Lower Upper

62 100

64 1544.8 24.4 45.2#

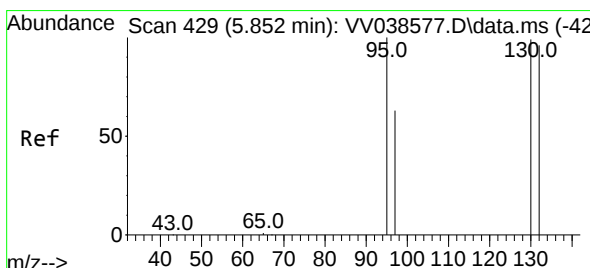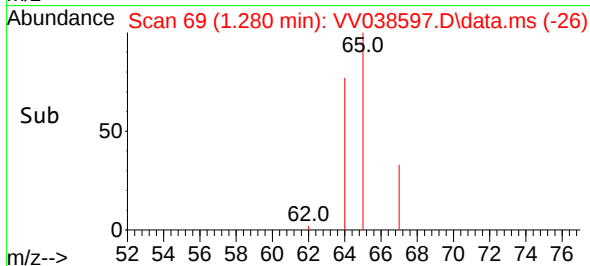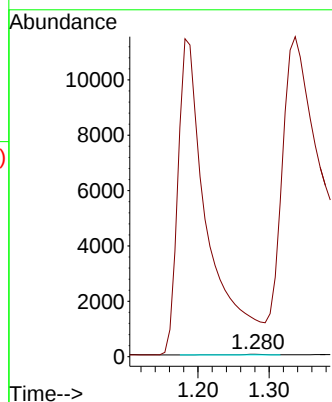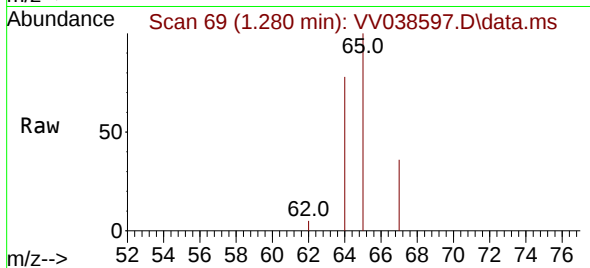

#6

Trichloroethene

Concen: 0.017 ug/L

RT: 5.876 min Scan# 430

Delta R.T. 0.024 min

Lab File: VV038597.D

Acq: 03 Feb 2025 19:44

Tgt Ion: 95 Resp: 97




Ion Ratio Lower Upper


95 100

97 90.7 47.9 88.9#

132 96.0 68.2 126.6


130 96.0 69.7 129.5

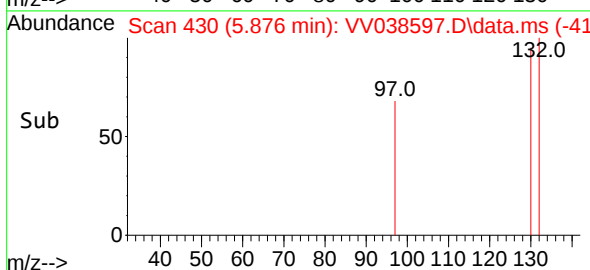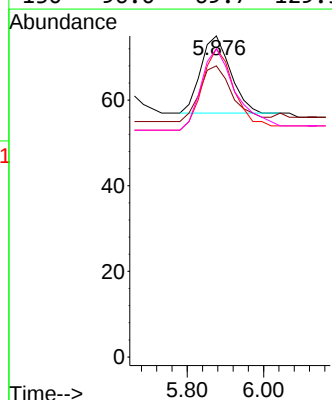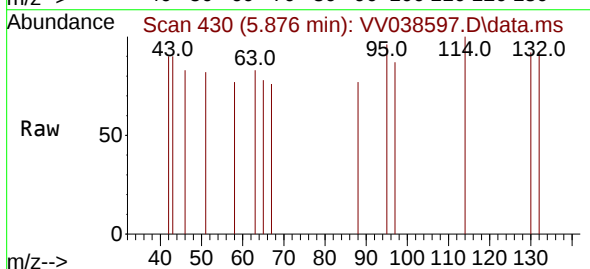



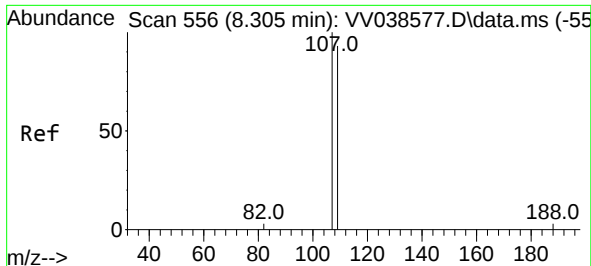


#9
1,2-Dibromoethane
Concen: 0.008 ug/L
RT: 8.336 min Scan# 51
Delta R.T. 0.031 min
Lab File: VV038597.D
Acq: 03 Feb 2025 19:44

Instrument :
MSVOA_V
ClientSampleId :



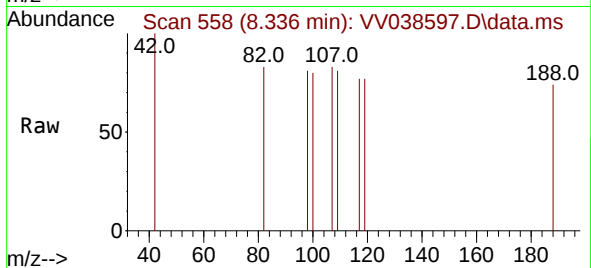



Tgt Ion:107 Resp: 34
Ion Ratio Lower Upper
107 100
109 98.3 66.3 123.1
188 89.7 11.9 17.9#

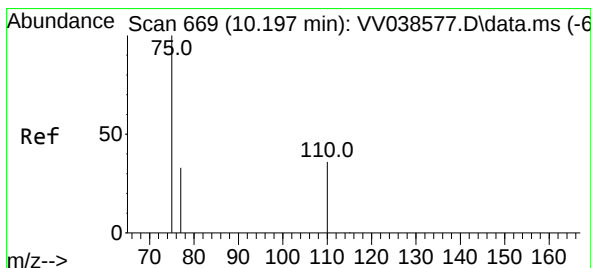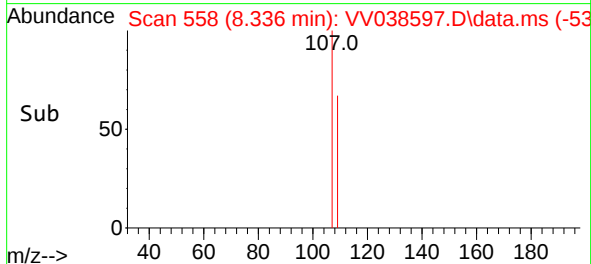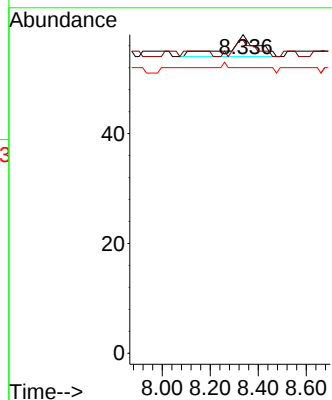

#12
1,2,3-Trichloropropane
Concen: 0.003 ug/L
RT: 10.197 min Scan# 669
Delta R.T. 0.000 min
Lab File: VV038597.D
Acq: 03 Feb 2025 19:44


Tgt Ion: 75 Resp: 12
Ion Ratio Lower Upper
75 100
110 0.0 32.7 49.1#
77 83.3 26.3 39.5#

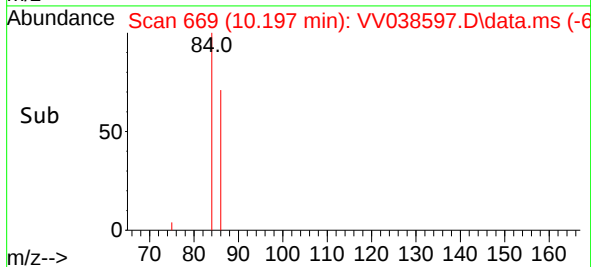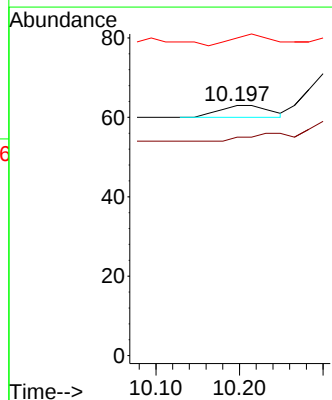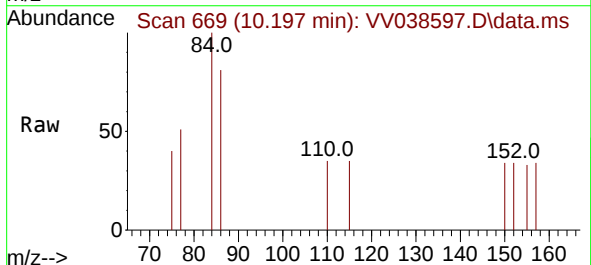

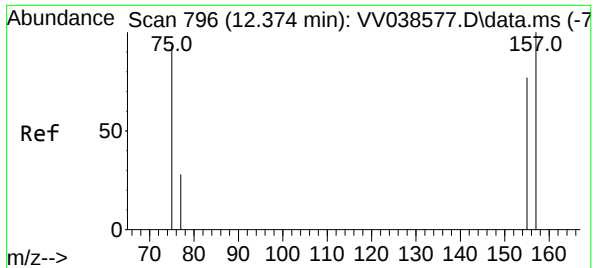

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.004 ug/L
 RT: 12.288 min Scan# 79
 Delta R.T. -0.085 min
 Lab File: VV038597.D
 Acq: 03 Feb 2025 19:44

Instrument :
 MSVOA_V
 ClientSampleId :

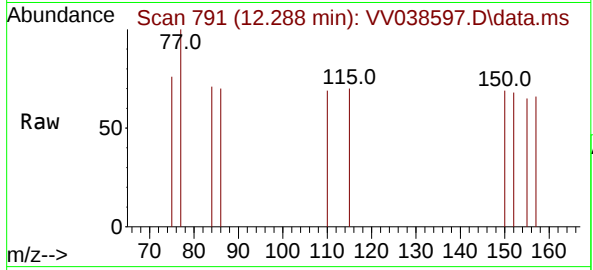

Tgt Ion: 75	Resp: 2
Ion Ratio	Lower Upper
75 100	
157 86.9	77.0 115.6
155 85.2	68.2 102.2

